

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018725.D
 Acq On : 11 Dec 2023 13:29
 Operator : MA/JU
 Sample : 05459-16
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA0

Quant Time: Dec 11 14:16:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 04 21:39:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.840	152	201498	20.000	ng/ul	-0.02
20) Naphthalene-d8	10.634	136	572191	20.000	ng/ul	-0.02
38) Acenaphthene-d10	14.469	164	466092	20.000	ng/ul	-0.02
64) Phenanthrene-d10	17.222	188	1075381	20.000	ng/ul	0.00
79) Chrysene-d12	21.310	240	1115522	20.000	ng/ul	0.00
88) Perylene-d12	23.680	264	1241278	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	7285	1.232	ng/uL	0.00
4) Pyridine-d5	3.693	84	29478	1.861	ng/ul	0.00
7) Phenol-d5	7.011	99	159590	7.892	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.175	67	125825	10.499	ng/ul	-0.02
11) 2-Chlorophenol-d4	7.369	132	136711	8.664	ng/ul	-0.02
15) 4-Methylphenol-d8	8.552	113	86634	5.294	ng/ul	-0.02
21) Nitrobenzene-d5	9.005	128	69142	13.577	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.722	143	59954	11.355	ng/ul	-0.02
28) 2,4-Dichlorophenol-d3	10.257	165	100583	9.316	ng/ul	-0.02
31) 4-Chloroaniline-d4	10.781	131	110085	7.802	ng/ul	-0.01
46) Dimethylphthalate-d6	13.887	166	469605	11.289	ng/ul	-0.02
49) Acenaphthylene-d8	14.163	160	504623	11.016	ng/ul	-0.02
54) 4-Nitrophenol-d4	14.675	143	34425	5.041	ng/ul	-0.01
60) Fluorene-d10	15.463	176	427249	12.236	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.581	200	26501	4.110	ng/ul	-0.01
73) Anthracene-d10	17.316	188	647627	11.455	ng/ul	-0.01
81) Pyrene-d10	19.557	212	856197	9.860	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.521	264	820196	11.333	ng/ul	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	8.669	105	89319	3.662	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018725.D
Acq On : 11 Dec 2023 13:29
Operator : MA/JU
Sample : 05459-16
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA0


Quant Time: Dec 11 14:16:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 04 21:39:40 2023
Response via : Initial Calibration

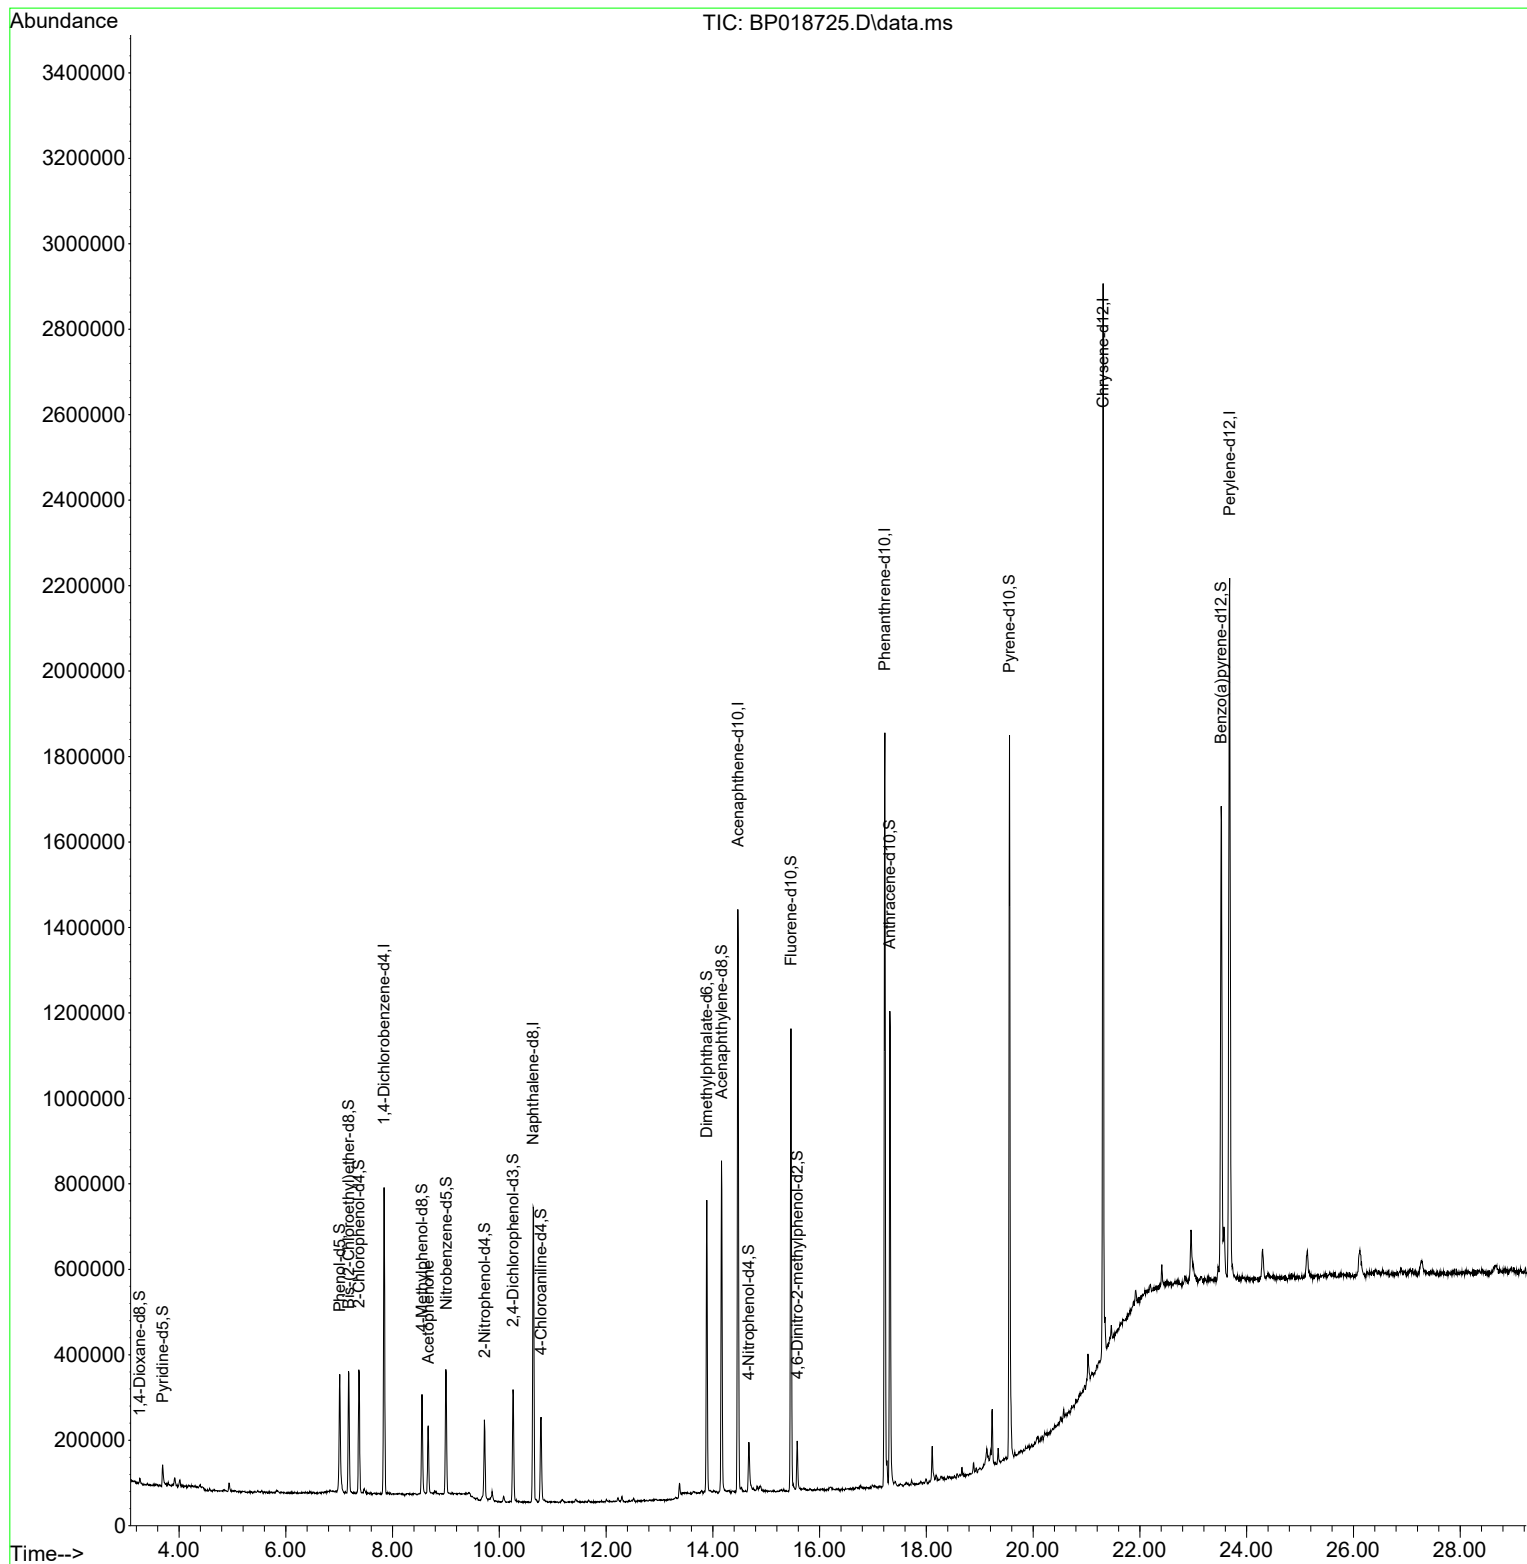

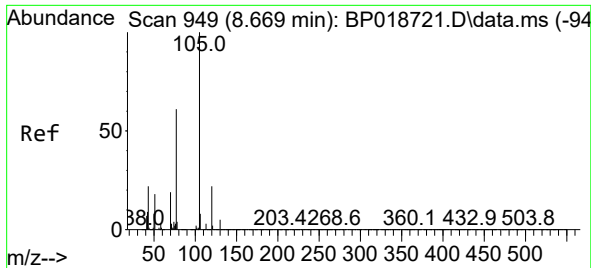

#16
 Acetophenone
 Concen: 3.662 ng/ul
 RT: 8.669 min Scan# 94
 Delta R.T. -0.012 min
 Lab File: BP018725.D
 Acq: 11 Dec 2023 13:29

Instrument :
 BNA_P
 ClientSampleId :
 C0AA0

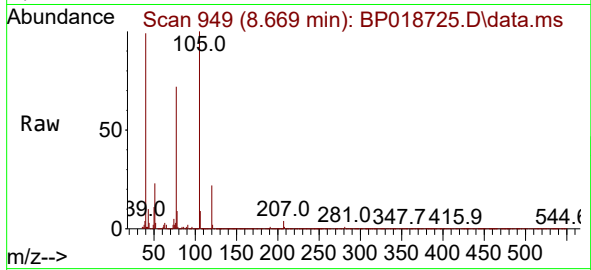

Tgt Ion:105 Resp: 89319
 Ion Ratio Lower Upper
 105 100
 77 72.3 59.4 89.0
 51 23.1 19.4 29.0

