

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018727.D
 Acq On : 11 Dec 2023 14:38
 Operator : MA/JU
 Sample : 05497-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB6

Quant Time: Dec 11 15:06:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 04 21:39:40 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.840	152	214266	20.000	ng/u1	-0.02
20) Naphthalene-d8	10.634	136	627796	20.000	ng/u1	-0.02
38) Acenaphthene-d10	14.469	164	411245	20.000	ng/u1	-0.02
64) Phenanthrene-d10	17.222	188	1117721	20.000	ng/u1	0.00
79) Chrysene-d12	21.310	240	1196295	20.000	ng/u1	0.00
88) Perylene-d12	23.674	264	1374926	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	7781	1.237	ng/uL	0.00
4) Pyridine-d5	3.693	84	21690	1.288	ng/u1	0.00
7) Phenol-d5	7.011	99	181805	8.455	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.175	67	125800	9.871	ng/u1	-0.02
11) 2-Chlorophenol-d4	7.369	132	147383	8.784	ng/u1	-0.02
15) 4-Methylphenol-d8	8.552	113	100111	5.753	ng/u1	-0.02
21) Nitrobenzene-d5	9.005	128	69888	12.508	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.722	143	70087	12.099	ng/u1	-0.02
28) 2,4-Dichlorophenol-d3	10.257	165	113233	9.559	ng/u1	-0.02
31) 4-Chloroaniline-d4	10.775	131	115024	7.430	ng/u1	-0.02
46) Dimethylphthalate-d6	13.887	166	403451	10.992	ng/u1	-0.02
49) Acenaphthylene-d8	14.163	160	438769	10.856	ng/u1	-0.02
54) 4-Nitrophenol-d4	14.675	143	35938	5.965	ng/u1	-0.01
60) Fluorene-d10	15.463	176	396825	12.880	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.581	200	32259	4.813	ng/u1	-0.01
73) Anthracene-d10	17.316	188	673167	11.456	ng/u1	-0.01
81) Pyrene-d10	19.557	212	890862	9.567	ng/u1	-0.01
92) Benzo(a)pyrene-d12	23.521	264	908646	11.334	ng/u1	-0.01
Target Compounds						
8) Phenol	7.040	94	23171	1.099	ng/u1	96
16) Acetophenone	8.669	105	122989	4.742	ng/u1	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018727.D
Acq On : 11 Dec 2023 14:38
Operator : MA/JU
Sample : 05497-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB6

Quant Time: Dec 11 15:06:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 04 21:39:40 2023
Response via : Initial Calibration




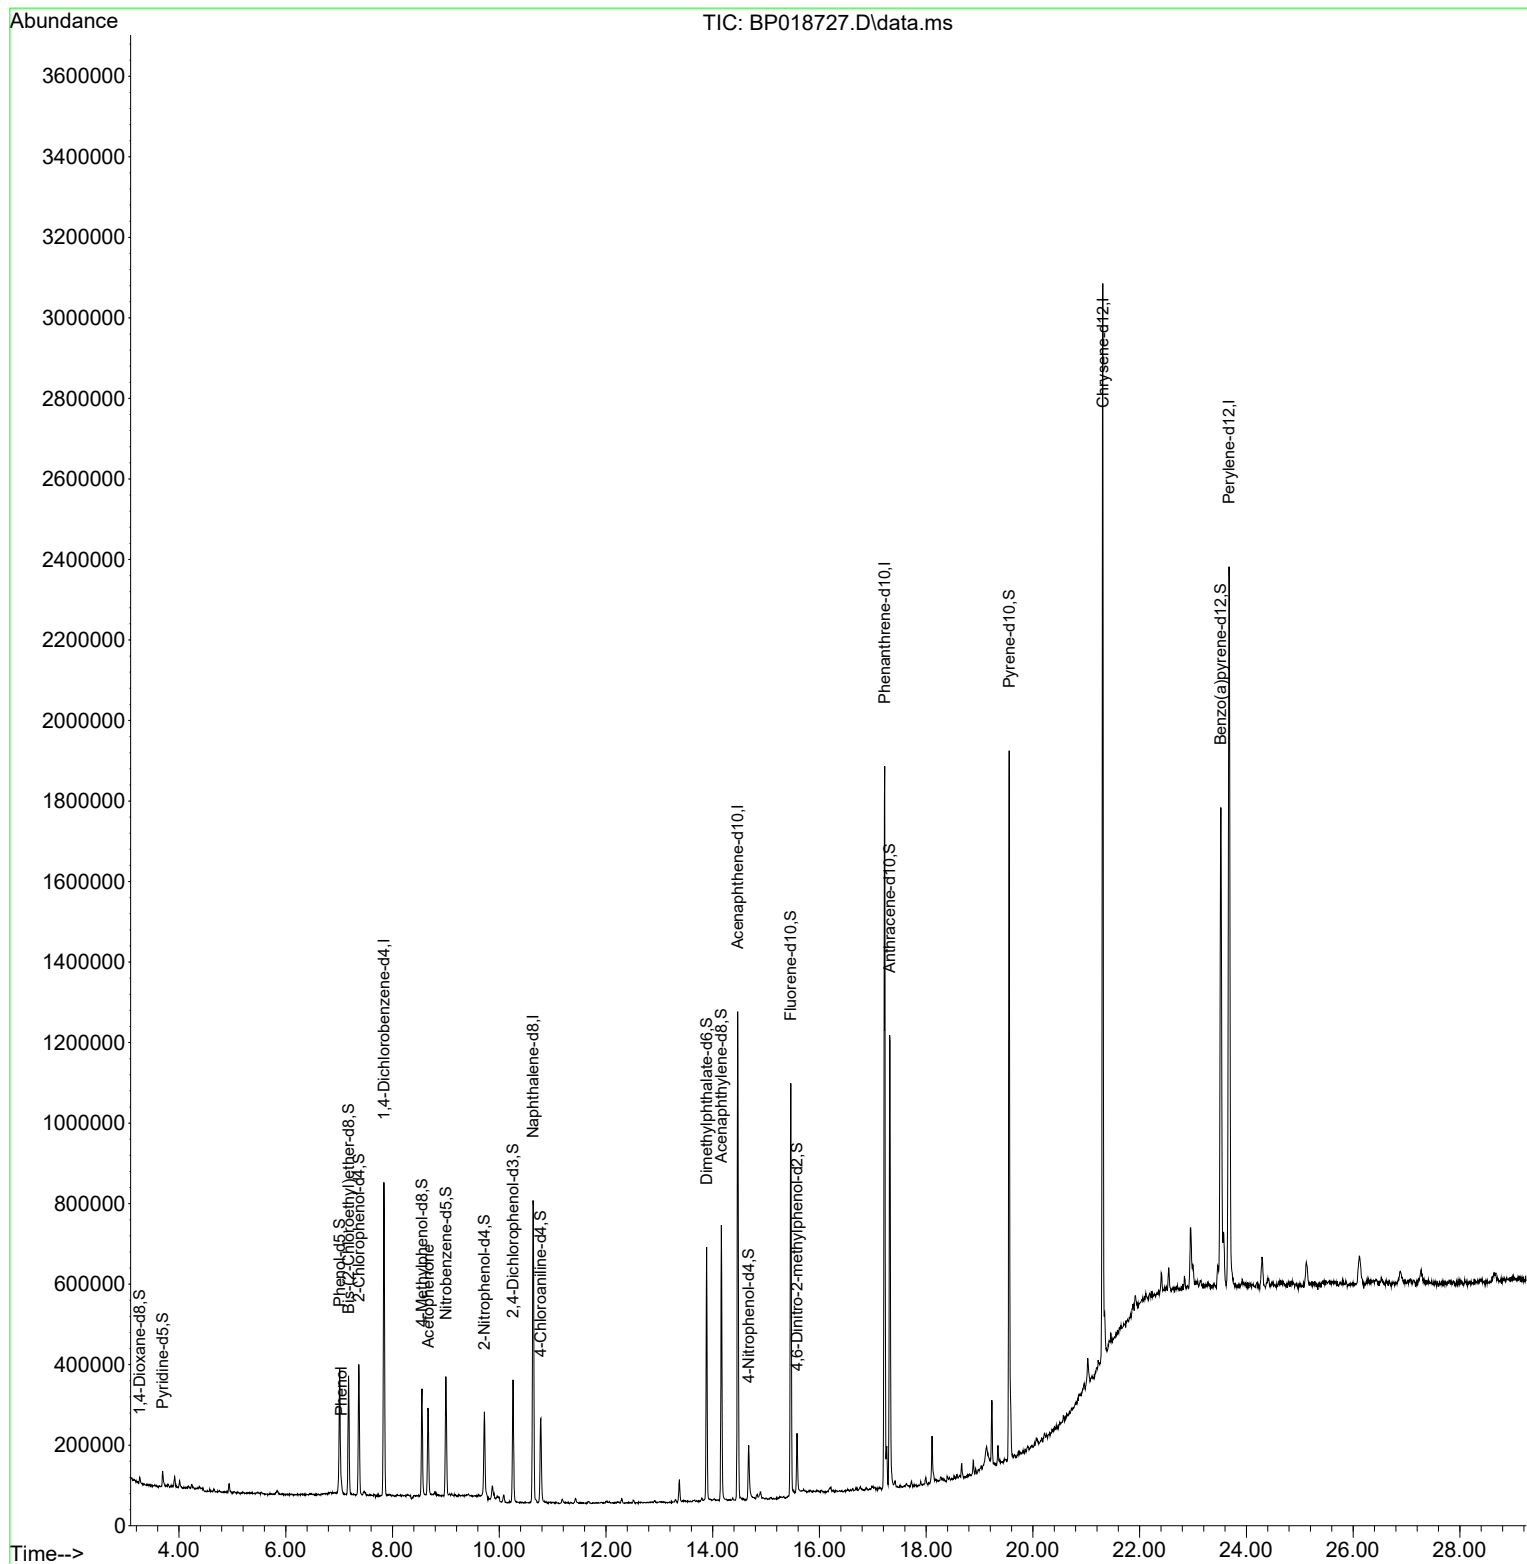


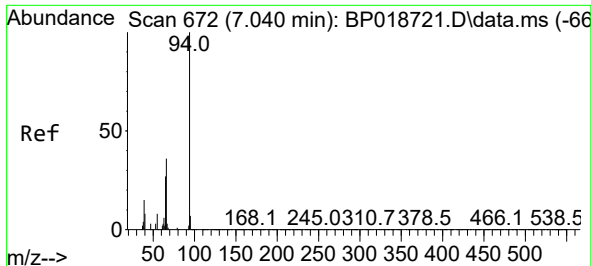

#8
Phenol
Concen: 1.099 ng/ul
RT: 7.040 min Scan# 61
Delta R.T. -0.012 min
Lab File: BP018727.D
Acq: 11 Dec 2023 14:38

Instrument :
BNA_P
ClientSampleId :
C0AB6

Tgt Ion: 94 Resp: 23171
Ion Ratio Lower Upper
94 100
65 28.2 21.0 31.6
66 38.5 28.6 43.0

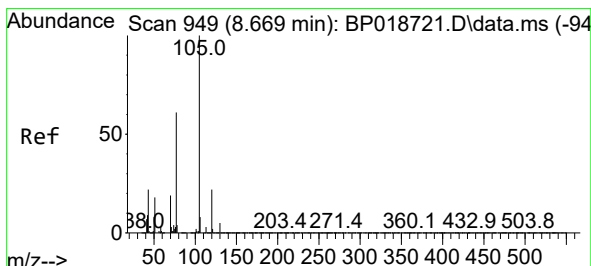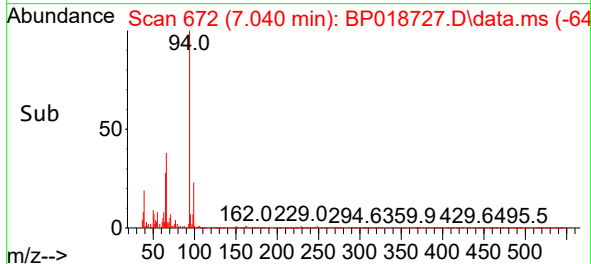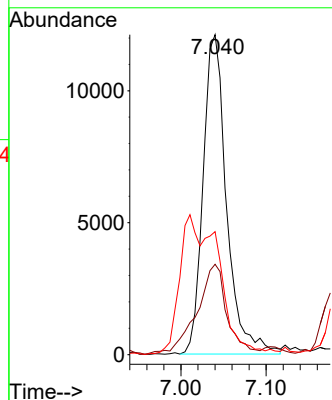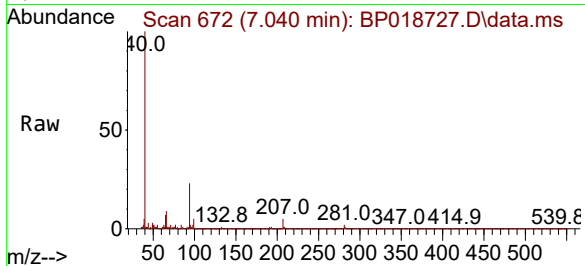

#16
Acetophenone
Concen: 4.742 ng/ul
RT: 8.669 min Scan# 949
Delta R.T. -0.012 min
Lab File: BP018727.D
Acq: 11 Dec 2023 14:38

Tgt Ion: 105 Resp: 122989
Ion Ratio Lower Upper
105 100
77 71.2 59.4 89.0
51 22.2 19.4 29.0

