

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018761.D
 Acq On : 12 Dec 2023 11:13
 Operator : MA/JU
 Sample : 05675-11
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AB2

Quant Time: Dec 12 21:56:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 11 22:02:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.840	152	164351	20.000	ng/u1	0.00
20) Naphthalene-d8	10.634	136	604928	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.469	164	397484	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.216	188	973147	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.304	240	1109130	20.000	ng/u1	# 0.00
88) Perylene-d12	23.669	264	1311313	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	18204	3.774	ng/uL	0.00
4) Pyridine-d5	3.687	84	124014	9.600	ng/u1	0.01
7) Phenol-d5	7.011	99	75681	4.589	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.175	67	246775	25.245	ng/u1	0.00
11) 2-Chlorophenol-d4	7.369	132	243167	18.895	ng/u1	0.00
15) 4-Methylphenol-d8	8.552	113	146984	11.012	ng/u1	0.00
21) Nitrobenzene-d5	8.999	128	161816	30.055	ng/u1	0.00
24) 2-Nitrophenol-d4	9.722	143	161894	29.003	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.258	165	301327	26.400	ng/u1	0.00
31) 4-Chloroaniline-d4	10.775	131	389245	26.094	ng/u1	0.00
46) Dimethylphthalate-d6	13.887	166	1134856	31.990	ng/u1	0.00
49) Acenaphthylene-d8	14.163	160	1182539	30.272	ng/u1	0.00
54) 4-Nitrophenol-d4	14.675	143	28550	4.903	ng/u1	0.00
60) Fluorene-d10	15.463	176	977796	32.836	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.581	200	168804	28.929	ng/u1	0.00
73) Anthracene-d10	17.316	188	1668963	32.622	ng/u1	0.00
81) Pyrene-d10	19.551	212	2208308	25.578	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.516	264	2489718	32.563	ng/u1	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.299	88	16169	3.057	ng/uL	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018761.D
Acq On : 12 Dec 2023 11:13
Operator : MA/JU
Sample : 05675-11
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AB2

Quant Time: Dec 12 21:56:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 11 22:02:13 2023
Response via : Initial Calibration

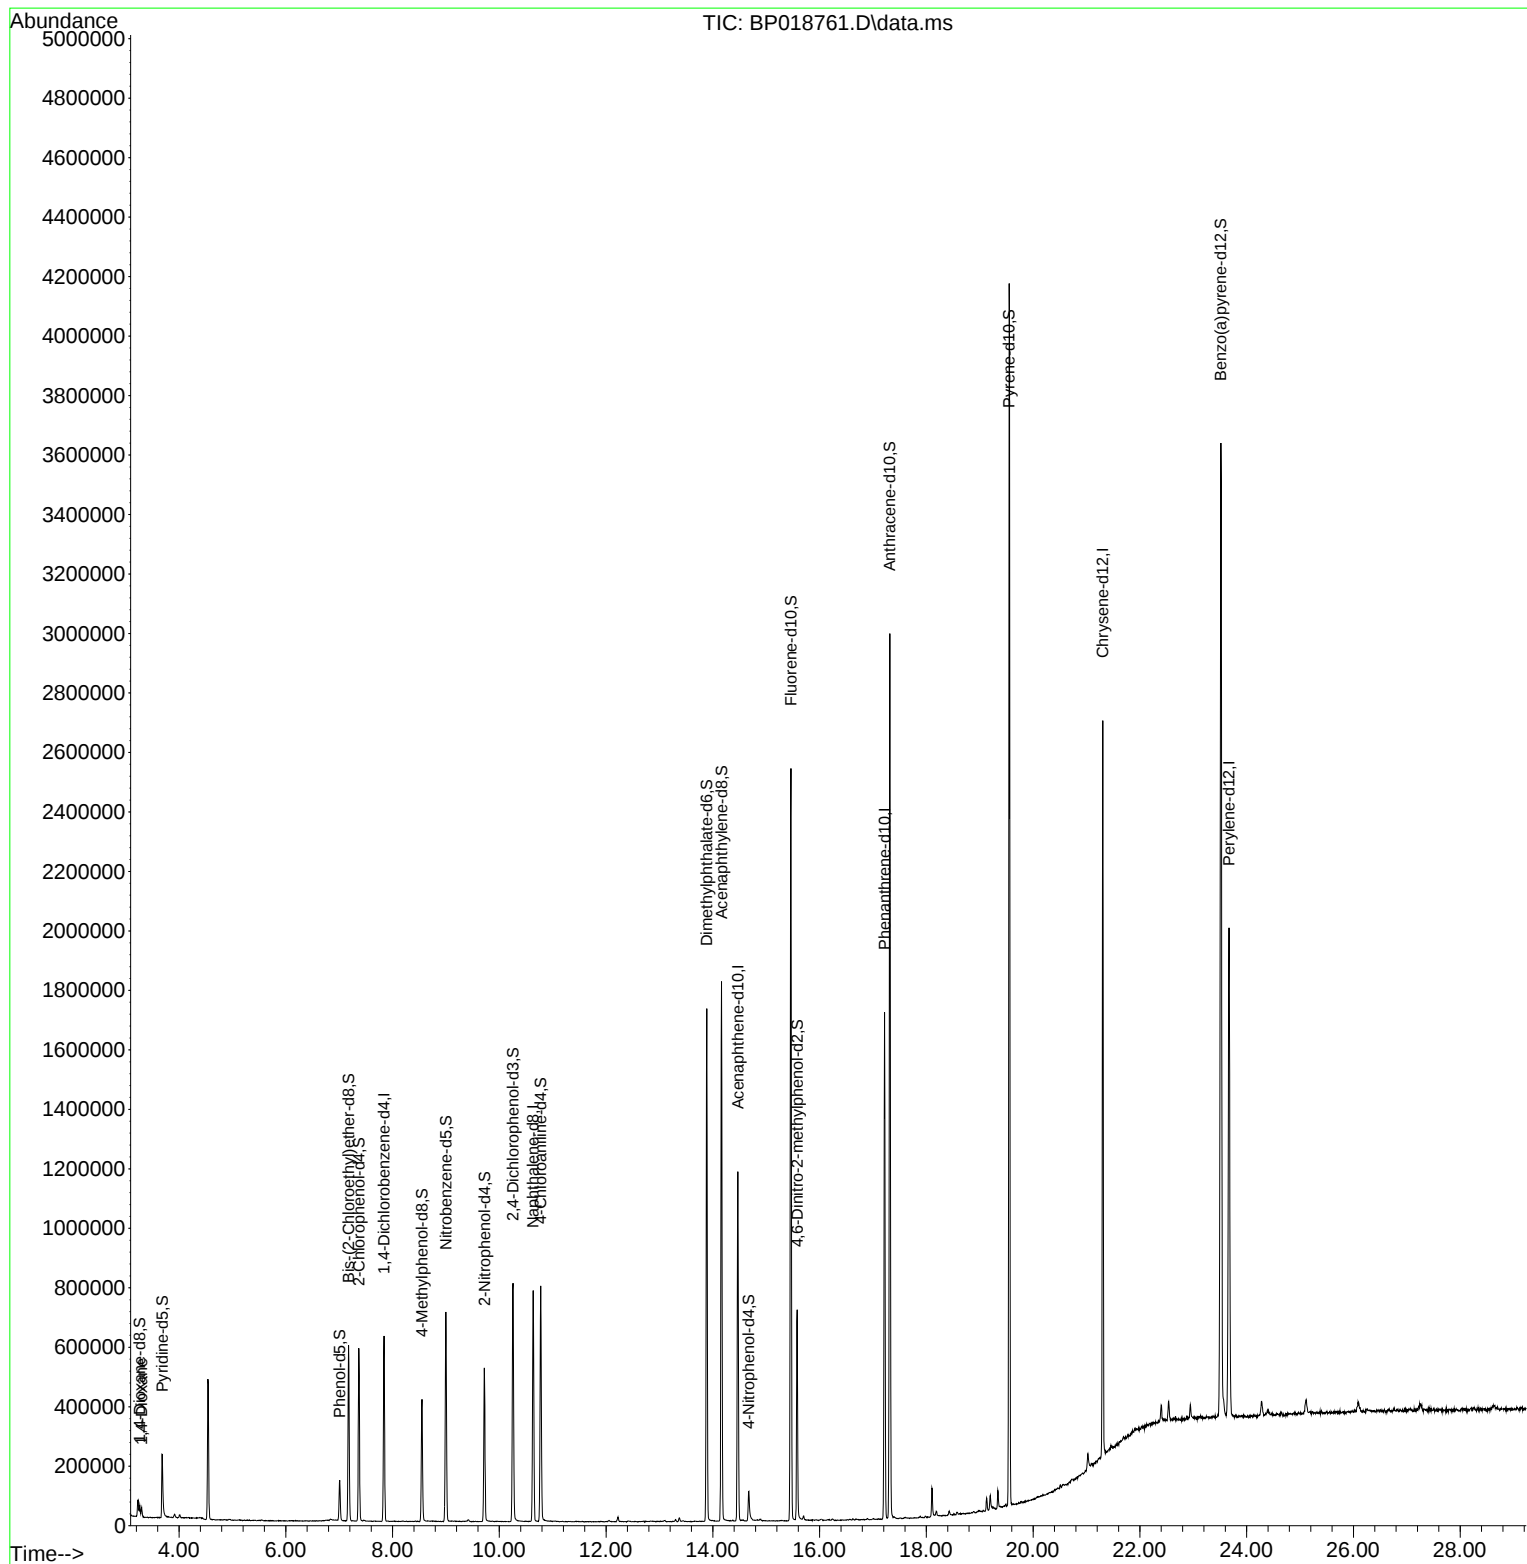

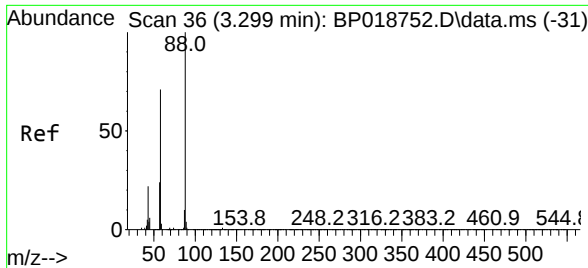

#2
 1,4-Dioxane
 Concen: 3.057 ng/uL
 RT: 3.299 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: BP018761.D
 Acq: 12 Dec 2023 11:13

Instrument :
 BNA_P
 ClientSampleId :
 H0AB2

Tgt Ion: 88 Resp: 16169
 Ion Ratio Lower Upper
 88 100
 43 25.8 21.8 32.6
 58 69.1 56.5 84.7

