

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018778.D
 Acq On : 12 Dec 2023 21:25
 Operator : MA/JU
 Sample : 05675-18
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AC1

Quant Time: Dec 12 22:40:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 11 22:02:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.840	152	187728	20.000	ng/u1	0.00
20) Naphthalene-d8	10.634	136	696277	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.469	164	451901	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.216	188	1079143	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.304	240	1234312	20.000	ng/u1	# 0.00
88) Perylene-d12	23.668	264	1467149	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	22015	3.996	ng/uL	0.00
4) Pyridine-d5	3.687	84	127133	8.616	ng/u1	0.01
7) Phenol-d5	7.010	99	95678	5.079	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.175	67	286466	25.656	ng/u1	0.00
11) 2-Chlorophenol-d4	7.369	132	292849	19.921	ng/u1	0.00
15) 4-Methylphenol-d8	8.552	113	179149	11.750	ng/u1	0.00
21) Nitrobenzene-d5	8.999	128	180610	29.144	ng/u1	0.00
24) 2-Nitrophenol-d4	9.722	143	187183	29.134	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.251	165	345185	26.275	ng/u1	0.00
31) 4-Chloroaniline-d4	10.775	131	424495	24.724	ng/u1	0.00
46) Dimethylphthalate-d6	13.887	166	1216363	30.158	ng/u1	0.00
49) Acenaphthylene-d8	14.163	160	1299120	29.252	ng/u1	0.00
54) 4-Nitrophenol-d4	14.675	143	32784	4.952	ng/u1	0.00
60) Fluorene-d10	15.457	176	1056272	31.200	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.581	200	172584	26.672	ng/u1	0.00
73) Anthracene-d10	17.310	188	1785419	31.471	ng/u1	-0.01
81) Pyrene-d10	19.551	212	2345112	24.408	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.515	264	2664844	31.151	ng/u1	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.299	88	16934	2.803	ng/uL	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018778.D
Acq On : 12 Dec 2023 21:25
Operator : MA/JU
Sample : 05675-18
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC1

Quant Time: Dec 12 22:40:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 11 22:02:13 2023
Response via : Initial Calibration

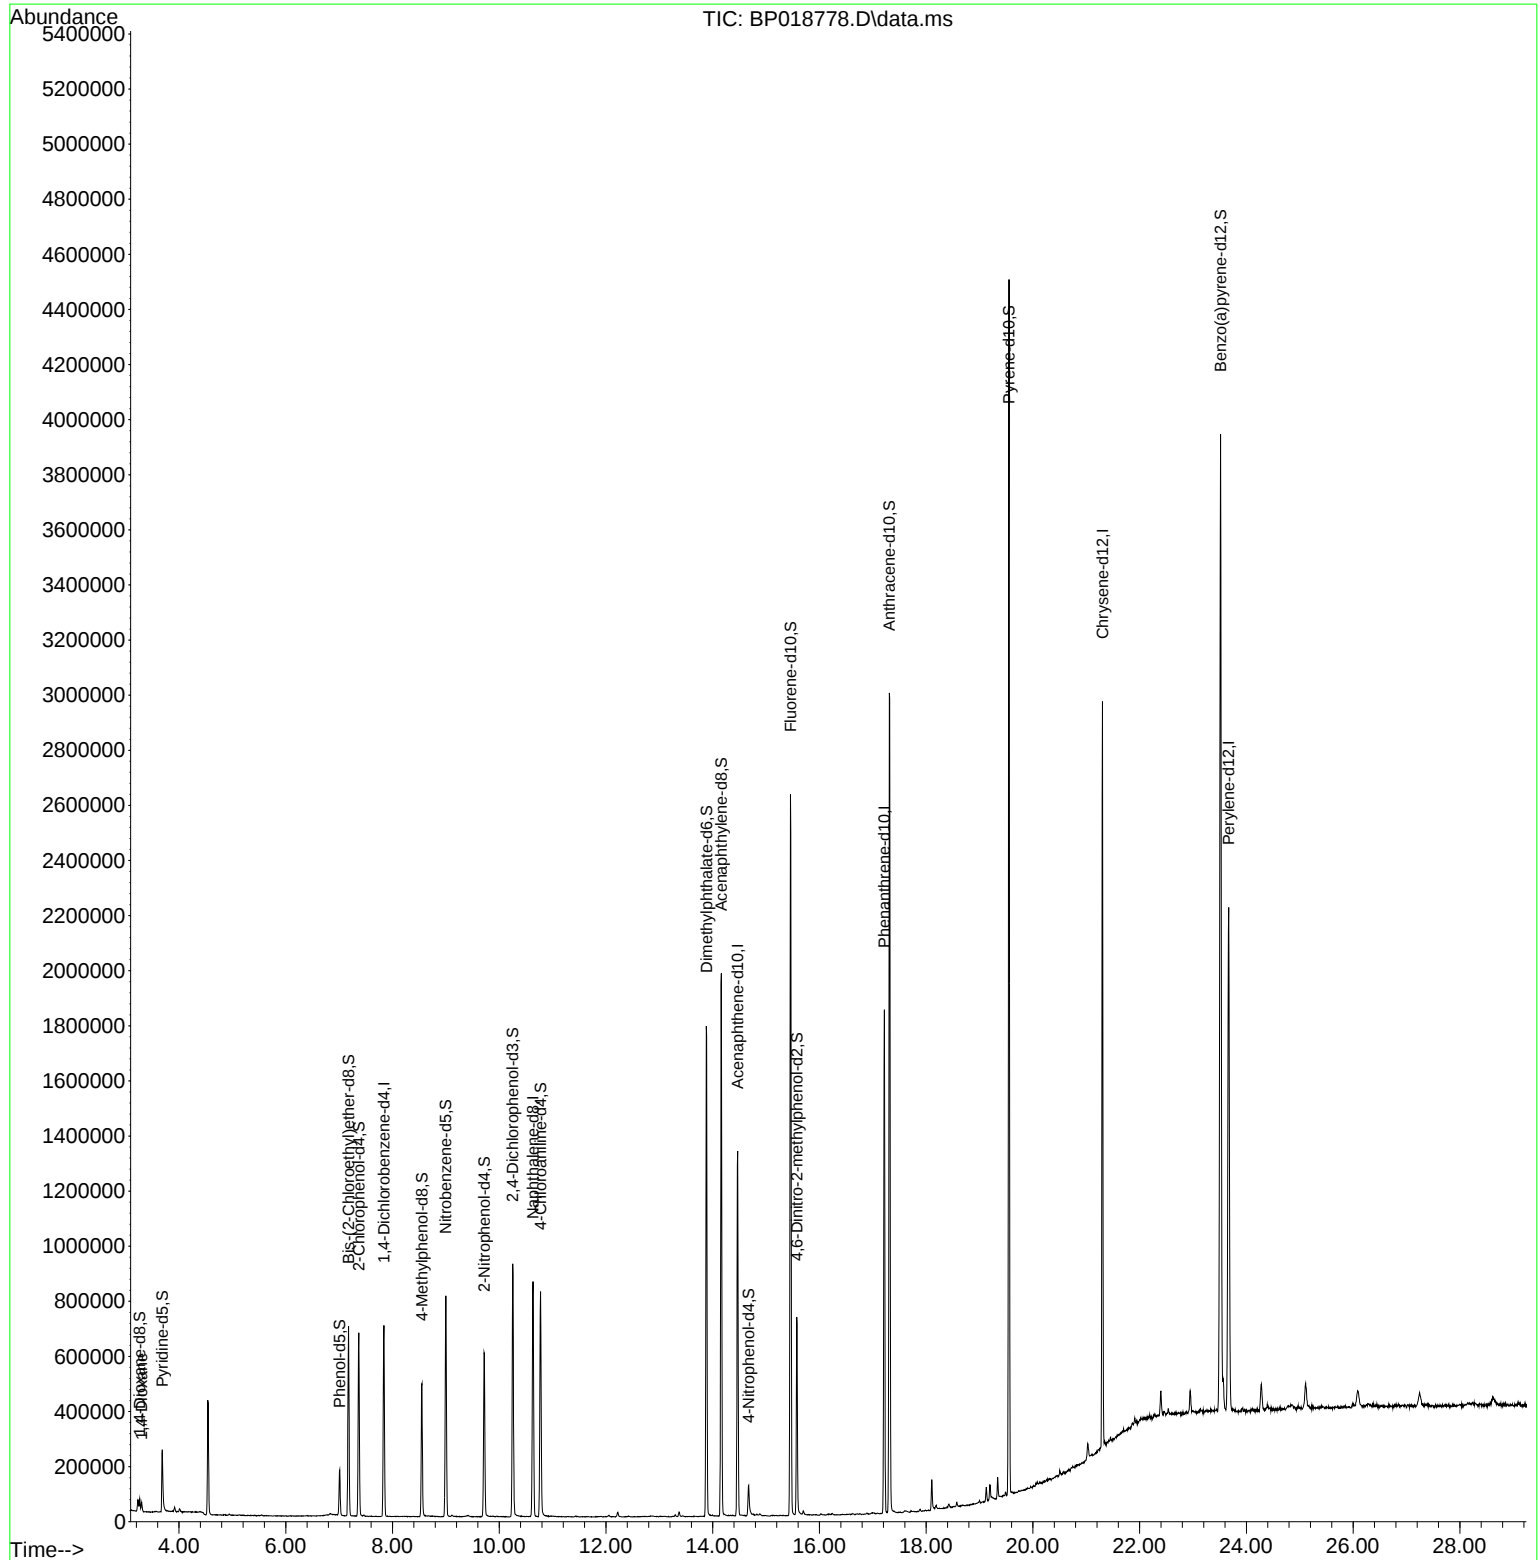

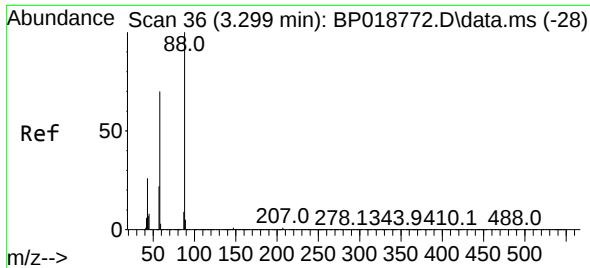

#2
 1,4-Dioxane
 Concen: 2.803 ng/uL
 RT: 3.299 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: BP018778.D
 Acq: 12 Dec 2023 21:25

Instrument :
 BNA_P
 ClientSampleId :
 H0AC1

Tgt Ion:	88	Resp:	16934
Ion	Ratio	Lower	Upper
88	100		
43	23.8	21.8	32.6
58	67.2	56.5	84.7

