

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018786.D
 Acq On : 13 Dec 2023 01:56
 Operator : MA/JU
 Sample : 05646-09
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AY5

Quant Time: Dec 13 02:26:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 11 22:02:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.840	152	171725	20.000	ng/u1	0.00
20) Naphthalene-d8	10.628	136	647205	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.463	164	422948	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.216	188	1009907	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.304	240	1161918	20.000	ng/u1	# 0.00
88) Perylene-d12	23.663	264	1387036	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	24356	4.833	ng/uL	0.00
4) Pyridine-d5	3.681	84	296467	21.964	ng/u1	0.00
7) Phenol-d5	7.011	99	413087	23.970	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.175	67	237674	23.270	ng/u1	0.00
11) 2-Chlorophenol-d4	7.369	132	328788	24.451	ng/u1	0.00
15) 4-Methylphenol-d8	8.546	113	348157	24.964	ng/u1	0.00
21) Nitrobenzene-d5	8.999	128	160598	27.880	ng/u1	0.00
24) 2-Nitrophenol-d4	9.716	143	180652	30.249	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.252	165	361812	29.628	ng/u1	0.00
31) 4-Chloroaniline-d4	10.775	131	450345	28.218	ng/u1	0.00
46) Dimethylphthalate-d6	13.881	166	1241754	32.895	ng/u1	0.00
49) Acenaphthylene-d8	14.157	160	1310848	31.536	ng/u1	0.00
54) 4-Nitrophenol-d4	14.669	143	194965	31.465	ng/u1	0.00
60) Fluorene-d10	15.457	176	1079971	34.084	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.581	200	160953	26.580	ng/u1	0.00
73) Anthracene-d10	17.316	188	1824559	34.366	ng/u1	0.00
81) Pyrene-d10	19.551	212	2361150	26.106	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.516	264	2764445	34.182	ng/u1	-0.01
Target Compounds						
12) 2-Chlorophenol	7.399	128	15703	1.154	ng/u1	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018786.D
Acq On : 13 Dec 2023 01:56
Operator : MA/JU
Sample : 05646-09
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AY5

Quant Time: Dec 13 02:26:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 11 22:02:13 2023
Response via : Initial Calibration

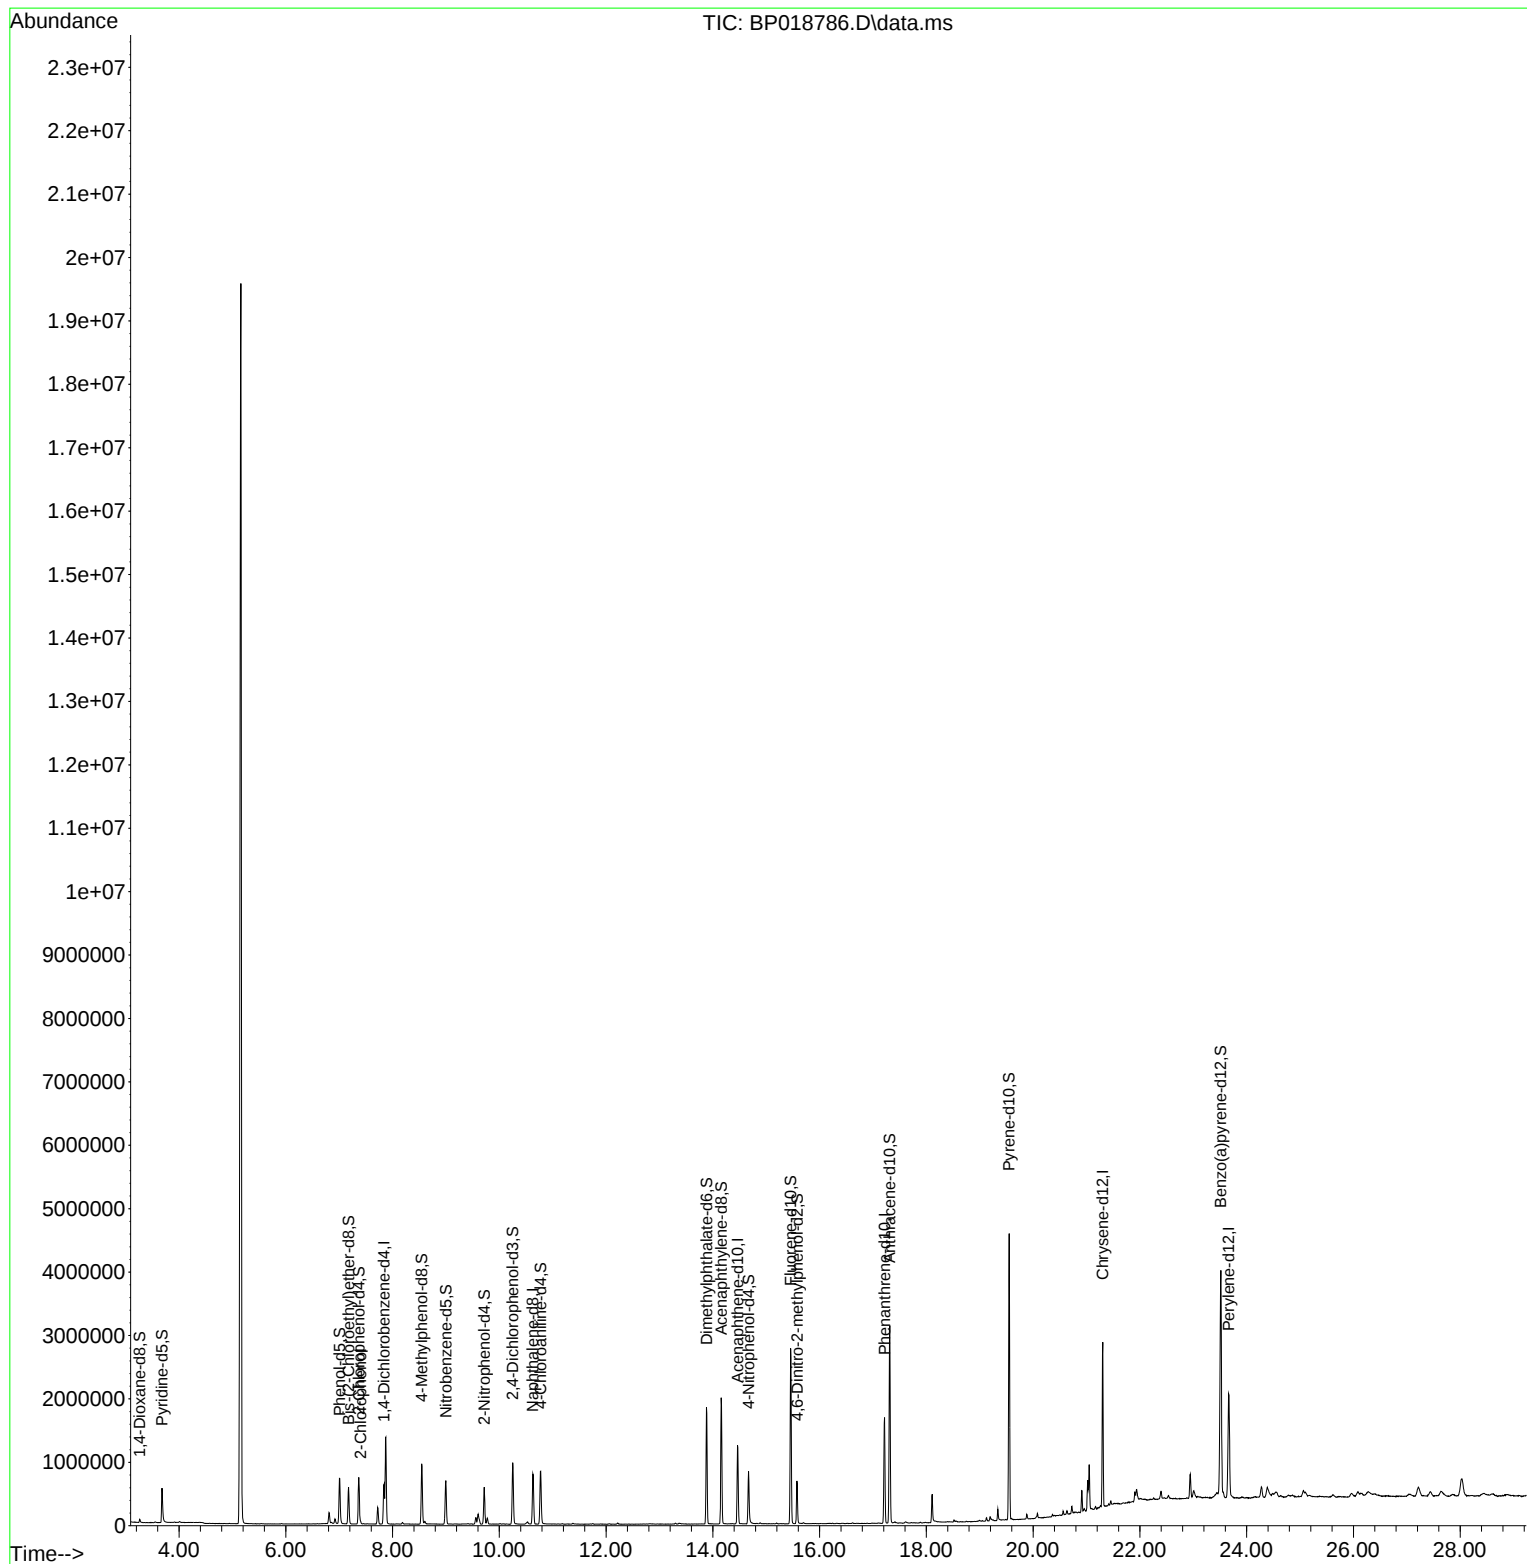

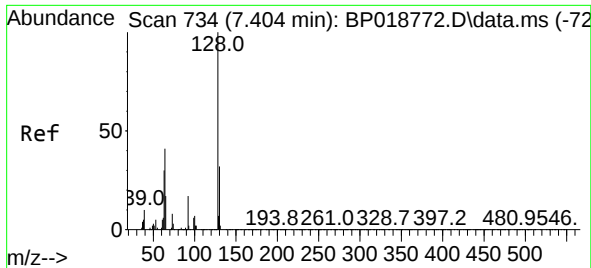

#12
 2-Chlorophenol
 Concen: 1.154 ng/ul
 RT: 7.399 min Scan# 71
 Delta R.T. 0.000 min
 Lab File: BP018786.D
 Acq: 13 Dec 2023 01:56

Instrument :
 BNA_P
 ClientSampleId :
 C0AY5

Tgt Ion:128 Resp: 15703
 Ion Ratio Lower Upper
 128 100
 64 52.8 37.0 55.4
 130 36.5 26.8 40.2

