

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018788.D
 Acq On : 13 Dec 2023 03:03
 Operator : MA/JU
 Sample : 05646-11
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AY7

Quant Time: Dec 13 03:32:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 11 22:02:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.840	152	169315	20.000	ng/u1	0.00
20) Naphthalene-d8	10.634	136	632566	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.463	164	415699	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.216	188	994592	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.304	240	1070833	20.000	ng/u1	# 0.00
88) Perylene-d12	23.663	264	1261144	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	12340	2.484	ng/uL	0.00
4) Pyridine-d5	3.687	84	45602	3.426	ng/u1	0.01
7) Phenol-d5	7.005	99	213771	12.581	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.175	67	127382	12.649	ng/u1	0.00
11) 2-Chlorophenol-d4	7.369	132	175927	13.269	ng/u1	0.00
15) 4-Methylphenol-d8	8.546	113	169650	12.337	ng/u1	0.00
21) Nitrobenzene-d5	8.999	128	81914	14.549	ng/u1	0.00
24) 2-Nitrophenol-d4	9.716	143	90723	15.543	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.252	165	182388	15.281	ng/u1	0.00
31) 4-Chloroaniline-d4	10.775	131	103062	6.607	ng/u1	0.00
46) Dimethylphthalate-d6	13.881	166	565914	15.253	ng/u1	0.00
49) Acenaphthylene-d8	14.157	160	609592	14.921	ng/u1	0.00
54) 4-Nitrophenol-d4	14.669	143	66620	10.939	ng/u1	0.00
60) Fluorene-d10	15.457	176	497791	15.984	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.575	200	60469	10.140	ng/u1	-0.01
73) Anthracene-d10	17.310	188	782031	14.956	ng/u1	-0.01
81) Pyrene-d10	19.551	212	1079523	12.951	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.510	264	1099850	14.957	ng/u1	-0.02
Target Compounds						
					Qvalue	
6) Benzaldehyde	6.981	77	13723	1.564	ng/u1	97
8) Phenol	7.034	94	32474	1.949	ng/u1	90
16) Acetophenone	8.663	105	139215	6.793	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018788.D
Acq On : 13 Dec 2023 03:03
Operator : MA/JU
Sample : 05646-11
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AY7

Quant Time: Dec 13 03:32:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 11 22:02:13 2023
Response via : Initial Calibration




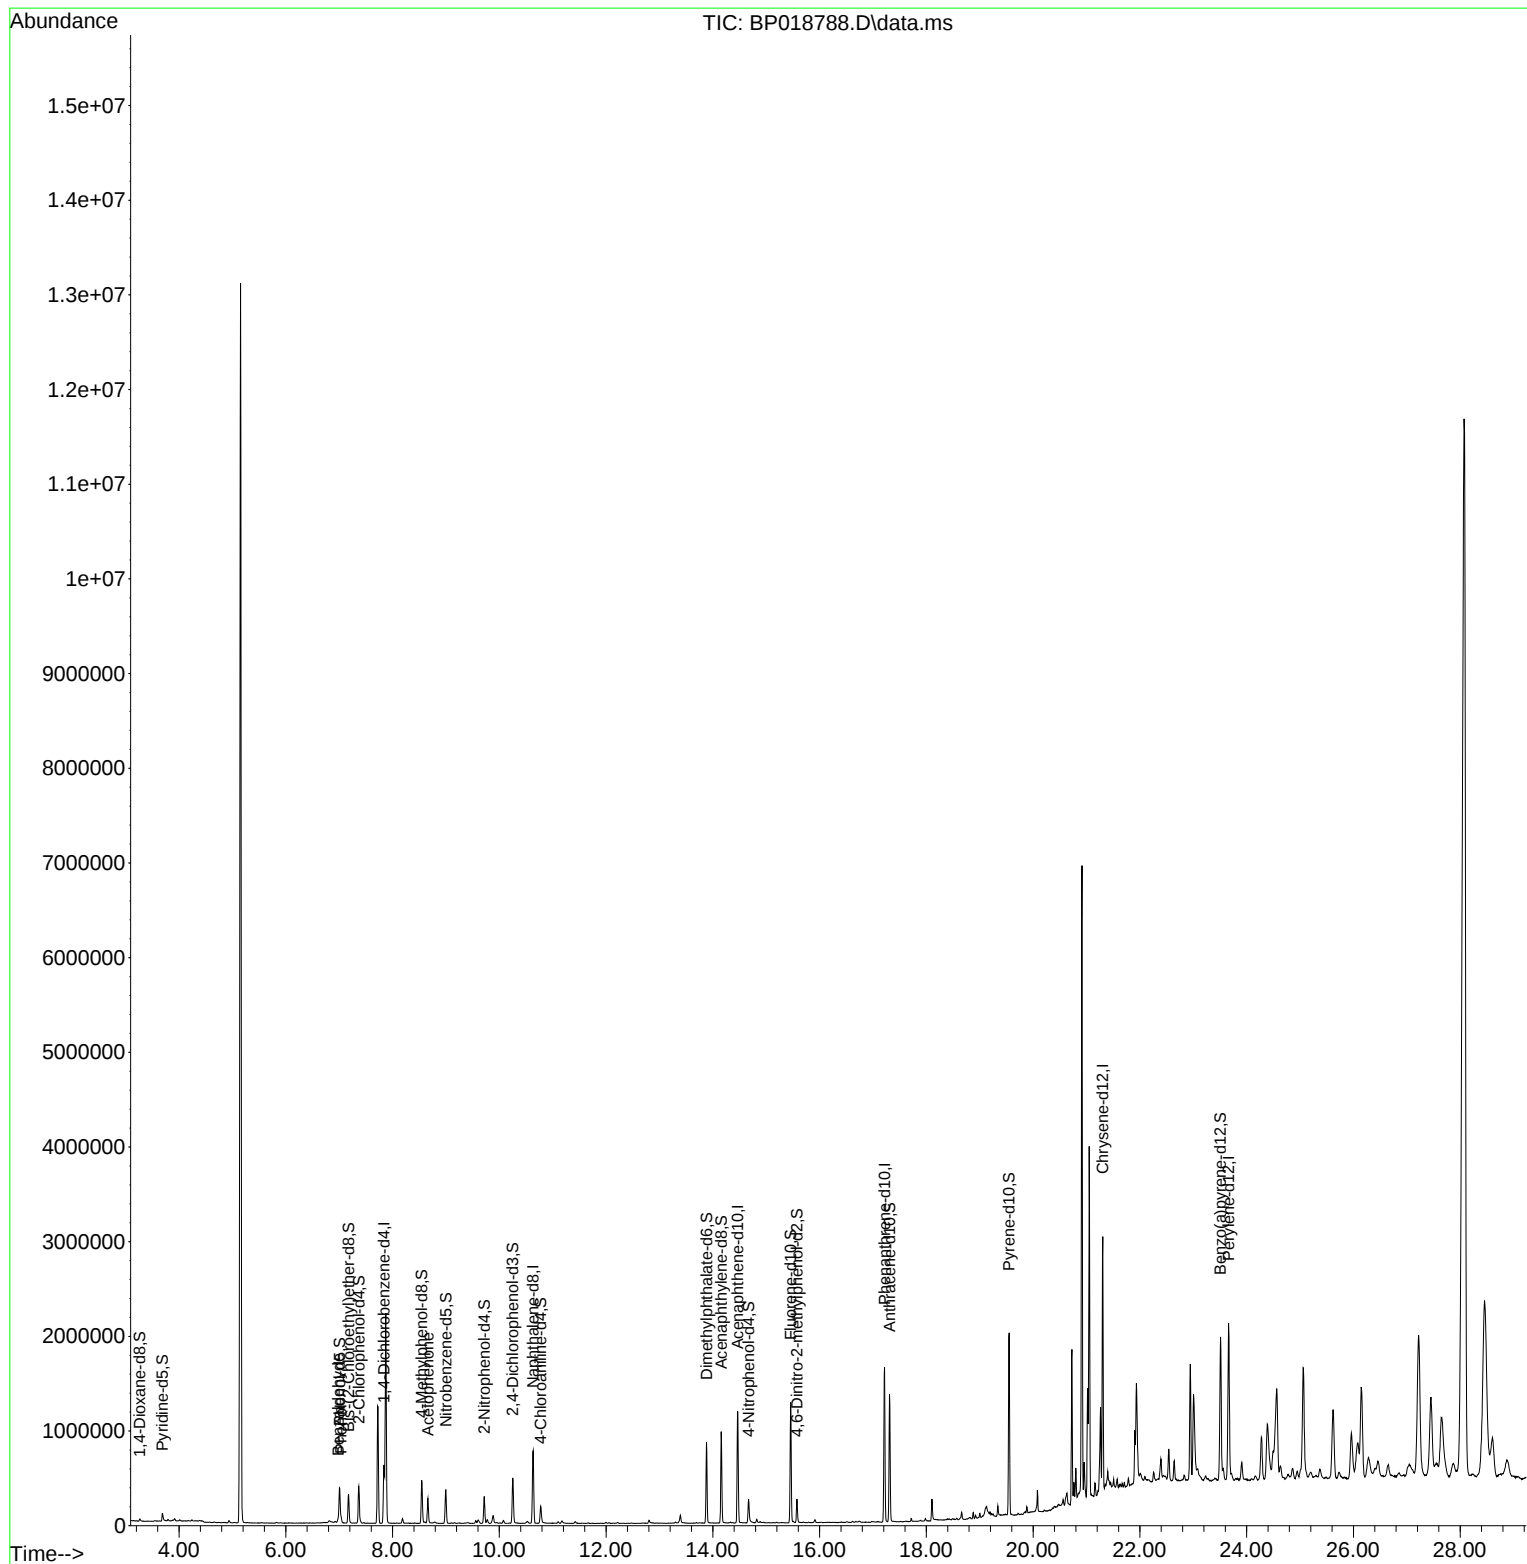


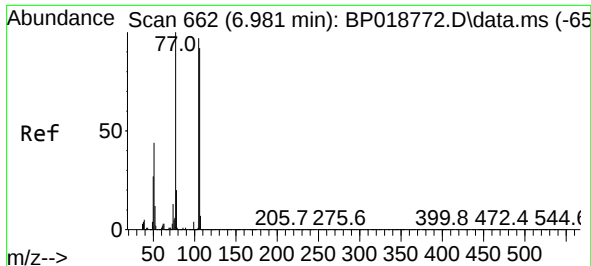

#6
Benzaldehyde
Concen: 1.564 ng/ul
RT: 6.981 min Scan# 662
Delta R.T. 0.006 min
Lab File: BP018788.D
Acq: 13 Dec 2023 03:03




Instrument :
BNA_P
ClientSampleId :
C0AY7


Tgt Ion: 77 Resp: 13723
Ion Ratio Lower Upper
77 100
105 95.8 77.9 116.9
106 89.7 74.6 111.8

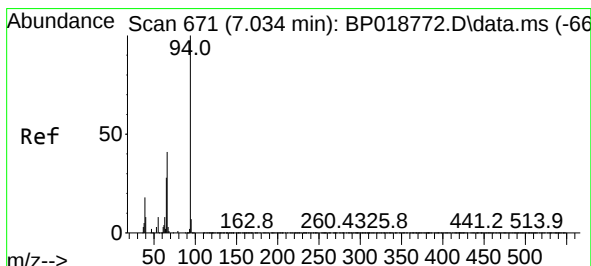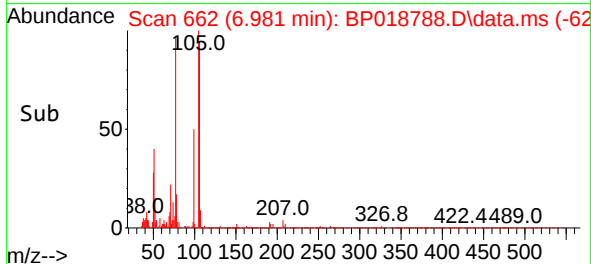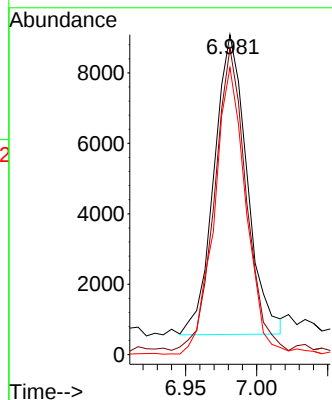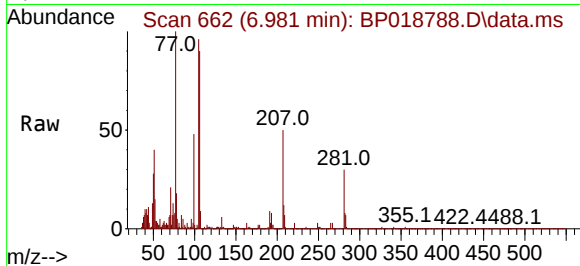

#8
Phenol
Concen: 1.949 ng/ul
RT: 7.034 min Scan# 671
Delta R.T. 0.000 min
Lab File: BP018788.D
Acq: 13 Dec 2023 03:03


Tgt Ion: 94 Resp: 32474
Ion Ratio Lower Upper
94 100
65 31.0 21.0 31.6
66 42.1 28.6 43.0

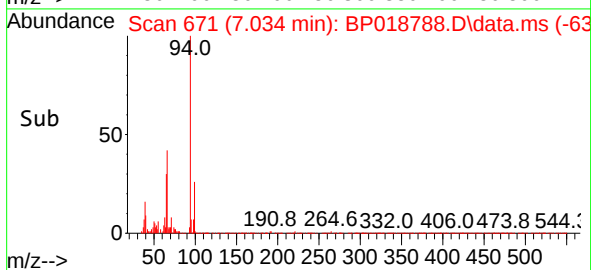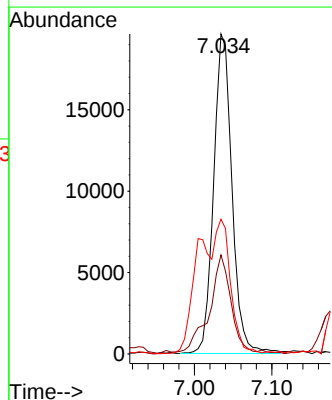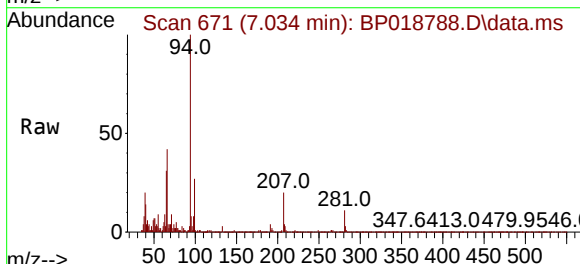

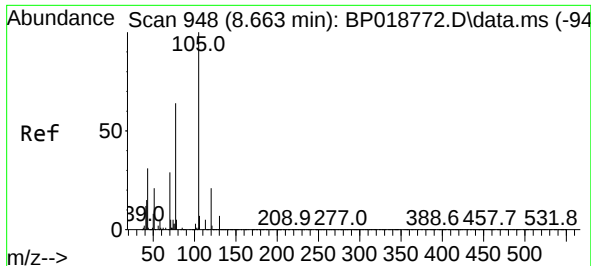

#16
 Acetophenone
 Concen: 6.793 ng/ul
 RT: 8.663 min Scan# 94
 Delta R.T. 0.000 min
 Lab File: BP018788.D
 Acq: 13 Dec 2023 03:03

Instrument :
 BNA_P
 ClientSampleId :
 C0AY7

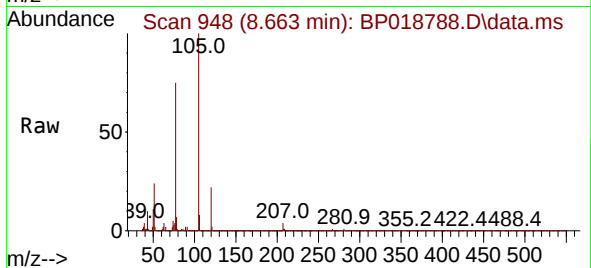

Tgt Ion:105 Resp: 139215
 Ion Ratio Lower Upper
 105 100
 77 75.0 59.4 89.0
 51 24.2 19.4 29.0

