

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018722.D
 Acq On : 11 Dec 2023 11:47
 Operator : MA/JU
 Sample : PB157521BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK521

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018722.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	37	rVB	84828	114783	1.19%	0.158%
2	3.681	97	101	116	rBV	1043933	1526361	15.82%	2.096%
3	4.017	154	158	161	rVB2	11705	15173	0.16%	0.021%
4	4.346	211	214	219	rVB2	19927	23884	0.25%	0.033%
5	7.011	659	667	677	rBV	1149102	1786373	18.51%	2.453%
6	7.181	689	696	708	rVB	944556	1470226	15.24%	2.019%
7	7.369	721	728	735	rBV	1123251	1786018	18.51%	2.452%
8	7.840	802	808	817	rBV	700920	1123223	11.64%	1.542%
9	7.934	817	824	826	rBV3	5970	13482	0.14%	0.019%
10	8.552	923	929	944	rBV	1443332	2267850	23.50%	3.114%
11	9.005	997	1006	1013	rBV	1049237	1684862	17.46%	2.313%
12	9.175	1031	1035	1040	rVB3	7659	13470	0.14%	0.018%
13	9.722	1120	1128	1136	rBV	806833	1292349	13.39%	1.774%
14	10.258	1212	1219	1229	rBV	1394447	2252530	23.34%	3.093%
15	10.640	1276	1284	1291	rVB	973436	1609136	16.68%	2.209%
16	10.781	1300	1308	1318	rBV	1432457	2430721	25.19%	3.337%
17	12.228	1549	1554	1561	rVB2	25689	44295	0.46%	0.061%
18	12.934	1665	1674	1675	rBV	10491	21052	0.22%	0.029%
19	13.375	1744	1749	1754	rBV5	14158	24370	0.25%	0.033%
20	13.887	1830	1836	1847	rBV	2643901	3700387	38.35%	5.081%
21	14.163	1876	1883	1893	rBV	2815433	4185397	43.37%	5.747%
22	14.475	1929	1936	1943	rVB	1411173	2107753	21.84%	2.894%
23	14.675	1963	1970	1981	rBV	1174660	1821647	18.88%	2.501%
24	15.463	2098	2104	2111	rBV	3955447	5529208	57.30%	7.592%
25	15.581	2118	2124	2140	rBV	1078469	1559072	16.16%	2.141%
26	15.704	2142	2145	2149	rVB2	16105	20023	0.21%	0.027%
27	17.222	2396	2403	2409	rBV	1874539	2668328	27.65%	3.664%
28	17.322	2413	2420	2431	rVV	4371182	6492342	67.28%	8.914%
29	18.110	2551	2554	2557	rVB3	17493	20036	0.21%	0.028%
30	19.134	2724	2728	2735	rVB	62949	78584	0.81%	0.108%
31	19.204	2736	2740	2744	rVV	57142	73685	0.76%	0.101%
32	19.345	2762	2764	2766	rBV2	15647	13117	0.14%	0.018%
33	19.557	2794	2800	2807	rBV	6296453	8401860	87.07%	11.536%
34	21.310	3093	3098	3107	rBV	2634281	3367723	34.90%	4.624%
35	23.527	3468	3475	3490	rVB2	4983157	9649868	100.00%	13.250%
36	23.680	3495	3501	3514	rVB	1789992	3641992	37.74%	5.001%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018722.D
Acq On : 11 Dec 2023 11:47
Operator : MA/JU
Sample : PB157521BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK521

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 72831180

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018722.D
Acq On : 11 Dec 2023 11:47
Operator : MA/JU
Sample : PB157521BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK521

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

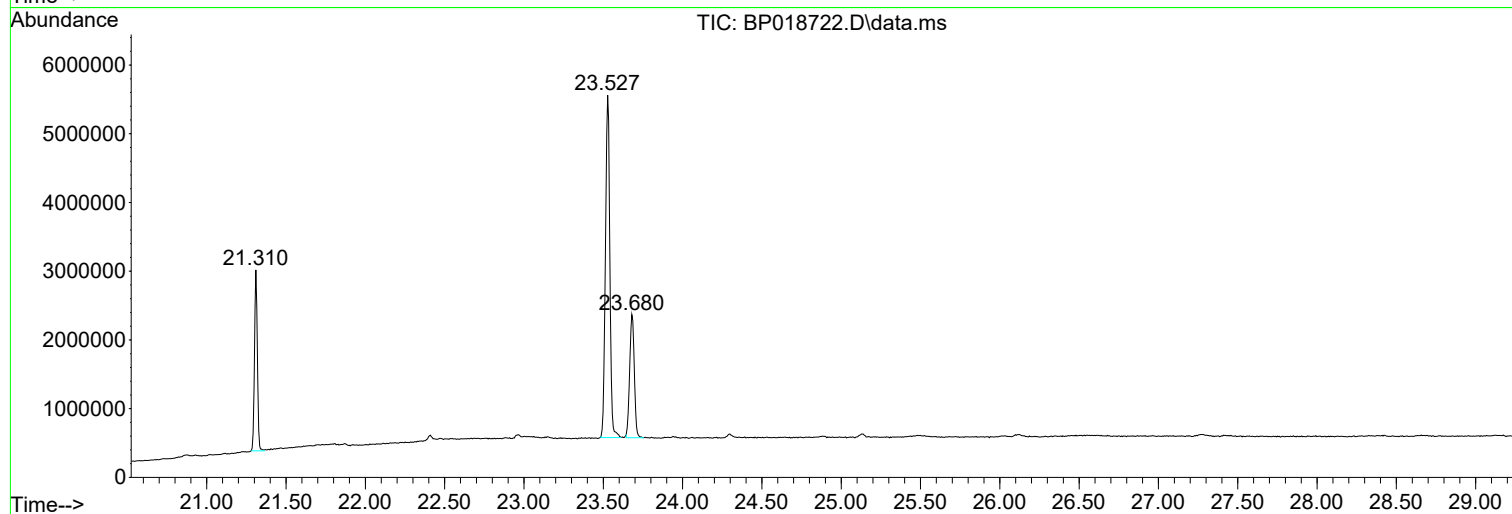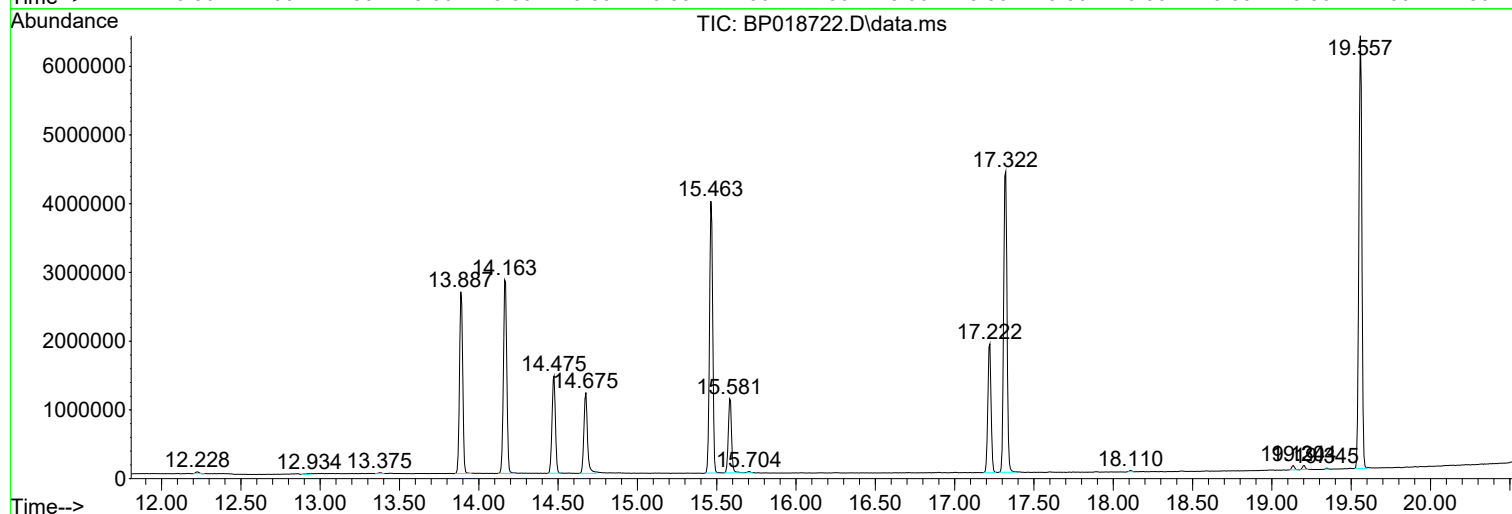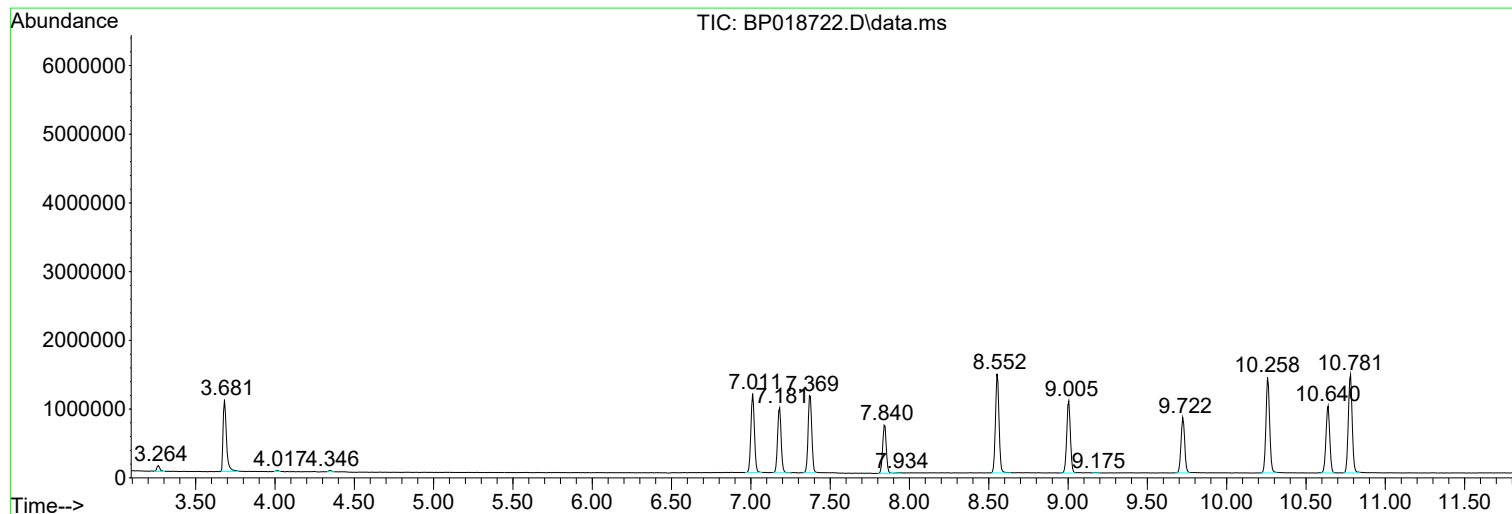

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018722.D
Acq On : 11 Dec 2023 11:47
Operator : MA/JU
Sample : PB157521BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK521

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018722.D
Acq On : 11 Dec 2023 11:47
Operator : MA/JU
Sample : PB157521BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK521

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc