

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018724.D
 Acq On : 11 Dec 2023 12:55
 Operator : MA/JU
 Sample : 05459-12
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AJ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018724.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	36	rVB4	10789	15858	0.55%	0.067%
2	3.693	100	103	113	rBV2	22346	38027	1.32%	0.162%
3	3.793	117	120	125	rVB	13663	19177	0.67%	0.082%
4	3.917	138	141	147	rVB	24005	37561	1.31%	0.160%
5	4.017	153	158	165	rVB2	15338	25961	0.90%	0.110%
6	4.240	194	196	203	rVB5	8253	11703	0.41%	0.050%
7	4.658	265	267	272	rVB4	7671	9831	0.34%	0.042%
8	4.746	280	282	285	rVB3	4807	4806	0.17%	0.020%
9	4.934	311	314	323	rVB	20673	29636	1.03%	0.126%
10	5.046	331	333	338	rVB2	4266	5500	0.19%	0.023%
11	5.264	367	370	372	rBV	2933	3716	0.13%	0.016%
12	5.299	374	376	378	rBV2	3433	3949	0.14%	0.017%
13	5.340	381	383	387	rBV2	3262	4507	0.16%	0.019%
14	5.546	415	418	420	rBV4	3981	4230	0.15%	0.018%
15	5.740	450	451	454	rBV	3588	3559	0.12%	0.015%
16	5.828	463	466	469	rBV3	4654	6543	0.23%	0.028%
17	5.946	482	486	489	rBV2	2682	3823	0.13%	0.016%
18	6.346	552	554	557	rVB2	3811	3410	0.12%	0.014%
19	7.011	659	667	679	rVB	259525	443232	15.41%	1.884%
20	7.175	689	695	703	rVB	228635	358471	12.47%	1.524%
21	7.369	722	728	736	rBV	252876	399382	13.89%	1.698%
22	7.469	740	745	753	rVB8	7815	15784	0.55%	0.067%
23	7.664	773	778	783	rVB2	4903	9638	0.34%	0.041%
24	7.840	802	808	817	rVB	683354	1067997	37.14%	4.540%
25	8.064	844	846	849	rBV2	2285	3561	0.12%	0.015%
26	8.240	874	876	878	rBV2	2985	3321	0.12%	0.014%
27	8.469	912	915	920	rBV2	2396	4607	0.16%	0.020%
28	8.552	922	929	937	rBV	218773	367070	12.76%	1.560%
29	8.669	943	949	957	rVB	126914	208100	7.24%	0.885%
30	8.799	965	971	975	rBV3	6090	9000	0.31%	0.038%
31	8.999	999	1005	1012	rBV	229196	379405	13.19%	1.613%
32	9.099	1019	1022	1024	rBV2	4136	4755	0.17%	0.020%
33	9.163	1030	1033	1035	rBV2	3399	3931	0.14%	0.017%
34	9.252	1045	1048	1049	rBV	6430	4954	0.17%	0.021%
35	9.493	1086	1089	1092	rVB2	3484	4545	0.16%	0.019%
36	9.605	1106	1108	1110	rBV2	3909	4351	0.15%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018724.D
 Acq On : 11 Dec 2023 12:55
 Operator : MA/JU
 Sample : 05459-12
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AJ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	9.722	1122	1128	1134	rBV	153449	242424	8.43%	1.030%
38	9.869	1147	1153	1163	rBV2	15218	41413	1.44%	0.176%
39	9.969	1168	1170	1172	rBV3	3439	3580	0.12%	0.015%
40	10.087	1184	1190	1195	rBV4	15406	26757	0.93%	0.114%
41	10.258	1212	1219	1229	rBV	266858	457866	15.92%	1.946%
42	10.358	1234	1236	1240	rVB	3895	3975	0.14%	0.017%
43	10.534	1262	1266	1267	rBV	6160	7589	0.26%	0.032%
44	10.640	1276	1284	1291	rBV	836786	1410285	49.04%	5.994%
45	10.781	1300	1308	1316	rBV	204131	375217	13.05%	1.595%
46	10.905	1328	1329	1332	rVB	4200	3342	0.12%	0.014%
47	10.963	1337	1339	1341	rVB2	3699	3284	0.11%	0.014%
48	11.116	1362	1365	1369	rBV	4312	5337	0.19%	0.023%
49	11.187	1369	1377	1384	rVV6	8725	25107	0.87%	0.107%
50	11.257	1387	1389	1392	rVB	5260	4099	0.14%	0.017%
51	11.434	1415	1419	1424	rBV4	7769	13952	0.49%	0.059%
52	11.587	1443	1445	1448	rBV2	3608	4595	0.16%	0.020%
53	11.681	1455	1461	1468	rBV2	5942	18023	0.63%	0.077%
54	11.905	1495	1499	1500	rBV2	4160	3769	0.13%	0.016%
55	12.010	1512	1517	1519	rBV3	6534	8984	0.31%	0.038%
56	12.216	1547	1552	1553	rBV2	9754	11305	0.39%	0.048%
57	12.340	1571	1573	1575	rBV	5190	4750	0.17%	0.020%
58	12.399	1580	1583	1584	rVB	3111	3535	0.12%	0.015%
59	12.734	1634	1640	1641	rBV2	5636	7683	0.27%	0.033%
60	12.757	1641	1644	1647	rBV3	3804	4626	0.16%	0.020%
61	12.834	1656	1657	1660	rBV2	4117	3937	0.14%	0.017%
62	12.910	1666	1670	1672	rBV5	4308	4648	0.16%	0.020%
63	13.375	1744	1749	1754	rBV	23613	33257	1.16%	0.141%
64	13.616	1787	1790	1791	rBV	4484	3231	0.11%	0.014%
65	13.887	1830	1836	1843	rBV	533828	727774	25.31%	3.093%
66	14.163	1877	1883	1891	rBV	576009	830230	28.87%	3.529%
67	14.304	1905	1907	1910	rBV2	4241	4781	0.17%	0.020%
68	14.469	1926	1935	1943	rBV	1175700	1813043	63.05%	7.706%
69	14.675	1963	1970	1982	rVB2	107695	224938	7.82%	0.956%
70	14.834	1993	1997	2001	rBV7	6618	8746	0.30%	0.037%
71	14.898	2003	2008	2013	rVB5	12385	24508	0.85%	0.104%
72	15.463	2097	2104	2111	rBV	743105	1041951	36.23%	4.429%
73	15.581	2117	2124	2132	rBV2	103216	164573	5.72%	0.700%
74	15.698	2141	2144	2145	rBV2	3732	4382	0.15%	0.019%
75	15.816	2159	2164	2166	rVV2	3134	5231	0.18%	0.022%
76	15.898	2176	2178	2181	rVB2	3792	3325	0.12%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018724.D
 Acq On : 11 Dec 2023 12:55
 Operator : MA/JU
 Sample : 05459-12
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AJ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

77	15.945	2181	2186	2189	rBV3	5230	10439	0.36%	0.044%
78	16.104	2212	2213	2218	rVB2	4482	5840	0.20%	0.025%
79	16.157	2218	2222	2223	rBV2	5235	5999	0.21%	0.025%
80	16.181	2223	2226	2227	rVV	6290	5566	0.19%	0.024%
81	16.198	2227	2229	2234	rVB	5871	8880	0.31%	0.038%
82	16.245	2234	2237	2239	rBV2	5254	6444	0.22%	0.027%
83	16.334	2251	2252	2256	rBV3	3404	4948	0.17%	0.021%
84	16.451	2271	2272	2276	rBV3	3336	3723	0.13%	0.016%
85	16.581	2292	2294	2298	rVB3	3829	3639	0.13%	0.015%
86	16.628	2298	2302	2304	rBV3	3843	5050	0.18%	0.021%
87	16.763	2322	2325	2329	rBV5	6698	8539	0.30%	0.036%
88	17.222	2396	2403	2408	rBV	1427942	2028209	70.53%	8.621%
89	17.322	2414	2420	2430	rVV	776728	1153640	40.12%	4.904%
90	17.422	2433	2437	2441	rVB5	13966	20645	0.72%	0.088%
91	17.828	2501	2506	2507	rBV2	11432	17019	0.59%	0.072%
92	18.110	2550	2554	2558	rBV3	53696	68347	2.38%	0.291%
93	18.663	2646	2648	2653	rBV3	14175	16638	0.58%	0.071%
94	18.886	2683	2686	2689	rBV	17820	20672	0.72%	0.088%
95	19.234	2742	2745	2749	rVB2	39294	49932	1.74%	0.212%
96	19.345	2761	2764	2769	rBV6	26536	32446	1.13%	0.138%
97	19.557	2795	2800	2812	rVB	1354928	1774888	61.72%	7.544%
98	21.310	3093	3098	3103	rBV	2275132	2781732	96.73%	11.824%
99	23.522	3469	3474	3481	rBV2	837687	1503709	52.29%	6.392%
100	23.680	3494	3501	3511	rVB	1445310	2875738	100.00%	12.223%


Sum of corrected areas: 23526635

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018724.D
Acq On : 11 Dec 2023 12:55
Operator : MA/JU
Sample : 05459-12
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AJ7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

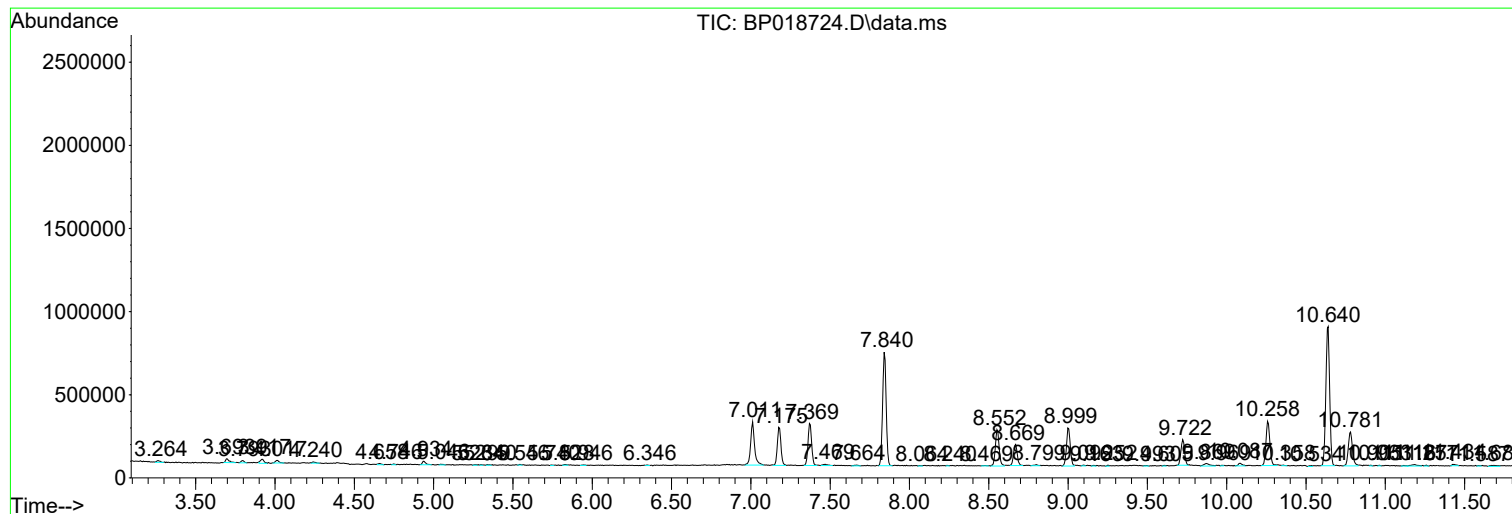

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018724.D
Acq On : 11 Dec 2023 12:55
Operator : MA/JU
Sample : 05459-12
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AJ7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018724.D
Acq On : 11 Dec 2023 12:55
Operator : MA/JU
Sample : 05459-12
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AJ7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc