

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018725.D
 Acq On : 11 Dec 2023 13:29
 Operator : MA/JU
 Sample : 05459-16
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018725.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	28	30	36	rVB3	12923	15107	0.47%	0.054%
2	3.693	100	103	112	rBV	50323	85327	2.67%	0.307%
3	3.799	119	121	123	rBV2	7165	5323	0.17%	0.019%
4	3.917	138	141	146	rVB2	18030	28549	0.89%	0.103%
5	4.017	154	158	163	rVB2	15606	23630	0.74%	0.085%
6	4.934	311	314	322	rVB2	19943	32447	1.01%	0.117%
7	5.593	423	426	427	rBV2	5080	5141	0.16%	0.018%
8	5.822	462	465	466	rBV3	5614	6347	0.20%	0.023%
9	6.134	516	518	520	rBV2	4098	3241	0.10%	0.012%
10	6.675	608	610	611	rBV	3982	3373	0.11%	0.012%
11	6.828	634	636	639	rBV	5565	6227	0.19%	0.022%
12	7.011	660	667	680	rVB	276380	481471	15.04%	1.732%
13	7.116	683	685	689	rBV4	4154	4135	0.13%	0.015%
14	7.175	689	695	702	rBV	285032	448597	14.01%	1.613%
15	7.369	722	728	736	rVB	288024	456161	14.25%	1.641%
16	7.469	742	745	751	rVB3	11363	19076	0.60%	0.069%
17	7.540	753	757	759	rBV3	4542	6200	0.19%	0.022%
18	7.840	801	808	815	rBV	717527	1136675	35.51%	4.088%
19	8.234	874	875	877	rBV	4257	3971	0.12%	0.014%
20	8.552	923	929	940	rBV	232998	363826	11.36%	1.309%
21	8.669	943	949	957	rVV	157929	255835	7.99%	0.920%
22	8.999	999	1005	1013	rBV	291136	477394	14.91%	1.717%
23	9.569	1100	1102	1104	rBV3	3824	4899	0.15%	0.018%
24	9.722	1116	1128	1137	rBV	188583	338140	10.56%	1.216%
25	9.805	1139	1142	1145	rVV2	5100	9043	0.28%	0.033%
26	9.863	1145	1152	1161	rVB3	23573	50841	1.59%	0.183%
27	9.922	1161	1162	1168	rVB2	2504	3490	0.11%	0.013%
28	10.081	1184	1189	1196	rVB3	14090	25794	0.81%	0.093%
29	10.205	1206	1210	1213	rBV4	2684	4312	0.13%	0.016%
30	10.257	1213	1219	1226	rBV	263056	442079	13.81%	1.590%
31	10.493	1258	1259	1263	rBV3	2791	3250	0.10%	0.012%
32	10.634	1275	1283	1291	rBV	691137	1178432	36.81%	4.239%
33	10.687	1291	1292	1297	rVB2	6989	7511	0.23%	0.027%
34	10.781	1299	1308	1318	rBV	199462	365872	11.43%	1.316%
35	10.852	1318	1320	1322	rVB	4125	3373	0.11%	0.012%
36	11.122	1363	1366	1370	rVB3	2463	3556	0.11%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018725.D
 Acq On : 11 Dec 2023 13:29
 Operator : MA/JU
 Sample : 05459-16
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	11.175	1370	1375	1381	rBV10	7444	19215	0.60%	0.069%
38	11.434	1415	1419	1421	rVV4	7206	11455	0.36%	0.041%
39	11.457	1421	1423	1425	rVB2	3365	3218	0.10%	0.012%
40	11.663	1453	1458	1459	rBV3	3517	4085	0.13%	0.015%
41	11.675	1459	1460	1464	rVB2	4983	4811	0.15%	0.017%
42	12.004	1512	1516	1523	rBV2	7260	13777	0.43%	0.050%
43	12.140	1536	1539	1543	rBV5	2765	3922	0.12%	0.014%
44	12.222	1548	1553	1558	rVV4	9557	16972	0.53%	0.061%
45	12.299	1561	1566	1570	rVV2	12264	17807	0.56%	0.064%
46	12.516	1599	1603	1610	rVB4	9430	18177	0.57%	0.065%
47	12.569	1610	1612	1614	rBV3	3226	3858	0.12%	0.014%
48	12.598	1616	1617	1622	rBV	3457	4354	0.14%	0.016%
49	12.681	1629	1631	1633	rBV2	2780	3457	0.11%	0.012%
50	12.810	1649	1653	1655	rBV4	3158	4066	0.13%	0.015%
51	12.916	1669	1671	1674	rBV3	4120	4865	0.15%	0.017%
52	13.081	1695	1699	1702	rVB6	4244	6581	0.21%	0.024%
53	13.298	1731	1736	1742	rBV3	5022	11077	0.35%	0.040%
54	13.375	1744	1749	1755	rBV4	34333	64298	2.01%	0.231%
55	13.434	1757	1759	1760	rBV	4506	3962	0.12%	0.014%
56	13.787	1817	1819	1824	rVB3	7281	11578	0.36%	0.042%
57	13.887	1830	1836	1847	rBV	682700	949808	29.67%	3.416%
58	14.163	1877	1883	1892	rBV	772227	1124168	35.11%	4.043%
59	14.469	1929	1935	1944	rBV	1362890	2034231	63.54%	7.317%
60	14.675	1965	1970	1981	rBV2	113762	210819	6.59%	0.758%
61	14.828	1993	1996	2000	rBV4	10094	13193	0.41%	0.047%
62	14.992	2022	2024	2029	rBV4	4635	6320	0.20%	0.023%
63	15.463	2098	2104	2111	rBV	1081015	1561735	48.78%	5.617%
64	15.581	2119	2124	2132	rBV	112905	166574	5.20%	0.599%
65	16.769	2322	2326	2328	rBV3	7181	8461	0.26%	0.030%
66	17.222	2396	2403	2408	rBV	1763761	2547252	79.57%	9.162%
67	17.316	2414	2419	2431	rVB	1106561	1626009	50.79%	5.848%
68	17.722	2486	2488	2493	rBV6	11373	15013	0.47%	0.054%
69	18.110	2550	2554	2562	rVB4	78787	111474	3.48%	0.401%
70	18.669	2646	2649	2651	rBV3	18264	20069	0.63%	0.072%
71	18.886	2683	2686	2689	rVB2	21959	24986	0.78%	0.090%
72	19.233	2741	2745	2749	rVB	124863	161223	5.04%	0.580%
73	19.345	2761	2764	2768	rBV4	34765	40374	1.26%	0.145%
74	19.557	2794	2800	2814	rBV	1692491	2375284	74.20%	8.543%
75	21.310	3093	3098	3103	rBV	2498720	3201393	100.00%	11.515%
76	23.521	3469	3474	3480	rBV2	1046115	1912335	59.73%	6.878%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018725.D
Acq On : 11 Dec 2023 13:29
Operator : MA/JU
Sample : 05459-16
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

77 23.680 3494 3501 3509 rBV 1620700 3151835 98.45% 11.336%




Sum of corrected areas: 27802736

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018725.D
Acq On : 11 Dec 2023 13:29
Operator : MA/JU
Sample : 05459-16
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

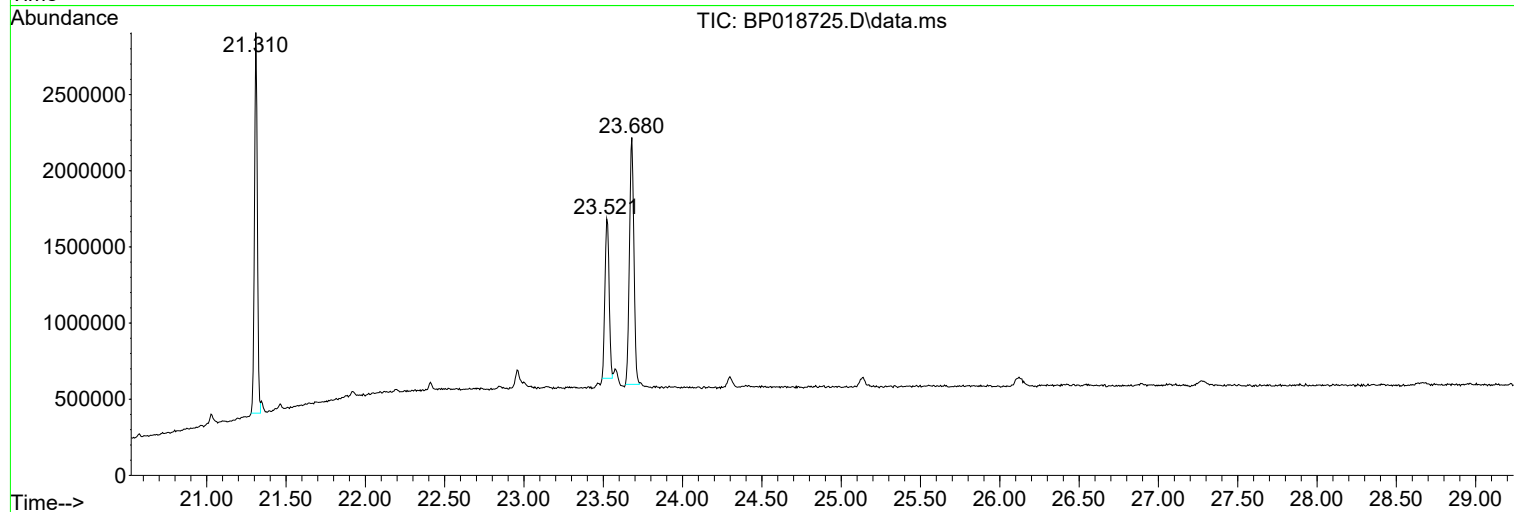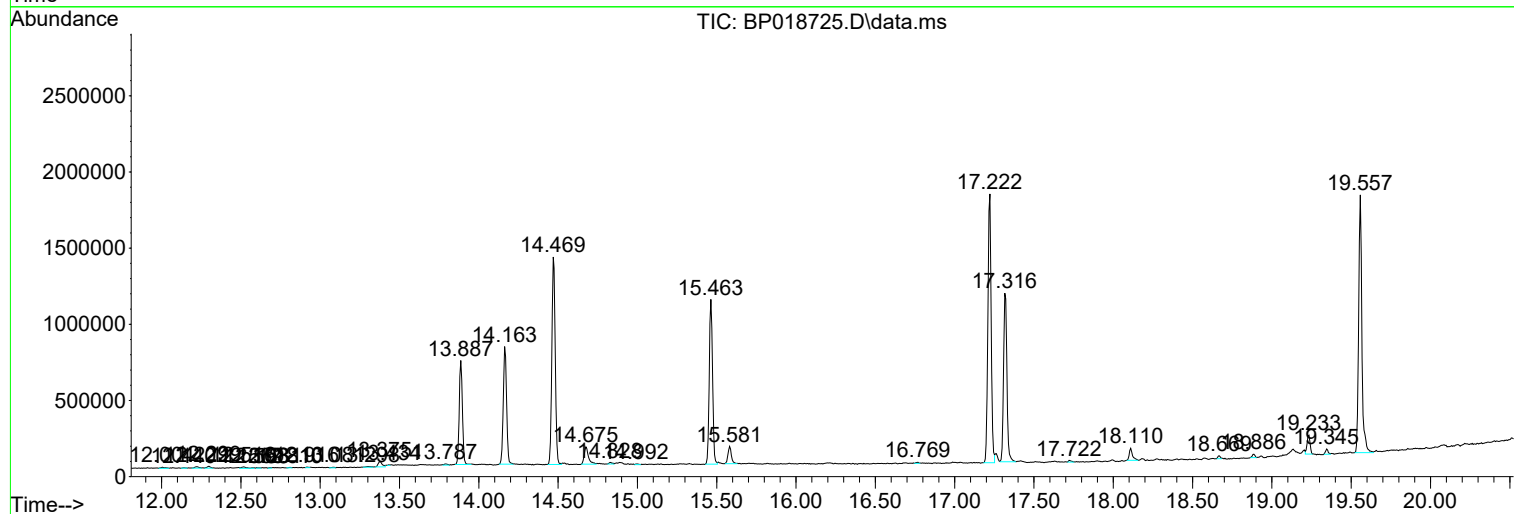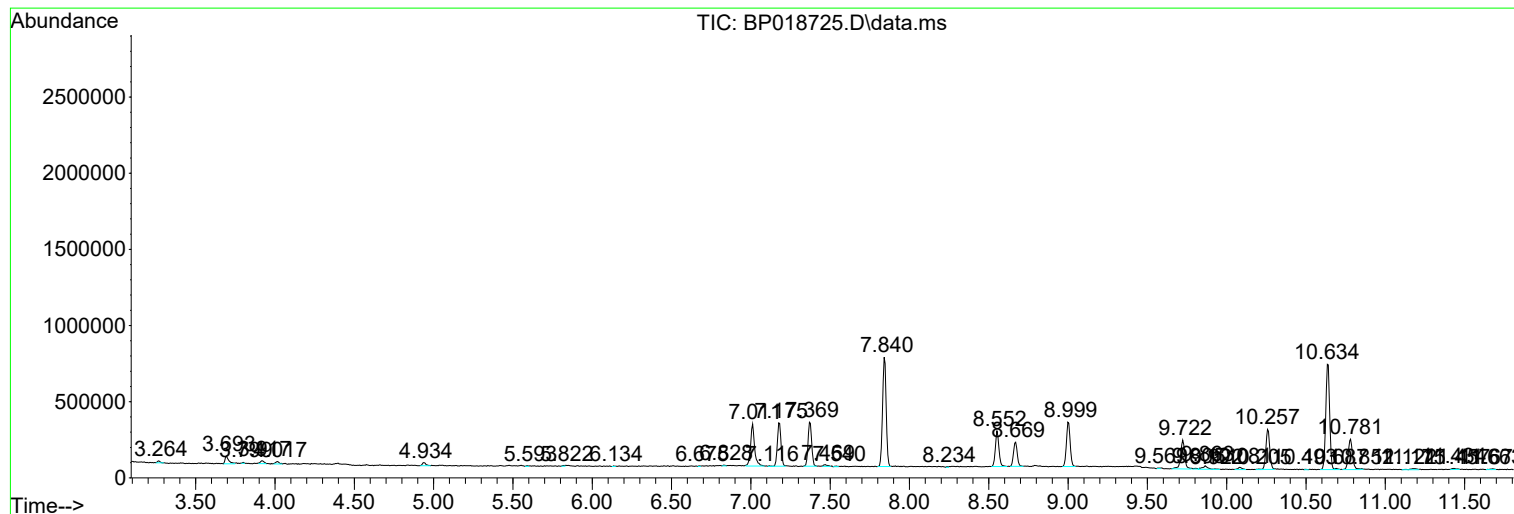

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018725.D
Acq On : 11 Dec 2023 13:29
Operator : MA/JU
Sample : 05459-16
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018725.D
Acq On : 11 Dec 2023 13:29
Operator : MA/JU
Sample : 05459-16
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc