

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018728.D
 Acq On : 11 Dec 2023 15:12
 Operator : MA/JU
 Sample : 05459-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018728.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.693	99	103	111	rBV	69847	112624	3.59%	0.433%
2	3.923	137	142	148	rVB2	23790	39595	1.26%	0.152%
3	4.017	154	158	164	rVB3	15996	27204	0.87%	0.105%
4	4.240	194	196	201	rVB6	8212	8880	0.28%	0.034%
5	4.358	214	216	217	rBV	6081	3897	0.12%	0.015%
6	4.940	310	315	319	rBV	22878	33825	1.08%	0.130%
7	5.105	339	343	344	rVB4	4018	3847	0.12%	0.015%
8	5.181	354	356	357	rBV	4272	3546	0.11%	0.014%
9	5.464	402	404	407	rBV2	6143	7926	0.25%	0.030%
10	5.570	420	422	425	rVB4	3489	3450	0.11%	0.013%
11	5.681	437	441	444	rBV4	3083	4609	0.15%	0.018%
12	5.840	462	468	472	rVV5	8183	19406	0.62%	0.075%
13	6.099	509	512	514	rBV	3831	4770	0.15%	0.018%
14	6.252	535	538	541	rBV2	3807	5026	0.16%	0.019%
15	6.375	557	559	561	rBV2	3056	3245	0.10%	0.012%
16	6.564	587	591	592	rBV4	2492	3462	0.11%	0.013%
17	7.011	659	667	680	rVB	261974	462849	14.77%	1.780%
18	7.175	690	695	702	rVV	222172	350041	11.17%	1.346%
19	7.275	710	712	714	rBV3	3464	4201	0.13%	0.016%
20	7.369	722	728	737	rVB	254013	401403	12.81%	1.544%
21	7.464	741	744	751	rBV5	9222	18375	0.59%	0.071%
22	7.758	792	794	798	rVB3	4749	5651	0.18%	0.022%
23	7.799	798	801	802	rBV	4384	5174	0.17%	0.020%
24	7.840	802	808	816	rVV	684024	1064579	33.97%	4.094%
25	8.246	871	877	878	rVV3	2964	4090	0.13%	0.016%
26	8.552	923	929	936	rBV	253360	391111	12.48%	1.504%
27	8.669	943	949	955	rBV	146177	241700	7.71%	0.930%
28	8.793	966	970	973	rBV3	7064	10788	0.34%	0.041%
29	8.822	973	975	978	rVB3	3753	3530	0.11%	0.014%
30	8.999	999	1005	1013	rVV	232022	384488	12.27%	1.479%
31	9.116	1022	1025	1027	rBV3	4111	3558	0.11%	0.014%
32	9.322	1058	1060	1063	rBV4	2989	3813	0.12%	0.015%
33	9.387	1068	1071	1072	rBV2	2667	3250	0.10%	0.012%
34	9.616	1108	1110	1115	rVB	8250	11365	0.36%	0.044%
35	9.669	1117	1119	1121	rVV	6354	5404	0.17%	0.021%
36	9.722	1121	1128	1142	rVB	156799	276018	8.81%	1.062%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018728.D
 Acq On : 11 Dec 2023 15:12
 Operator : MA/JU
 Sample : 05459-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	9.869	1147	1153	1158	rBV3	19943	33914	1.08%	0.130%
38	10.087	1183	1190	1196	rBV2	17899	37868	1.21%	0.146%
39	10.146	1196	1200	1202	rBV	5644	7813	0.25%	0.030%
40	10.258	1212	1219	1229	rBV	286973	474235	15.13%	1.824%
41	10.634	1276	1283	1290	rBV	845464	1436712	45.85%	5.525%
42	10.687	1290	1292	1298	rVB	12752	16473	0.53%	0.063%
43	10.781	1298	1308	1321	rBV	223476	417069	13.31%	1.604%
44	11.181	1371	1376	1381	rBV6	9022	20401	0.65%	0.078%
45	11.299	1392	1396	1399	rBV2	3945	6329	0.20%	0.024%
46	11.434	1413	1419	1425	rBV2	9546	19789	0.63%	0.076%
47	11.557	1439	1440	1447	rVB2	3905	6734	0.21%	0.026%
48	11.669	1455	1459	1467	rVB5	9767	18158	0.58%	0.070%
49	12.005	1513	1516	1521	rVB4	8281	13851	0.44%	0.053%
50	12.057	1521	1525	1530	rBV6	6873	9157	0.29%	0.035%
51	12.222	1549	1553	1558	rVB3	10648	19043	0.61%	0.073%
52	12.299	1561	1566	1573	rVB3	18209	31448	1.00%	0.121%
53	12.510	1598	1602	1608	rVB5	12801	20433	0.65%	0.079%
54	12.716	1636	1637	1639	rBV2	3979	3578	0.11%	0.014%
55	12.904	1666	1669	1670	rBV	4560	3579	0.11%	0.014%
56	12.999	1683	1685	1686	rBV	3177	3254	0.10%	0.013%
57	13.299	1733	1736	1741	rBV4	8524	13052	0.42%	0.050%
58	13.375	1744	1749	1756	rVB3	24969	44330	1.41%	0.170%
59	13.440	1758	1760	1765	rBV6	3065	5265	0.17%	0.020%
60	13.528	1774	1775	1781	rVB2	4214	6225	0.20%	0.024%
61	13.628	1789	1792	1793	rBV2	5879	4920	0.16%	0.019%
62	13.646	1793	1795	1798	rVV	6651	9233	0.29%	0.036%
63	13.763	1811	1815	1816	rBV2	2509	3717	0.12%	0.014%
64	13.787	1816	1819	1820	rBV3	10228	9445	0.30%	0.036%
65	13.846	1827	1829	1830	rBV2	4216	3259	0.10%	0.013%
66	13.887	1830	1836	1844	rVV	554908	744412	23.75%	2.863%
67	13.963	1846	1849	1852	rVB4	6990	8203	0.26%	0.032%
68	14.028	1858	1860	1865	rVV6	6249	8432	0.27%	0.032%
69	14.069	1865	1867	1870	rVB	6012	5985	0.19%	0.023%
70	14.163	1877	1883	1896	rBV	596894	899729	28.71%	3.460%
71	14.375	1915	1919	1922	rVB2	11727	14870	0.47%	0.057%
72	14.469	1929	1935	1943	rBV	1299704	1906653	60.84%	7.333%
73	14.675	1964	1970	1983	rBV2	123743	243094	7.76%	0.935%
74	14.828	1993	1996	2000	rBV4	9905	14426	0.46%	0.055%
75	14.875	2000	2004	2005	rBV	8083	10715	0.34%	0.041%
76	15.140	2044	2049	2051	rBV3	4873	7450	0.24%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018728.D
 Acq On : 11 Dec 2023 15:12
 Operator : MA/JU
 Sample : 05459-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

77	15.257	2067	2069	2074	rBV4	5982	9472	0.30%	0.036%
78	15.328	2078	2081	2083	rBV4	6927	6971	0.22%	0.027%
79	15.463	2098	2104	2110	rBV	883218	1236762	39.47%	4.756%
80	15.581	2119	2124	2131	rVB	116255	166779	5.32%	0.641%
81	15.787	2157	2159	2160	rBV	5964	4178	0.13%	0.016%
82	16.022	2197	2199	2201	rBV3	3745	3625	0.12%	0.014%
83	16.187	2224	2227	2228	rBV	12179	10543	0.34%	0.041%
84	16.245	2236	2237	2241	rVB	7306	4645	0.15%	0.018%
85	16.610	2298	2299	2300	rBV	6122	3797	0.12%	0.015%
86	16.757	2322	2324	2334	rVB7	10178	19481	0.62%	0.075%
87	17.216	2396	2402	2408	rBV	1702323	2466180	78.70%	9.485%
88	17.257	2408	2409	2414	rVV	52358	56428	1.80%	0.217%
89	17.316	2414	2419	2430	rVB	873554	1298666	41.44%	4.995%
90	17.722	2486	2488	2493	rVB5	12996	15113	0.48%	0.058%
91	18.110	2549	2554	2564	rBV4	90889	134792	4.30%	0.518%
92	18.398	2600	2603	2605	rVB4	9820	9659	0.31%	0.037%
93	18.663	2645	2648	2654	rVB4	22130	30819	0.98%	0.119%
94	18.886	2682	2686	2689	rBV3	30457	43298	1.38%	0.167%
95	19.228	2741	2744	2748	rVB	78170	99021	3.16%	0.381%
96	19.345	2760	2764	2770	rBV3	69410	96629	3.08%	0.372%
97	19.557	2794	2800	2813	rBV	1344056	1919488	61.25%	7.382%
98	21.304	3092	3097	3103	rBV	2422504	3133783	100.00%	12.052%
99	23.516	3468	3473	3480	rBV2	866104	1625590	51.87%	6.252%
100	23.674	3493	3500	3511	rVB	1590637	3105866	99.11%	11.945%




Sum of corrected areas: 26001538

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018728.D
Acq On : 11 Dec 2023 15:12
Operator : MA/JU
Sample : 05459-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

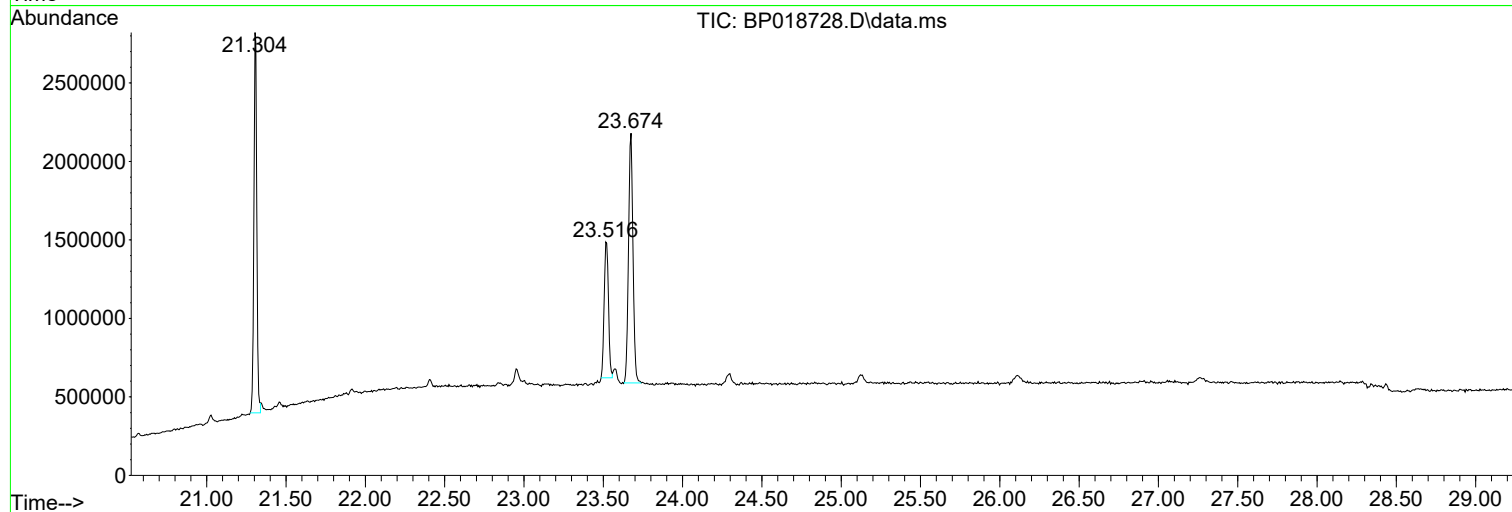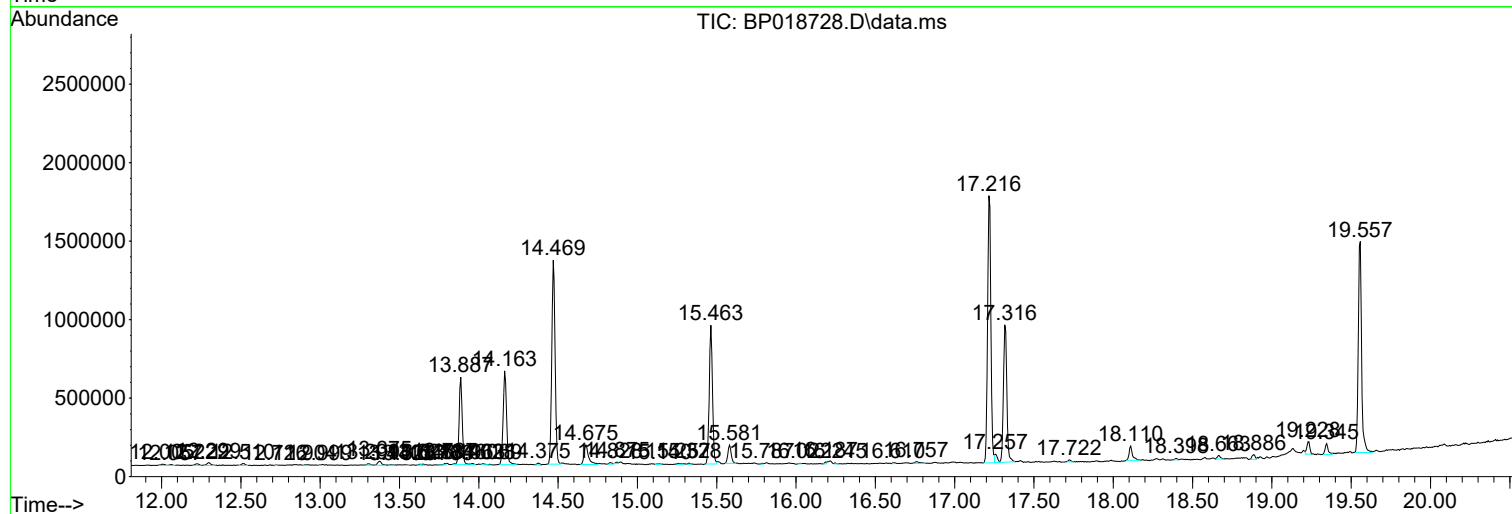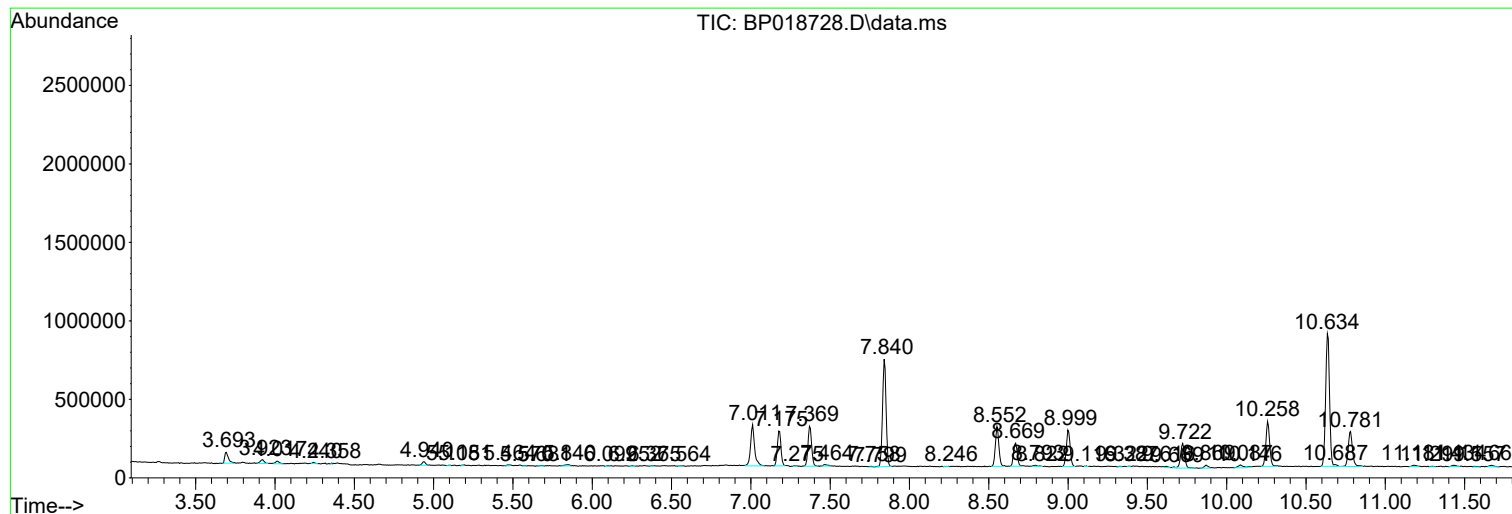

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018728.D
Acq On : 11 Dec 2023 15:12
Operator : MA/JU
Sample : 05459-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018728.D
Acq On : 11 Dec 2023 15:12
Operator : MA/JU
Sample : 05459-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc