

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018729.D
 Acq On : 11 Dec 2023 16:20
 Operator : MA/JU
 Sample : 05459-21
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018729.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	37	rVB2	30329	38581	0.87%	0.092%
2	3.693	99	103	111	rBV2	55540	93200	2.10%	0.222%
3	3.793	118	120	129	rVB2	15765	25227	0.57%	0.060%
4	3.923	137	142	146	rVB3	25084	40323	0.91%	0.096%
5	4.011	154	157	164	rVB2	20078	31126	0.70%	0.074%
6	4.575	250	253	254	rBV3	4992	5656	0.13%	0.013%
7	4.940	310	315	319	rBV	27724	40418	0.91%	0.096%
8	5.187	355	357	361	rBV3	4558	7465	0.17%	0.018%
9	5.546	416	418	424	rVB2	6732	7164	0.16%	0.017%
10	5.764	453	455	458	rBV2	4631	5033	0.11%	0.012%
11	5.822	463	465	470	rVV5	4404	6663	0.15%	0.016%
12	7.011	659	667	679	rVB	474306	787633	17.74%	1.876%
13	7.175	689	695	706	rVB	400216	616991	13.90%	1.469%
14	7.275	711	712	715	rVB2	6032	4854	0.11%	0.012%
15	7.322	715	720	721	rBV3	4105	7042	0.16%	0.017%
16	7.369	721	728	736	rBV	444982	687495	15.49%	1.637%
17	7.458	738	743	748	rBV3	15582	24554	0.55%	0.058%
18	7.540	754	757	759	rVB	4178	4896	0.11%	0.012%
19	7.840	801	808	815	rBV	776679	1214149	27.35%	2.891%
20	8.511	915	922	923	rBV2	3277	6268	0.14%	0.015%
21	8.552	923	929	938	rVV	372945	579554	13.06%	1.380%
22	8.669	941	949	957	rVB	129447	220712	4.97%	0.526%
23	8.999	998	1005	1012	rBV	415339	670224	15.10%	1.596%
24	9.052	1012	1014	1019	rVV4	3478	4710	0.11%	0.011%
25	9.105	1021	1023	1026	rBV4	3615	5025	0.11%	0.012%
26	9.175	1030	1035	1038	rBV3	4293	5456	0.12%	0.013%
27	9.422	1075	1077	1080	rVB4	5510	6415	0.14%	0.015%
28	9.722	1118	1128	1135	rBV	287402	474227	10.68%	1.129%
29	9.869	1147	1153	1159	rBV3	16955	33624	0.76%	0.080%
30	9.952	1165	1167	1173	rVB4	3759	6332	0.14%	0.015%
31	10.081	1184	1189	1196	rBV3	15354	27053	0.61%	0.064%
32	10.258	1213	1219	1233	rBV	492849	792225	17.85%	1.887%
33	10.634	1276	1283	1290	rBV	972598	1622952	36.56%	3.865%
34	10.687	1290	1292	1298	rVB4	9377	10851	0.24%	0.026%
35	10.775	1301	1307	1320	rVB	367393	638586	14.39%	1.521%
36	11.181	1372	1376	1381	rVB6	7473	15500	0.35%	0.037%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018729.D
 Acq On : 11 Dec 2023 16:20
 Operator : MA/JU
 Sample : 05459-21
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	11.293	1391	1395	1398	rVB5	3584	5287	0.12%	0.013%
38	11.428	1414	1418	1423	rBV3	8132	14167	0.32%	0.034%
39	12.005	1512	1516	1522	rBV4	7254	10445	0.24%	0.025%
40	12.222	1547	1553	1558	rBV2	19108	31506	0.71%	0.075%
41	12.299	1562	1566	1569	rBV4	4781	7535	0.17%	0.018%
42	12.616	1619	1620	1624	rBV2	3659	4671	0.11%	0.011%
43	13.375	1743	1749	1756	rBV2	50517	84807	1.91%	0.202%
44	13.440	1758	1760	1767	rVB5	7376	12223	0.28%	0.029%
45	13.699	1802	1804	1811	rVB4	7583	9775	0.22%	0.023%
46	13.799	1817	1821	1824	rBV3	5321	8097	0.18%	0.019%
47	13.887	1830	1836	1845	rBV	1122916	1524371	34.34%	3.630%
48	14.163	1875	1883	1896	rBV	1278558	1877871	42.30%	4.472%
49	14.469	1929	1935	1946	rBV	1742782	2562458	57.72%	6.102%
50	14.675	1964	1970	1980	rBV2	113855	205129	4.62%	0.489%
51	14.828	1991	1996	2000	rBV4	16465	25854	0.58%	0.062%
52	14.893	2005	2007	2013	rVB5	18961	27086	0.61%	0.065%
53	15.328	2078	2081	2083	rVB	6053	5237	0.12%	0.012%
54	15.463	2097	2104	2111	rBV	1771572	2473345	55.72%	5.890%
55	15.581	2119	2124	2131	rBV2	102180	149856	3.38%	0.357%
56	16.022	2196	2199	2206	rBV5	5139	10502	0.24%	0.025%
57	16.193	2224	2228	2229	rBV4	6376	8210	0.18%	0.020%
58	16.622	2299	2301	2307	rVB2	9879	10631	0.24%	0.025%
59	16.763	2321	2325	2330	rBV5	17308	26805	0.60%	0.064%
60	17.216	2396	2402	2407	rBV	2170228	3180877	71.66%	7.575%
61	17.263	2407	2410	2414	rVV	220004	297512	6.70%	0.709%
62	17.316	2414	2419	2431	rVB	1867055	2611634	58.83%	6.220%
63	17.892	2514	2517	2522	rBV4	20190	26898	0.61%	0.064%
64	17.987	2530	2533	2539	rVB5	14061	24395	0.55%	0.058%
65	18.110	2547	2554	2564	rBV2	166707	293237	6.61%	0.698%
66	18.275	2578	2582	2585	rBV2	29494	46148	1.04%	0.110%
67	18.575	2630	2633	2636	rVB	27595	28263	0.64%	0.067%
68	18.663	2646	2648	2655	rVB3	24116	32205	0.73%	0.077%
69	18.886	2683	2686	2689	rVB2	23683	26983	0.61%	0.064%
70	19.134	2722	2728	2733	rBV6	40144	90535	2.04%	0.216%
71	19.228	2736	2744	2754	rVB	564420	802946	18.09%	1.912%
72	19.345	2761	2764	2767	rBV2	66512	71961	1.62%	0.171%
73	19.557	2794	2800	2811	rBV2	2660721	4159837	93.71%	9.907%
74	21.310	3091	3098	3102	rBV	3110541	4439107	100.00%	10.572%
75	22.951	3374	3377	3383	rBV	186537	308367	6.95%	0.734%
76	23.522	3468	3474	3480	rBV2	1815059	3412076	76.86%	8.126%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018729.D
Acq On : 11 Dec 2023 16:20
Operator : MA/JU
Sample : 05459-21
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

77 23.674 3493 3500 3514 rVB 2182264 4273290 96.26% 10.177%




Sum of corrected areas: 41990323

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018729.D
Acq On : 11 Dec 2023 16:20
Operator : MA/JU
Sample : 05459-21
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

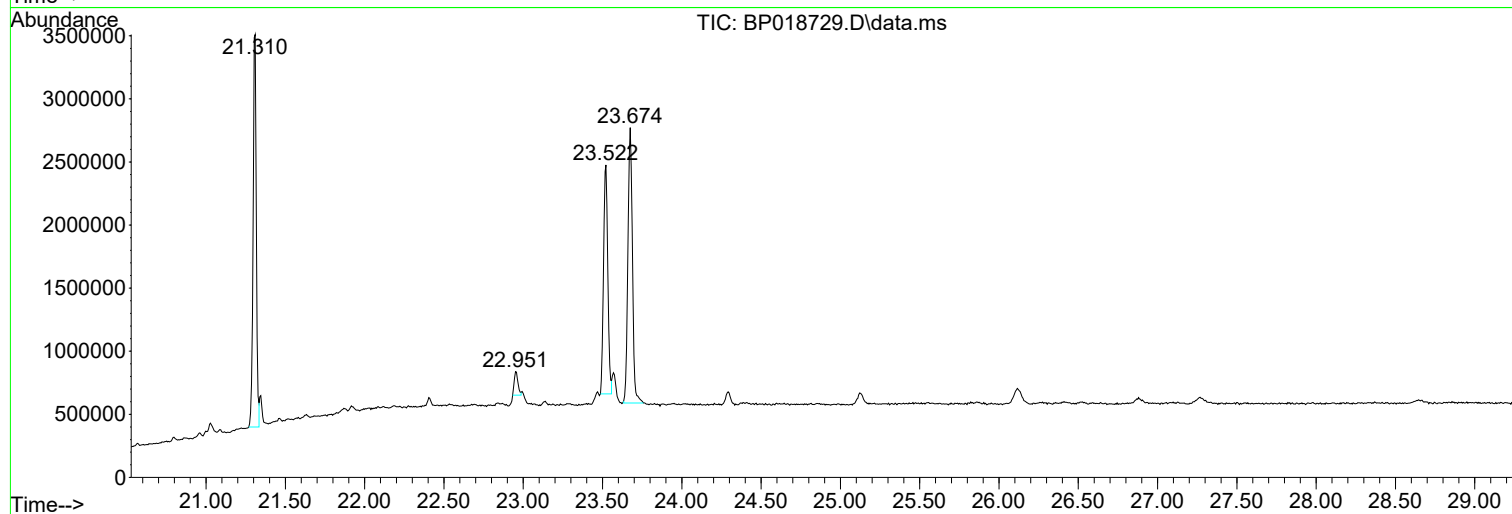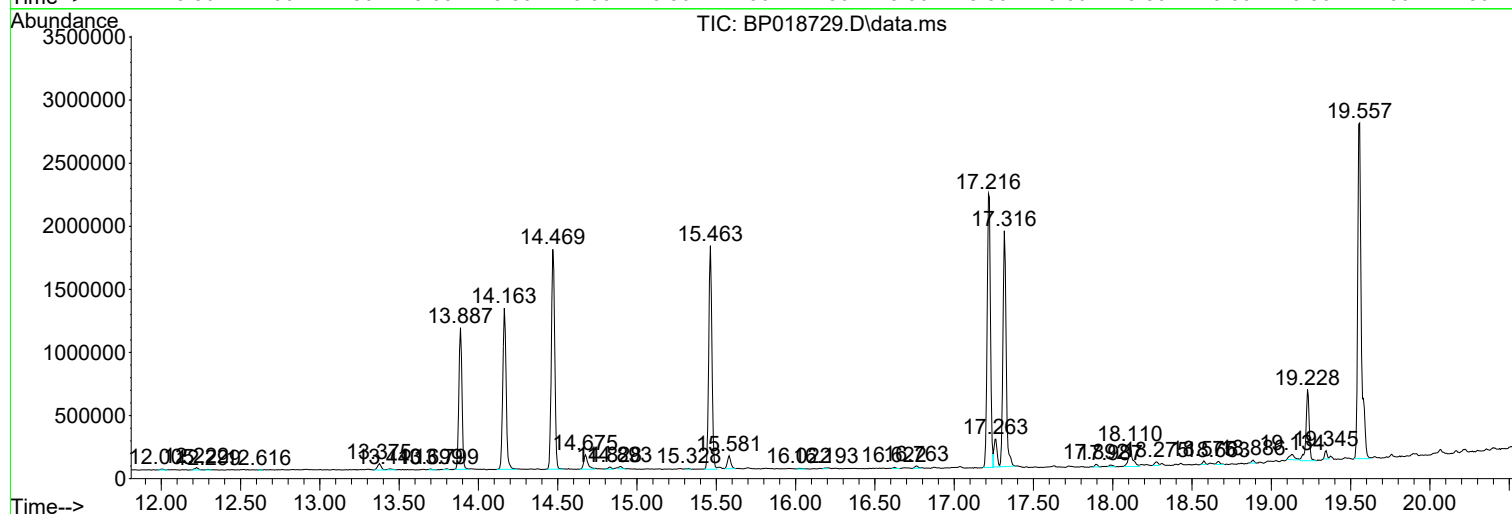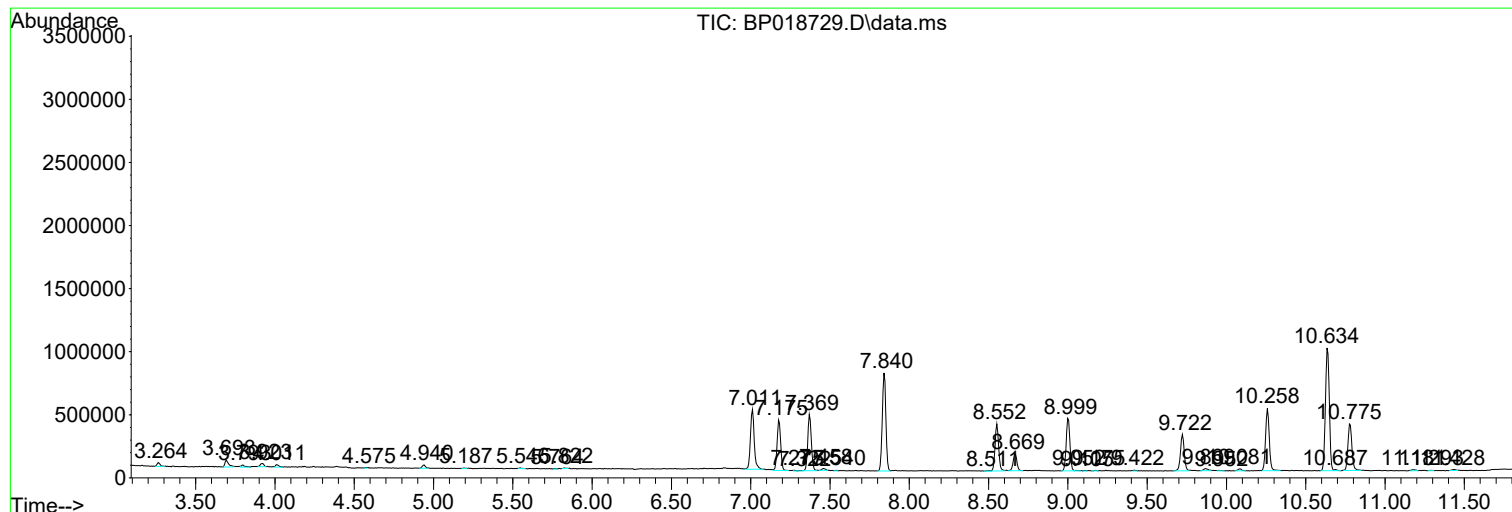

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018729.D
Acq On : 11 Dec 2023 16:20
Operator : MA/JU
Sample : 05459-21
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018729.D
Acq On : 11 Dec 2023 16:20
Operator : MA/JU
Sample : 05459-21
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc