

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018730.D
 Acq On : 11 Dec 2023 17:01
 Operator : MA/JU
 Sample : 05459-18
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018730.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	27	29	36	rVB2	16336	22602	0.61%	0.075%
2	3.687	98	102	114	rBV	55074	86212	2.34%	0.288%
3	3.911	136	140	145	rVB2	25674	35502	0.96%	0.118%
4	4.005	153	156	164	rBV2	15945	25412	0.69%	0.085%
5	4.387	219	221	227	rVB6	8635	10499	0.28%	0.035%
6	4.522	240	244	248	rBV2	4045	7093	0.19%	0.024%
7	4.934	310	314	318	rVB	24422	32785	0.89%	0.109%
8	5.816	463	464	466	rBV2	4966	4259	0.12%	0.014%
9	5.934	482	484	489	rVB5	3700	4498	0.12%	0.015%
10	6.052	502	504	507	rBV4	4199	4386	0.12%	0.015%
11	6.393	560	562	566	rBV	3167	5079	0.14%	0.017%
12	7.005	658	666	679	rVB	275980	479118	12.99%	1.599%
13	7.175	687	695	705	rBV	271909	433533	11.76%	1.447%
14	7.363	720	727	738	rVB	291497	474626	12.87%	1.584%
15	7.452	738	742	747	rBV3	19332	35258	0.96%	0.118%
16	7.646	774	775	779	rBV4	4581	4060	0.11%	0.014%
17	7.834	800	807	816	rBV	821907	1298686	35.22%	4.335%
18	7.987	832	833	837	rVB2	3166	3838	0.10%	0.013%
19	8.058	843	845	848	rVB3	5567	6090	0.17%	0.020%
20	8.099	848	852	854	rBV4	4900	8544	0.23%	0.029%
21	8.293	883	885	889	rVB3	4167	4740	0.13%	0.016%
22	8.328	889	891	894	rVB2	3717	4337	0.12%	0.014%
23	8.363	894	897	899	rBV	5096	5972	0.16%	0.020%
24	8.546	920	928	935	rBV	218623	368019	9.98%	1.228%
25	8.663	941	948	958	rVB	149276	244554	6.63%	0.816%
26	8.787	967	969	979	rVB4	11141	25433	0.69%	0.085%
27	8.999	998	1005	1011	rBV	275513	446775	12.12%	1.491%
28	9.240	1041	1046	1048	rBV2	4872	6257	0.17%	0.021%
29	9.416	1074	1076	1085	rVB4	6775	9541	0.26%	0.032%
30	9.675	1114	1120	1121	rBV2	6192	9173	0.25%	0.031%
31	9.716	1121	1127	1136	rVB	183829	309739	8.40%	1.034%
32	9.869	1146	1153	1162	rVB2	24381	54972	1.49%	0.183%
33	9.952	1164	1167	1169	rVB	12184	12750	0.35%	0.043%
34	10.004	1172	1176	1177	rBV2	3990	3965	0.11%	0.013%
35	10.040	1177	1182	1183	rBV5	2879	4130	0.11%	0.014%
36	10.081	1183	1189	1196	rBV2	20216	47128	1.28%	0.157%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018730.D
 Acq On : 11 Dec 2023 17:01
 Operator : MA/JU
 Sample : 05459-18
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	10.257	1212	1219	1228	rBV	324662	539398	14.63%	1.800%
38	10.634	1276	1283	1290	rBV	1027868	1717308	46.57%	5.732%
39	10.775	1297	1307	1319	rBV	262654	474619	12.87%	1.584%
40	10.910	1327	1330	1333	rBV3	2652	4046	0.11%	0.014%
41	11.175	1368	1375	1380	rBV10	9246	19829	0.54%	0.066%
42	11.346	1402	1404	1408	rVB3	3750	4369	0.12%	0.015%
43	11.434	1414	1419	1422	rBV3	8763	13738	0.37%	0.046%
44	11.657	1454	1457	1458	rBV3	4704	5447	0.15%	0.018%
45	11.675	1458	1460	1463	rVB4	4612	5534	0.15%	0.018%
46	12.004	1512	1516	1520	rBV7	4845	8865	0.24%	0.030%
47	12.063	1523	1526	1532	rVB8	4746	7543	0.20%	0.025%
48	12.222	1545	1553	1560	rBV2	14353	28656	0.78%	0.096%
49	12.298	1561	1566	1569	rBV3	8951	12821	0.35%	0.043%
50	12.510	1599	1602	1610	rVB4	6222	11776	0.32%	0.039%
51	12.604	1613	1618	1620	rBV4	3131	4258	0.12%	0.014%
52	12.751	1639	1643	1644	rBV	3635	4808	0.13%	0.016%
53	12.922	1666	1672	1676	rBV6	6041	9967	0.27%	0.033%
54	13.087	1698	1700	1702	rBV2	5031	4702	0.13%	0.016%
55	13.304	1734	1737	1739	rBV4	4196	5001	0.14%	0.017%
56	13.375	1742	1749	1754	rBV2	32579	54538	1.48%	0.182%
57	13.634	1790	1793	1797	rBV2	5171	10951	0.30%	0.037%
58	13.693	1801	1803	1806	rVB3	4339	4268	0.12%	0.014%
59	13.793	1815	1820	1821	rBV2	6171	9591	0.26%	0.032%
60	13.887	1830	1836	1844	rBV	651585	863835	23.43%	2.883%
61	14.028	1858	1860	1864	rVB2	6084	8328	0.23%	0.028%
62	14.163	1876	1883	1894	rBV	697412	1026371	27.83%	3.426%
63	14.369	1914	1918	1924	rVB5	7271	13269	0.36%	0.044%
64	14.469	1926	1935	1944	rBV	1520372	2279715	61.82%	7.609%
65	14.675	1964	1970	1979	rBV	117944	217613	5.90%	0.726%
66	14.834	1993	1997	2001	rBV4	9405	17263	0.47%	0.058%
67	14.892	2003	2007	2013	rVB5	17760	28138	0.76%	0.094%
68	14.998	2024	2025	2032	rBV	2754	5825	0.16%	0.019%
69	15.092	2038	2041	2044	rBV3	3267	3989	0.11%	0.013%
70	15.463	2098	2104	2115	rBV	1033797	1434164	38.89%	4.787%
71	15.581	2119	2124	2132	rVV	117673	172574	4.68%	0.576%
72	15.869	2169	2173	2176	rVB2	10355	13880	0.38%	0.046%
73	16.022	2195	2199	2202	rBV6	3908	7282	0.20%	0.024%
74	16.045	2202	2203	2209	rVB5	4695	4693	0.13%	0.016%
75	16.192	2226	2228	2230	rBV3	4276	5025	0.14%	0.017%
76	16.210	2230	2231	2235	rVB2	6168	5854	0.16%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018730.D
 Acq On : 11 Dec 2023 17:01
 Operator : MA/JU
 Sample : 05459-18
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

77	16.481	2275	2277	2280	rBV	4686	5881	0.16%	0.020%
78	16.604	2290	2298	2299	rBV2	6328	14441	0.39%	0.048%
79	16.639	2300	2304	2305	rBV	7346	7905	0.21%	0.026%
80	16.704	2313	2315	2319	rVB2	6174	6900	0.19%	0.023%
81	16.763	2320	2325	2330	rBV7	7460	13804	0.37%	0.046%
82	16.986	2361	2363	2365	rBV3	6286	5341	0.14%	0.018%
83	17.222	2396	2403	2408	rBV	1999406	2898995	78.62%	9.676%
84	17.263	2408	2410	2414	rVV	50895	62842	1.70%	0.210%
85	17.316	2414	2419	2431	rVV	997234	1516389	41.12%	5.061%
86	17.422	2433	2437	2443	rVB6	15896	27746	0.75%	0.093%
87	17.510	2450	2452	2456	rBV4	4487	6047	0.16%	0.020%
88	17.728	2486	2489	2494	rVB7	9642	13313	0.36%	0.044%
89	17.898	2515	2518	2522	rVB4	13599	17152	0.47%	0.057%
90	17.986	2531	2533	2540	rVB4	12191	18328	0.50%	0.061%
91	18.110	2547	2554	2564	rBV2	114334	193537	5.25%	0.646%
92	18.669	2646	2649	2652	rVB2	18914	22047	0.60%	0.074%
93	18.886	2683	2686	2691	rVB	22063	25297	0.69%	0.084%
94	19.204	2737	2740	2741	rBV2	21346	22611	0.61%	0.075%
95	19.233	2742	2745	2749	rVB	69176	77993	2.12%	0.260%
96	19.345	2761	2764	2768	rBV3	42513	52619	1.43%	0.176%
97	19.557	2795	2800	2814	rBV	1615155	2149544	58.29%	7.175%
98	21.310	3093	3098	3108	rBV	2837786	3682459	99.87%	12.291%
99	23.527	3469	3475	3481	rBV	963075	1821619	49.40%	6.080%
100	23.680	3495	3501	3514	rVB	1882534	3687430	100.00%	12.308%




Sum of corrected areas: 29959656

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018730.D
Acq On : 11 Dec 2023 17:01
Operator : MA/JU
Sample : 05459-18
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

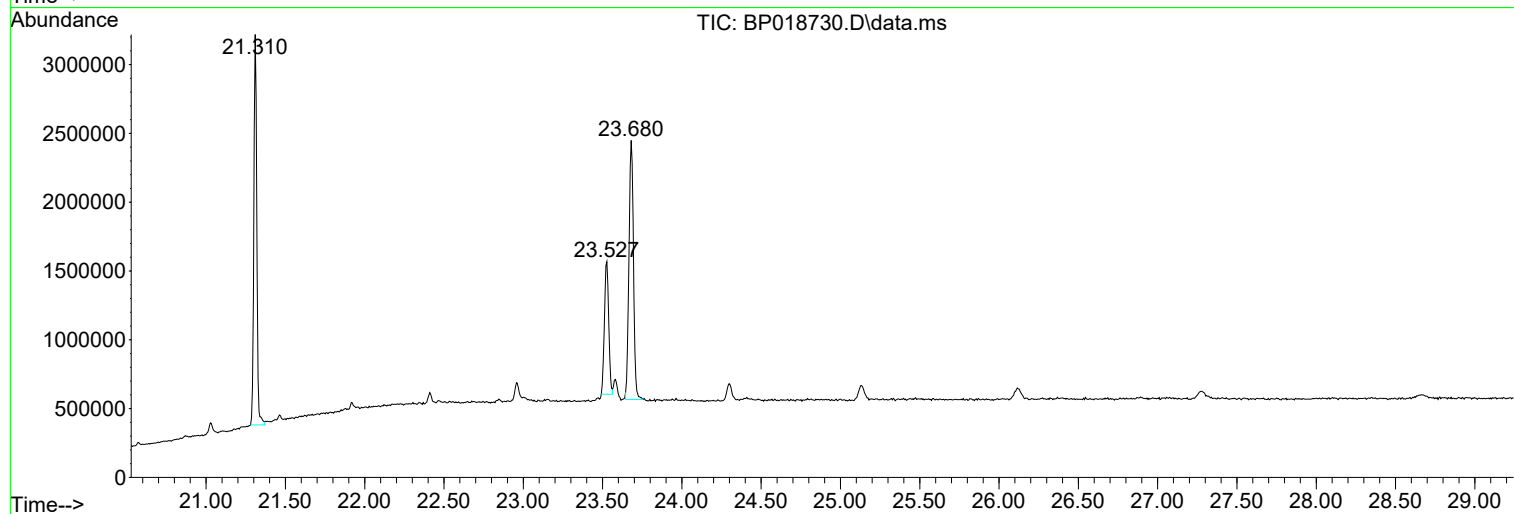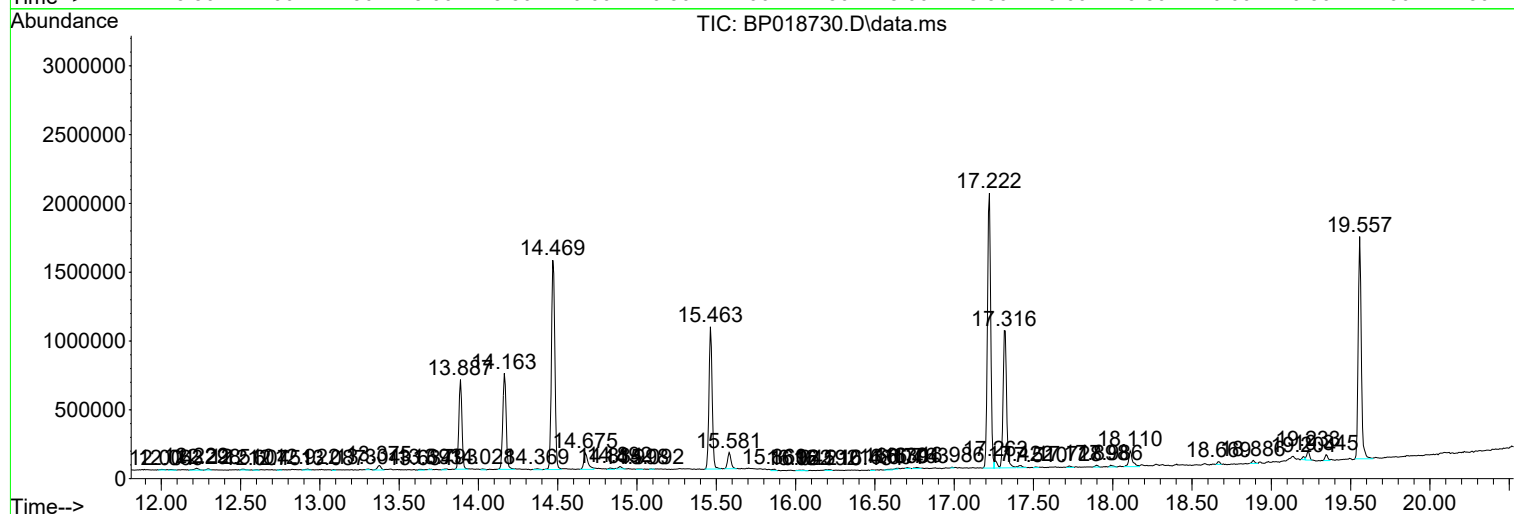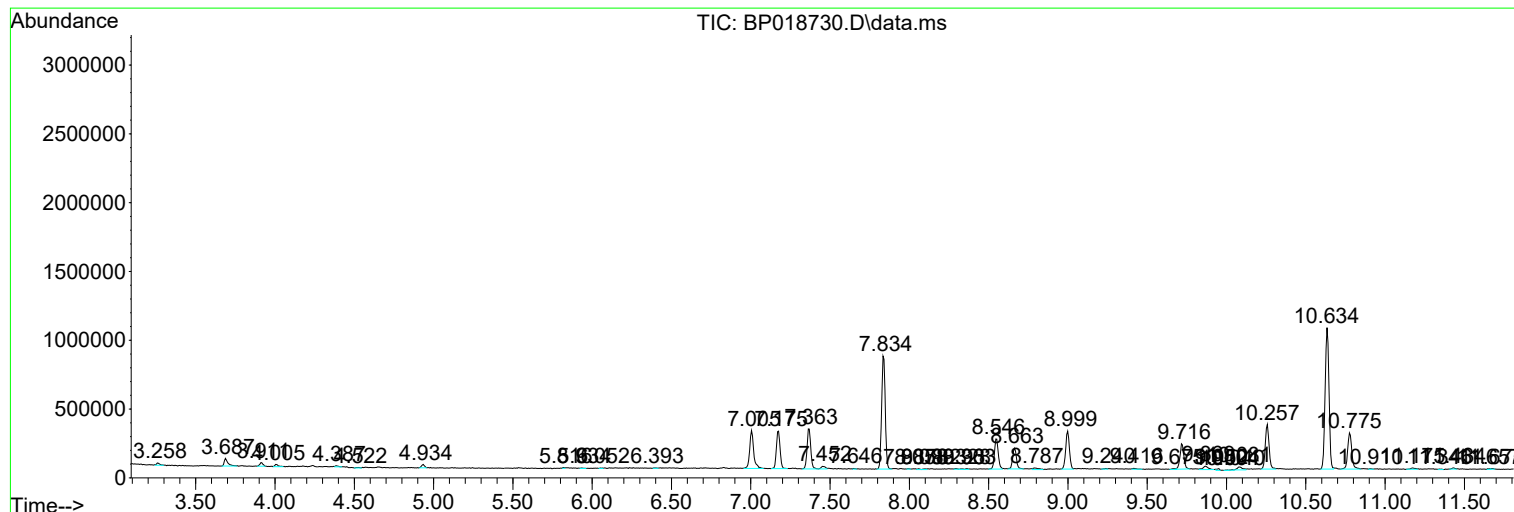

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018730.D
Acq On : 11 Dec 2023 17:01
Operator : MA/JU
Sample : 05459-18
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018730.D
Acq On : 11 Dec 2023 17:01
Operator : MA/JU
Sample : 05459-18
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc