

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018734.D
 Acq On : 11 Dec 2023 19:25
 Operator : MA/JU
 Sample : PB157621BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK621

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018734.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	37	rVB	74048	95538	1.64%	0.179%
2	3.681	97	101	118	rBV	823552	1233858	21.19%	2.316%
3	4.011	154	157	162	rVB2	15031	21370	0.37%	0.040%
4	7.011	660	667	681	rVB	892783	1399625	24.04%	2.627%
5	7.175	689	695	703	rBV	763354	1176292	20.20%	2.208%
6	7.369	719	728	736	rBV	916510	1444102	24.80%	2.711%
7	7.840	801	808	816	rVB	714801	1082939	18.60%	2.033%
8	8.552	922	929	941	rBV	1085251	1715106	29.46%	3.220%
9	8.999	998	1005	1015	rBV	805028	1299719	22.32%	2.440%
10	9.552	1097	1099	1103	rVB4	5111	5926	0.10%	0.011%
11	9.634	1107	1113	1117	rBV2	3281	6949	0.12%	0.013%
12	9.722	1121	1128	1139	rBV	590459	965572	16.59%	1.813%
13	10.257	1212	1219	1233	rBV	1031679	1708343	29.34%	3.207%
14	10.634	1276	1283	1295	rVB	874734	1465946	25.18%	2.752%
15	10.775	1300	1307	1319	rBV	1042966	1731371	29.74%	3.250%
16	12.222	1548	1553	1561	rVB4	15752	27675	0.48%	0.052%
17	12.551	1601	1609	1610	rBV4	4737	9270	0.16%	0.017%
18	13.375	1745	1749	1754	rVB4	15960	25875	0.44%	0.049%
19	13.887	1829	1836	1847	rBV	1817782	2505255	43.03%	4.703%
20	14.163	1876	1883	1895	rBV	2095762	3011238	51.72%	5.653%
21	14.469	1928	1935	1944	rBV	1352821	1943419	33.38%	3.648%
22	14.669	1962	1969	1990	rBV	686776	1164422	20.00%	2.186%
23	15.463	2097	2104	2118	rBV	2793976	3912021	67.19%	7.344%
24	15.581	2118	2124	2133	rBV	633873	870056	14.94%	1.633%
25	15.698	2142	2144	2150	rVB3	13403	17636	0.30%	0.033%
26	16.245	2235	2237	2242	rVB5	4917	5945	0.10%	0.011%
27	16.904	2344	2349	2353	rBV8	5393	9843	0.17%	0.018%
28	17.216	2395	2402	2413	rBV	1721438	2461839	42.29%	4.622%
29	17.316	2413	2419	2435	rVV2	3096738	4363469	74.95%	8.191%
30	19.128	2724	2727	2733	rVB3	39514	56713	0.97%	0.106%
31	19.198	2735	2739	2747	rBV3	40101	63107	1.08%	0.118%
32	19.557	2794	2800	2806	rBV	4145752	5467334	93.91%	10.264%
33	21.304	3093	3097	3104	rBV	2377287	2941746	50.53%	5.522%
34	23.521	3467	3474	3481	rBV2	2962679	5821901	100.00%	10.929%
35	23.674	3493	3500	3511	rVB	1647070	3237623	55.61%	6.078%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018734.D
Acq On : 11 Dec 2023 19:25
Operator : MA/JU
Sample : PB157621BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK621

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 53269043

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018734.D
Acq On : 11 Dec 2023 19:25
Operator : MA/JU
Sample : PB157621BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK621

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

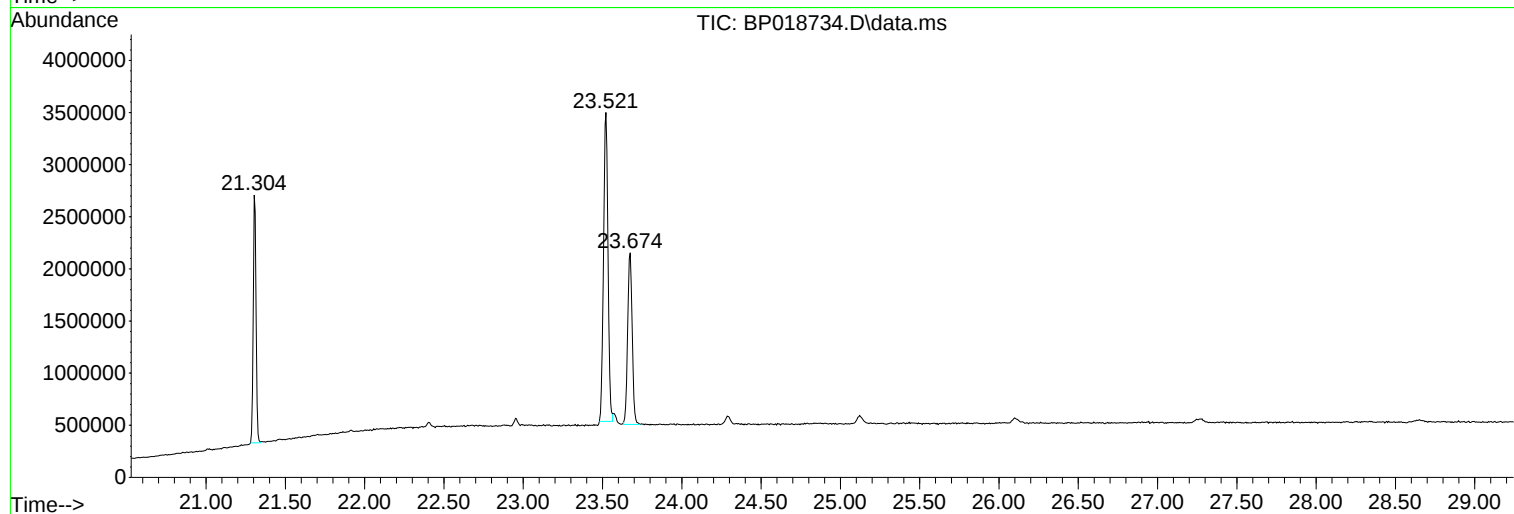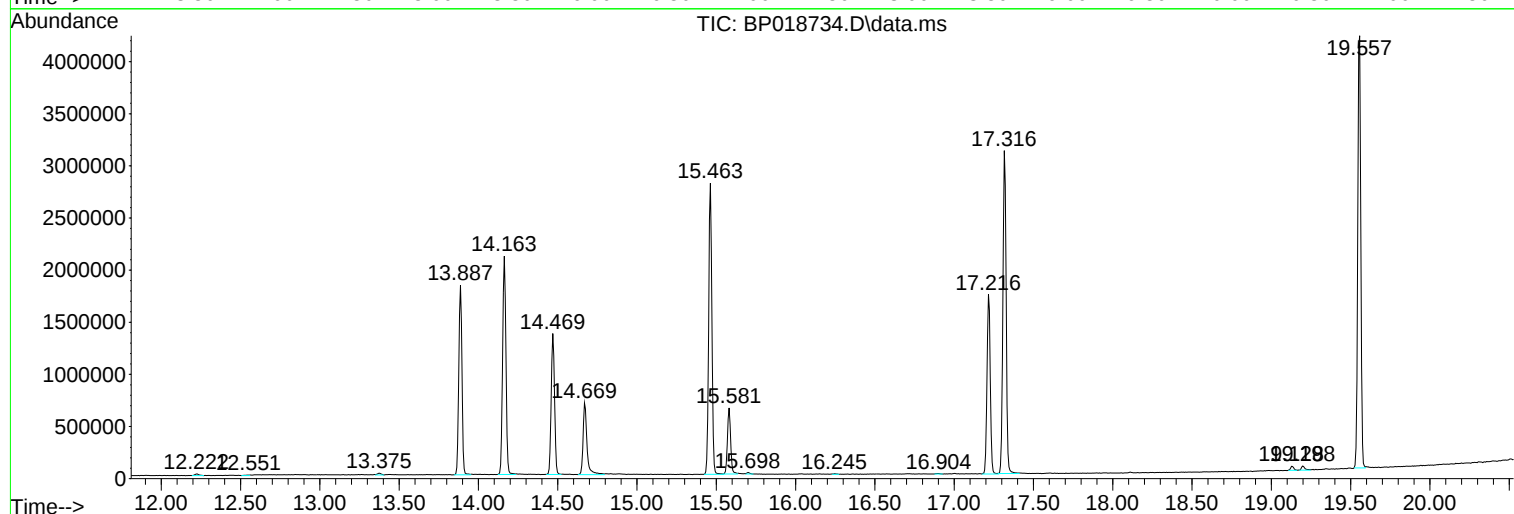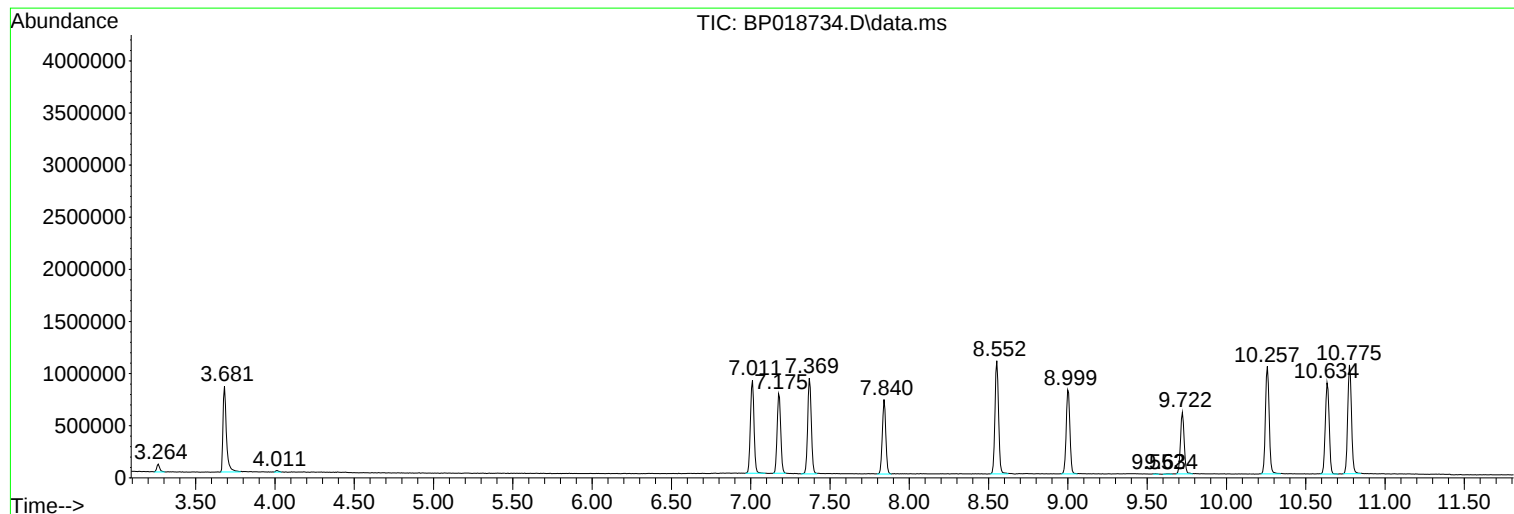

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018734.D
Acq On : 11 Dec 2023 19:25
Operator : MA/JU
Sample : PB157621BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK621

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018734.D
Acq On : 11 Dec 2023 19:25
Operator : MA/JU
Sample : PB157621BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK621

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc