

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018754.D
 Acq On : 12 Dec 2023 07:16
 Operator : MA/JU
 Sample : PB157623BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK623

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018754.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	35	rBV	54236	65384	1.28%	0.145%
2	3.681	97	101	112	rBV	611351	921309	18.00%	2.044%
3	4.011	154	157	162	rVB2	10547	15687	0.31%	0.035%
4	4.240	194	196	201	rVB6	5861	8043	0.16%	0.018%
5	7.011	660	667	677	rVB	709157	1088161	21.26%	2.414%
6	7.175	689	695	703	rBV	554378	849632	16.60%	1.885%
7	7.369	720	728	741	rVB	737665	1130956	22.10%	2.509%
8	7.840	801	808	816	rBV	653129	987935	19.31%	2.192%
9	8.552	922	929	940	rBV	851966	1340797	26.20%	2.974%
10	8.999	998	1005	1013	rBV	645705	1042444	20.37%	2.313%
11	9.722	1118	1128	1138	rBV	530602	856955	16.75%	1.901%
12	10.258	1209	1219	1231	rBV	848279	1418581	27.72%	3.147%
13	10.634	1275	1283	1293	rVB	795998	1307707	25.56%	2.901%
14	10.775	1299	1307	1320	rBV	823678	1359290	26.56%	3.015%
15	12.222	1545	1553	1558	rBV2	15440	27960	0.55%	0.062%
16	13.375	1742	1749	1754	rBV2	17557	30582	0.60%	0.068%
17	13.887	1827	1836	1845	rBV	1514849	2074334	40.54%	4.602%
18	14.163	1876	1883	1897	rBV	1631849	2405125	47.00%	5.336%
19	14.469	1928	1935	1942	rBV	1242645	1792407	35.03%	3.976%
20	14.669	1962	1969	1987	rBV	629849	1009521	19.73%	2.240%
21	15.463	2097	2104	2114	rBV	2084910	3079897	60.19%	6.832%
22	15.581	2117	2124	2134	rBV	607576	829736	16.21%	1.841%
23	15.698	2140	2144	2152	rVB4	11595	22244	0.43%	0.049%
24	16.240	2231	2236	2243	rVB4	4440	8882	0.17%	0.020%
25	16.892	2343	2347	2352	rVB7	3777	6376	0.12%	0.014%
26	17.004	2361	2366	2372	rBV6	3623	8045	0.16%	0.018%
27	17.098	2378	2382	2387	rBV7	4671	7960	0.16%	0.018%
28	17.216	2395	2402	2412	rBV	1629562	2294241	44.83%	5.090%
29	17.316	2412	2419	2429	rBV	2382624	3325952	65.00%	7.378%
30	18.110	2550	2554	2556	rBV4	5910	7407	0.14%	0.016%
31	18.428	2604	2608	2613	rBV5	13187	21424	0.42%	0.048%
32	18.981	2698	2702	2708	rBV8	10118	20009	0.39%	0.044%
33	19.128	2723	2727	2734	rBV	36608	53256	1.04%	0.118%
34	19.198	2735	2739	2744	rVB	32938	45731	0.89%	0.101%
35	19.551	2793	2799	2806	rBV	3238074	4363302	85.27%	9.680%
36	21.304	3092	3097	3103	rBV	2314243	2896637	56.61%	6.426%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018754.D
Acq On : 12 Dec 2023 07:16
Operator : MA/JU
Sample : PB157623BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK623

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	23.516	3466	3473	3489	rVB2	2515042	5117218	100.00%	11.352%
38	23.669	3493	3499	3510	rVB	1634352	3236293	63.24%	7.179%




Sum of corrected areas: 45077420

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018754.D
Acq On : 12 Dec 2023 07:16
Operator : MA/JU
Sample : PB157623BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK623

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

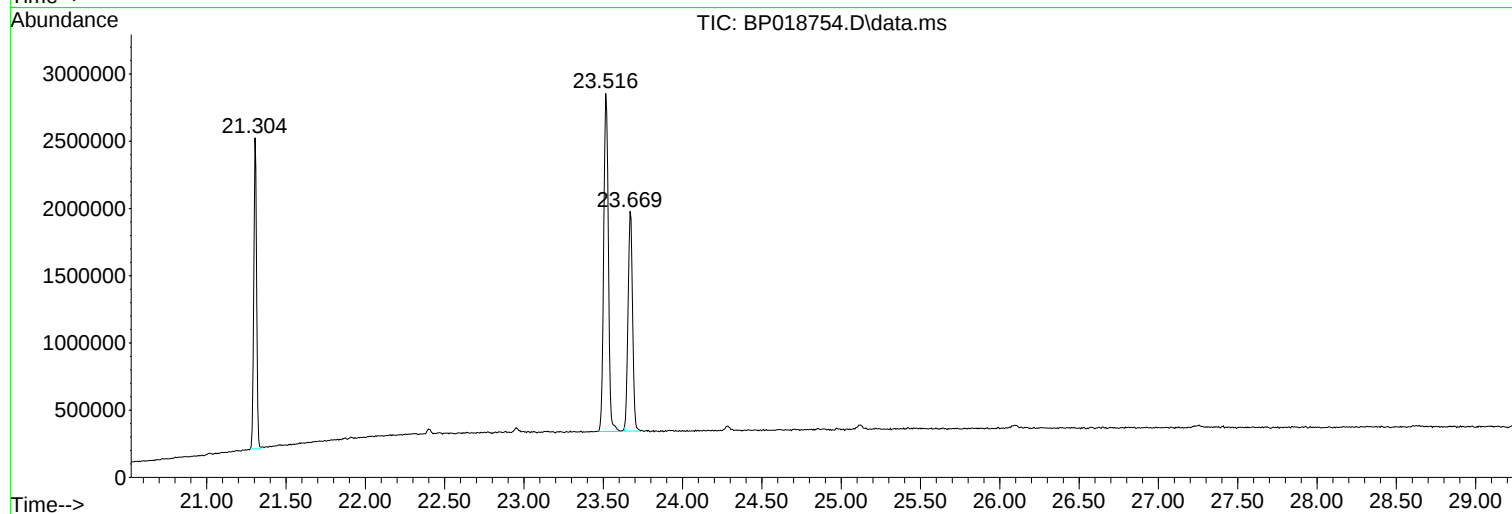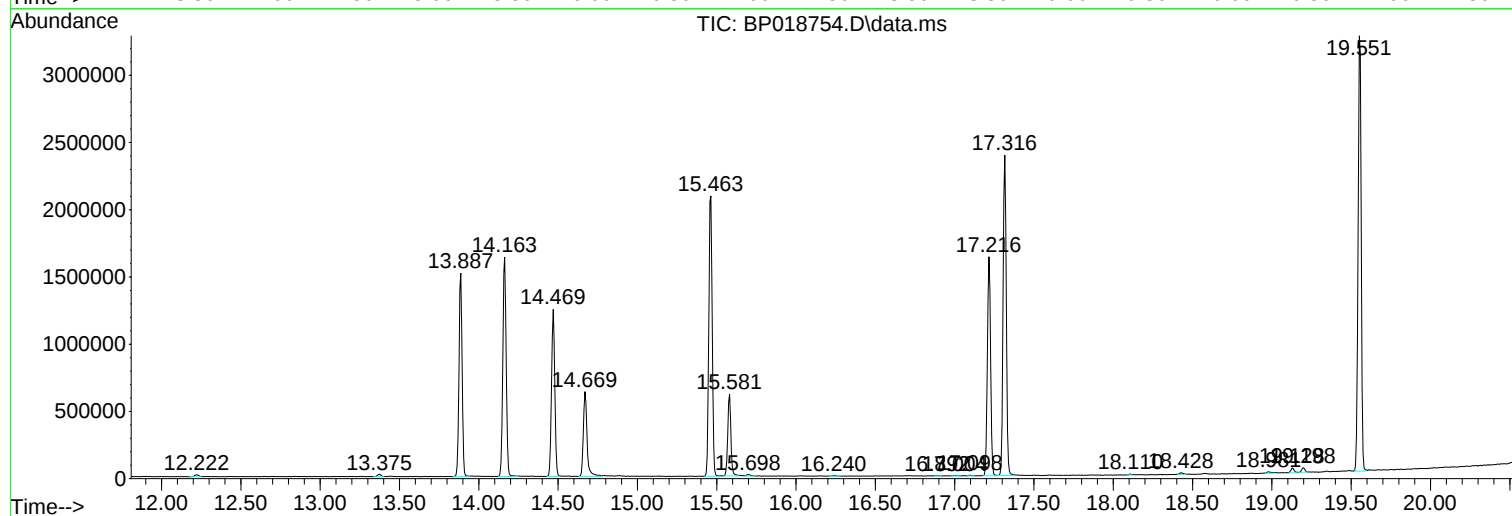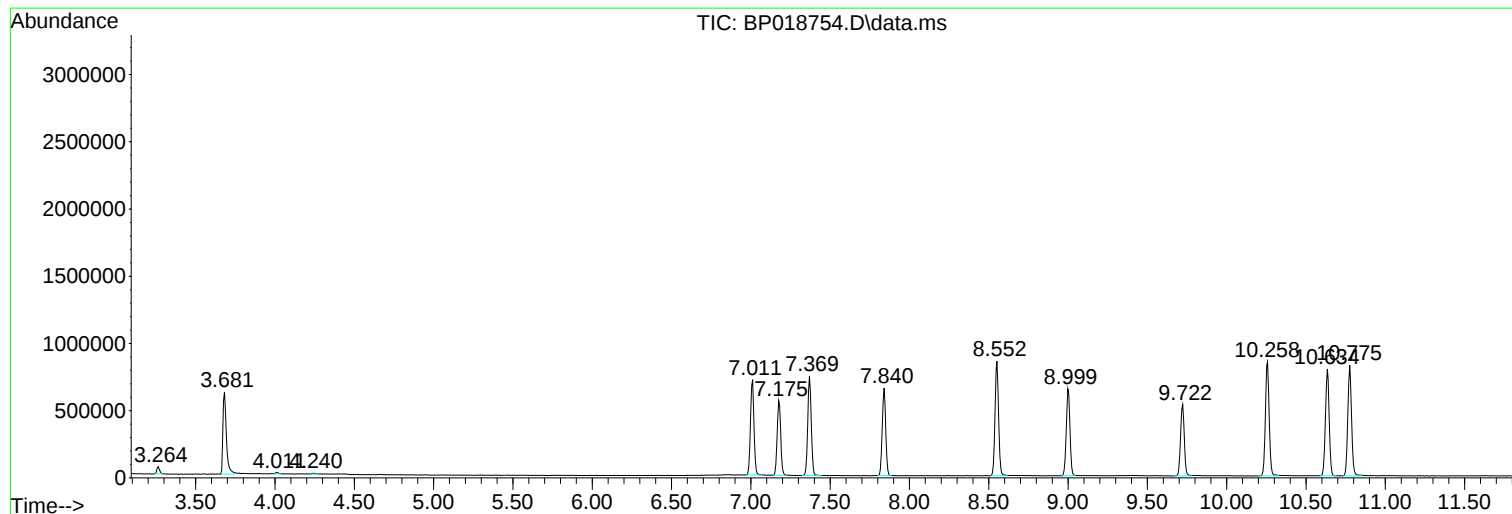

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018754.D
Acq On : 12 Dec 2023 07:16
Operator : MA/JU
Sample : PB157623BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK623

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018754.D
Acq On : 12 Dec 2023 07:16
Operator : MA/JU
Sample : PB157623BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK623

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc