

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018755.D
 Acq On : 12 Dec 2023 07:50
 Operator : MA/JU
 Sample : 05675-05
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018755.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	26	30	38	rVB	38300	52029	0.89%	0.119%
2	3.687	98	102	117	rBV	175465	283421	4.83%	0.648%
3	3.916	138	141	147	rVB2	12481	18008	0.31%	0.041%
4	4.016	153	158	165	rBV3	12893	23973	0.41%	0.055%
5	7.010	661	667	677	rVB	124665	202284	3.45%	0.463%
6	7.175	689	695	708	rVB	534836	826623	14.08%	1.890%
7	7.369	722	728	737	rBV	533383	811483	13.82%	1.856%
8	7.463	740	744	751	rVB9	4826	8341	0.14%	0.019%
9	7.840	801	808	817	rBV	610067	951058	16.20%	2.175%
10	8.551	921	929	938	rBV	350555	554869	9.45%	1.269%
11	8.998	996	1005	1014	rBV	639696	1025347	17.46%	2.345%
12	9.116	1021	1025	1030	rBV4	6382	9822	0.17%	0.022%
13	9.416	1073	1076	1082	rVB6	5002	9044	0.15%	0.021%
14	9.722	1120	1128	1141	rBV	493916	799362	13.61%	1.828%
15	10.257	1210	1219	1229	rBV	761703	1239612	21.11%	2.835%
16	10.634	1276	1283	1291	rBV	765280	1240557	21.13%	2.837%
17	10.775	1299	1307	1317	rBV	691820	1165017	19.84%	2.664%
18	12.045	1516	1523	1532	rVB9	8556	20417	0.35%	0.047%
19	12.222	1549	1553	1560	rVB3	14170	23712	0.40%	0.054%
20	13.298	1732	1736	1742	rVB6	6881	9240	0.16%	0.021%
21	13.375	1742	1749	1755	rVV2	14902	24116	0.41%	0.055%
22	13.439	1755	1760	1767	rVB9	3486	6600	0.11%	0.015%
23	13.886	1827	1836	1850	rBV	1589616	2173360	37.01%	4.970%
24	14.163	1874	1883	1893	rBV	1678149	2440527	41.57%	5.581%
25	14.263	1897	1900	1905	rVB6	4592	8328	0.14%	0.019%
26	14.469	1928	1935	1944	rBV	1184638	1724837	29.38%	3.944%
27	14.669	1964	1969	1978	rBV	95976	181493	3.09%	0.415%
28	14.757	1981	1984	1987	rVB4	6545	8136	0.14%	0.019%
29	14.886	2002	2006	2012	rVB7	8491	15972	0.27%	0.037%
30	15.463	2097	2104	2112	rBV	2286893	3305070	56.29%	7.558%
31	15.580	2117	2124	2138	rVV	683597	935180	15.93%	2.138%
32	15.698	2140	2144	2158	rVB5	13115	25538	0.43%	0.058%
33	16.622	2297	2301	2306	rBV8	5319	7812	0.13%	0.018%
34	16.763	2319	2325	2331	rBV9	7761	15361	0.26%	0.035%
35	16.892	2343	2347	2352	rVB8	3815	6875	0.12%	0.016%
36	17.216	2395	2402	2412	rBV	1627467	2263232	38.55%	5.175%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018755.D
 Acq On : 12 Dec 2023 07:50
 Operator : MA/JU
 Sample : 05675-05
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	17.316	2412	2419	2431	rVV	2748156	3754063	63.94%	8.584%
38	17.980	2529	2532	2536	rBV6	4636	7692	0.13%	0.018%
39	18.104	2549	2553	2562	rBV	119960	165981	2.83%	0.380%
40	18.427	2604	2608	2615	rVB4	11405	17103	0.29%	0.039%
41	18.574	2630	2633	2639	rVB6	13239	18900	0.32%	0.043%
42	19.127	2723	2727	2731	rBV3	42413	53310	0.91%	0.122%
43	19.198	2734	2739	2743	rBV	49652	77320	1.32%	0.177%
44	19.339	2759	2763	2769	rBV2	95469	127453	2.17%	0.291%
45	19.551	2793	2799	2808	rBV	3798071	5028806	85.65%	11.499%
46	21.304	3092	3097	3103	rBV	2479709	2952264	50.28%	6.751%
47	23.515	3466	3473	3488	rVB2	2863390	5871590	100.00%	13.426%
48	23.668	3492	3499	3508	rVB	1677766	3240808	55.19%	7.411%




Sum of corrected areas: 43731946

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018755.D
Acq On : 12 Dec 2023 07:50
Operator : MA/JU
Sample : 05675-05
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

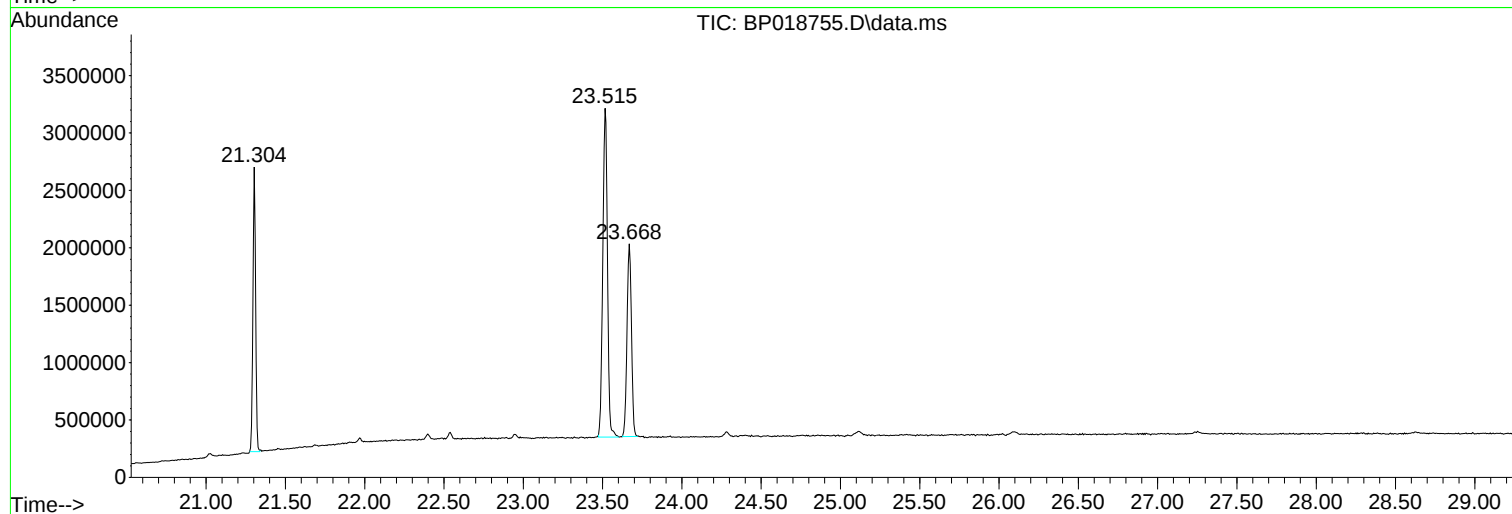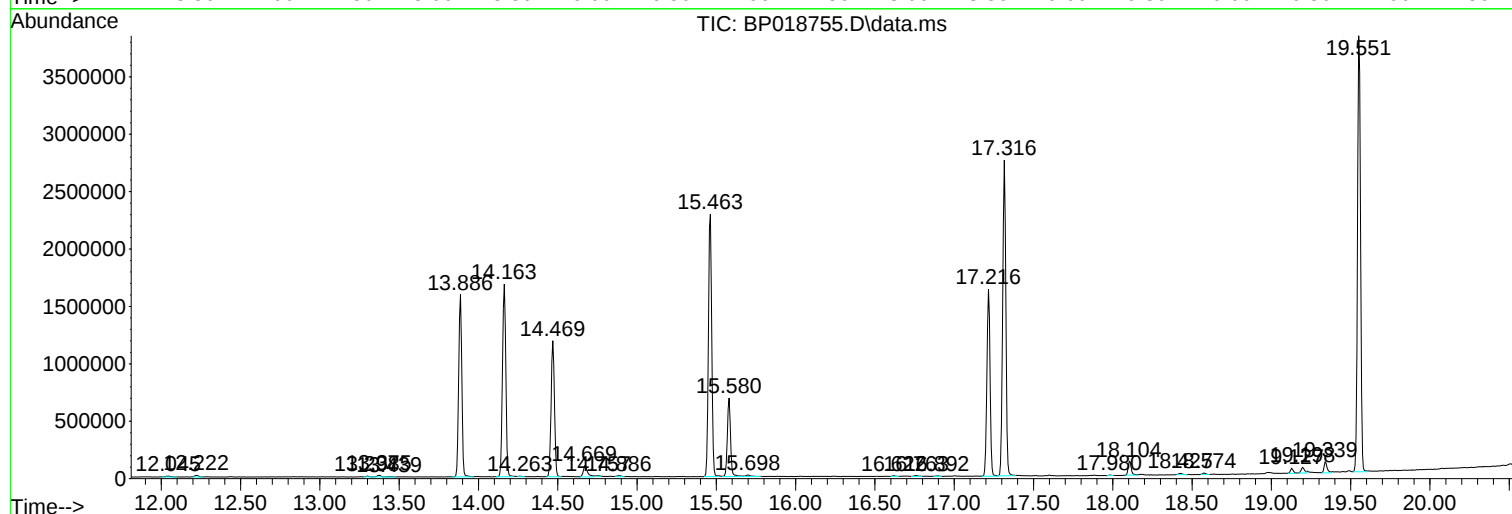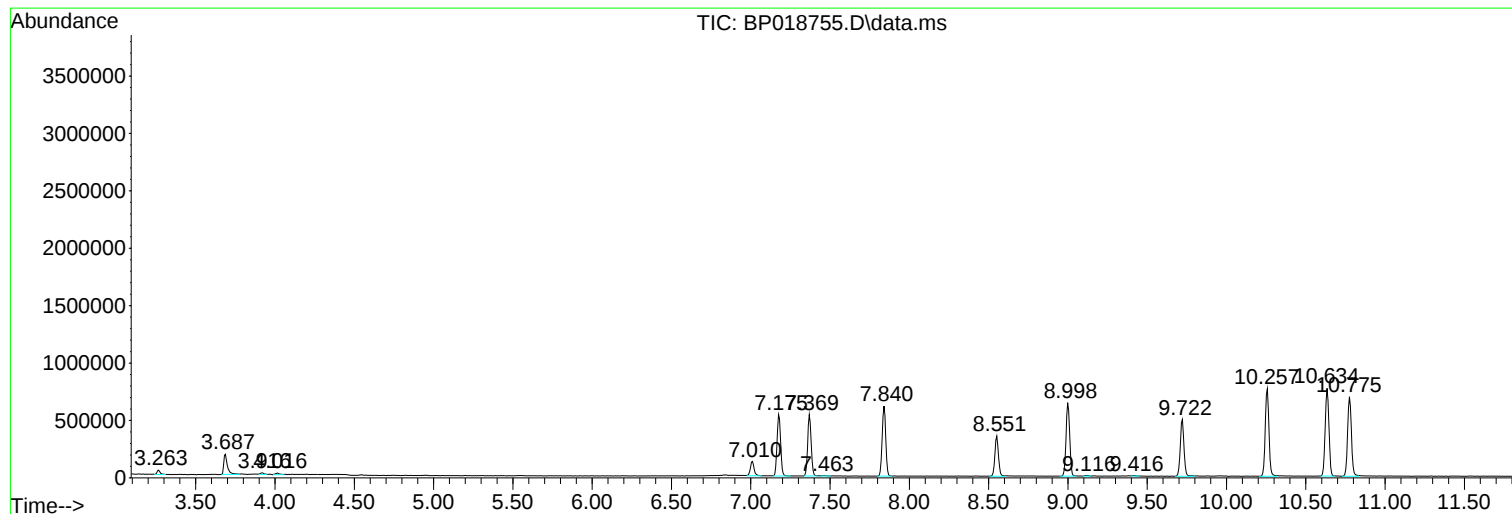

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018755.D
Acq On : 12 Dec 2023 07:50
Operator : MA/JU
Sample : 05675-05
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018755.D
Acq On : 12 Dec 2023 07:50
Operator : MA/JU
Sample : 05675-05
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc