

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018762.D
 Acq On : 12 Dec 2023 11:47
 Operator : MA/JU
 Sample : 05675-12
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AB5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018762.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	19	25	27	rBV	46314	71350	1.10%	0.141%
2	3.264	27	30	33	rVV	39428	51229	0.79%	0.102%
3	3.299	33	36	42	rVB	29372	38632	0.60%	0.077%
4	3.681	97	101	114	rBV	236958	374308	5.79%	0.742%
5	3.916	137	141	150	rVB2	13973	24917	0.39%	0.049%
6	4.011	153	157	162	rVB2	13913	18683	0.29%	0.037%
7	4.546	240	248	258	rVB	418427	646020	9.99%	1.280%
8	4.940	309	315	320	rBV7	4170	8557	0.13%	0.017%
9	7.010	660	667	675	rVB	158438	252661	3.91%	0.501%
10	7.175	688	695	704	rBV	601996	913453	14.13%	1.810%
11	7.369	721	728	738	rBV	601127	930015	14.39%	1.843%
12	7.840	801	808	818	rBV	698678	1065704	16.48%	2.112%
13	8.552	922	929	942	rBV	460671	719099	11.12%	1.425%
14	8.999	997	1005	1020	rBV	700299	1144220	17.70%	2.268%
15	9.422	1070	1077	1085	rVB10	5660	13870	0.21%	0.027%
16	9.722	1120	1128	1139	rBV	544968	883732	13.67%	1.751%
17	10.257	1211	1219	1229	rBV	836338	1374642	21.26%	2.724%
18	10.634	1274	1283	1290	rBV	852078	1414277	21.88%	2.803%
19	10.775	1299	1307	1324	rBV	734271	1258156	19.46%	2.493%
20	12.057	1517	1525	1532	rVB	6005	12921	0.20%	0.026%
21	12.222	1546	1553	1558	rVB	15301	26322	0.41%	0.052%
22	13.298	1731	1736	1744	rBV4	8068	11429	0.18%	0.023%
23	13.375	1744	1749	1755	rVB4	13627	22350	0.35%	0.044%
24	13.887	1829	1836	1842	rBV	1696627	2269005	35.10%	4.497%
25	14.004	1852	1856	1861	rVB6	7570	11972	0.19%	0.024%
26	14.163	1871	1883	1891	rBV	1767781	2613371	40.42%	5.179%
27	14.469	1928	1935	1944	rBV	1323829	1945867	30.10%	3.856%
28	14.675	1963	1970	1982	rBV	130125	246885	3.82%	0.489%
29	14.881	2001	2005	2012	rVB10	6374	13589	0.21%	0.027%
30	15.128	2042	2047	2052	rVB8	5990	8455	0.13%	0.017%
31	15.463	2097	2104	2117	rBV	2410577	3467873	53.64%	6.872%
32	15.581	2117	2124	2135	rBV	754788	1032467	15.97%	2.046%
33	15.704	2141	2145	2149	rVB3	13140	20664	0.32%	0.041%
34	16.151	2215	2221	2226	rBV8	7223	14570	0.23%	0.029%
35	16.245	2233	2237	2240	rBV6	5746	8828	0.14%	0.017%
36	16.622	2297	2301	2305	rBV6	6493	10483	0.16%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018762.D
 Acq On : 12 Dec 2023 11:47
 Operator : MA/JU
 Sample : 05675-12
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AB5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	17.216	2395	2402	2412	rBV	1845922	2525226	39.06%	5.004%
38	17.316	2412	2419	2429	rBV	3034334	4155132	64.27%	8.234%
39	17.892	2514	2517	2521	rVB6	5403	7188	0.11%	0.014%
40	18.104	2549	2553	2559	rBV	114179	154888	2.40%	0.307%
41	18.186	2562	2567	2573	rVB3	25886	41815	0.65%	0.083%
42	18.427	2604	2608	2612	rBV3	10588	16898	0.26%	0.033%
43	18.575	2630	2633	2637	rVB3	11705	15260	0.24%	0.030%
44	19.127	2723	2727	2732	rBV2	46438	64397	1.00%	0.128%
45	19.198	2735	2739	2742	rBV	51906	70614	1.09%	0.140%
46	19.286	2749	2754	2760	rBV	1245069	1386179	21.44%	2.747%
47	19.345	2760	2764	2769	rVB	84625	108075	1.67%	0.214%
48	19.551	2794	2799	2805	rBV	4296715	5559352	85.99%	11.017%
49	21.304	3092	3097	3104	rBV	2715796	3310177	51.20%	6.560%
50	23.515	3466	3473	3480	rBV2	3230248	6464981	100.00%	12.812%
51	23.668	3492	3499	3510	rVB	1841550	3639558	56.30%	7.213%




Sum of corrected areas: 50460316

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018762.D
Acq On : 12 Dec 2023 11:47
Operator : MA/JU
Sample : 05675-12
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AB5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

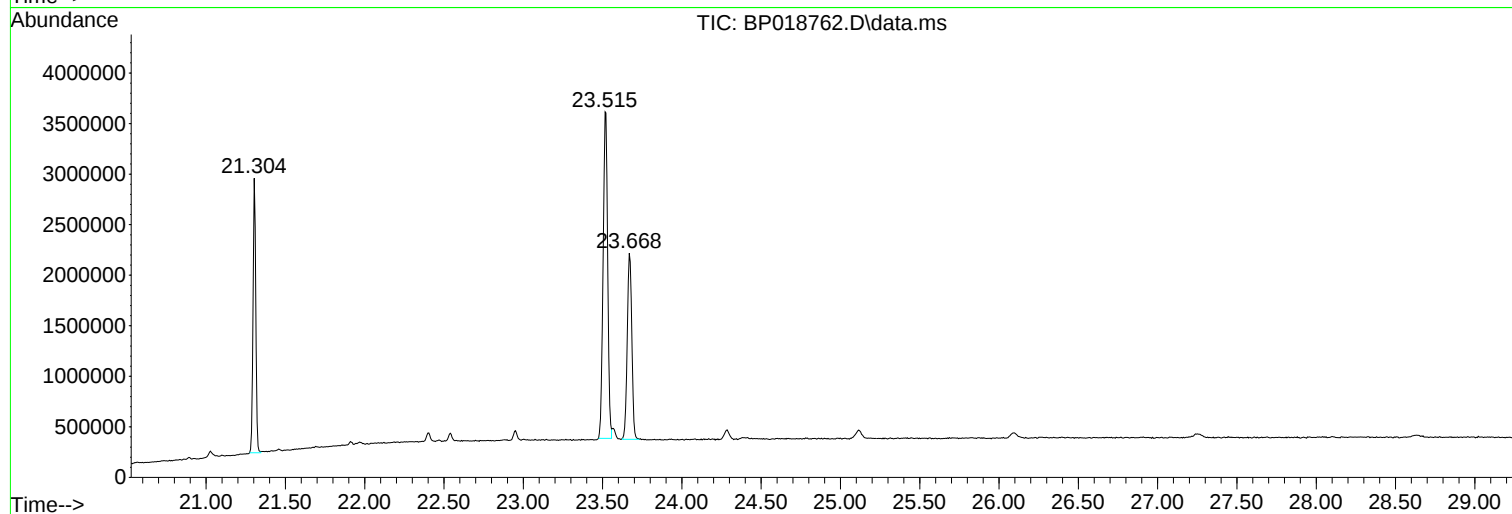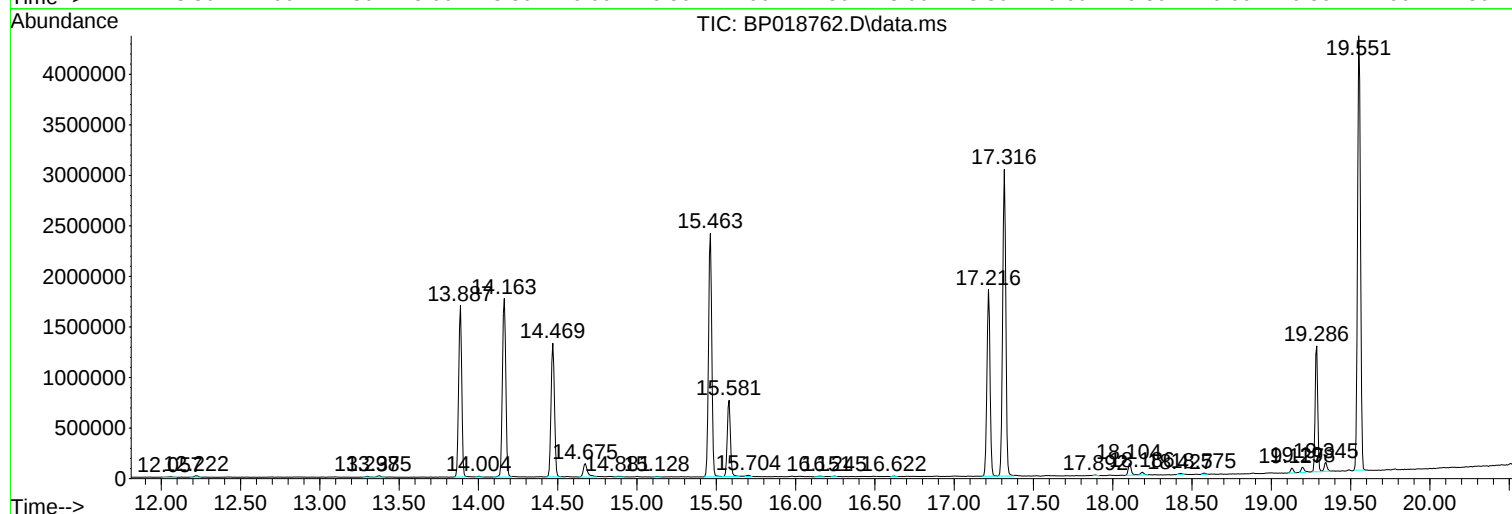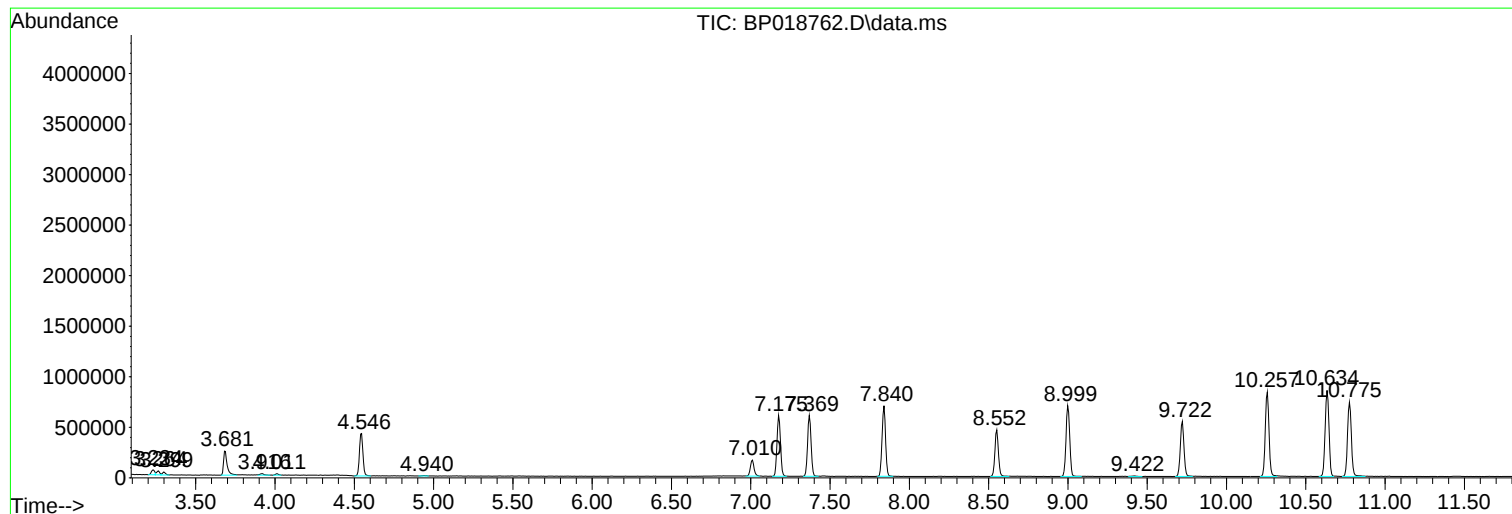

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018762.D
Acq On : 12 Dec 2023 11:47
Operator : MA/JU
Sample : 05675-12
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AB5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
19.286	8.38 ng/ul	1386180	Chrysene-d12	21.304

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-tert-Butoxy-2-ethoxyethane	146	C8H18O2	051422-54-9	38		
2	1-tert-Butoxy-2-ethoxyethane	146	C8H18O2	051422-54-9	38		
3	Butane, 1,1'-[ethylidenebis(oxy)]...	174	C10H22O2	000871-22-7	35		
4	2-[2-[2-[2-[2-[2-[2-(2-Methox...	428	C19H40O10	006048-68-6	27		
5	Propane, 1,1'-[ethylidenebis(oxy)]...	174	C10H22O2	005669-09-0	27		

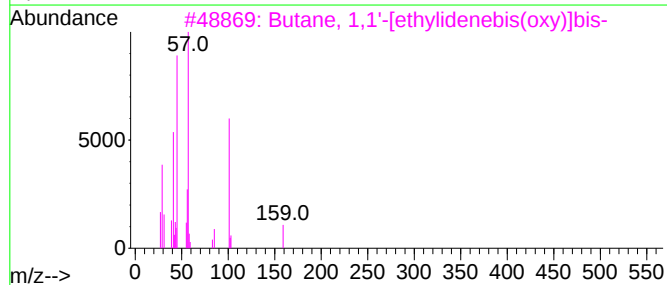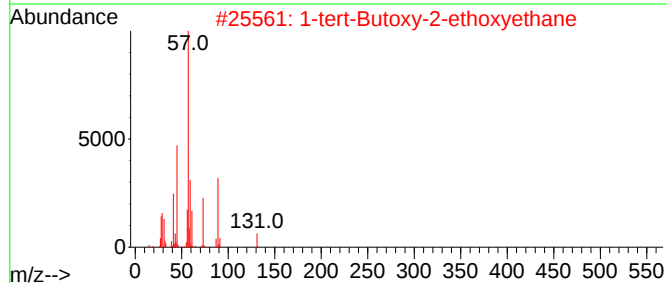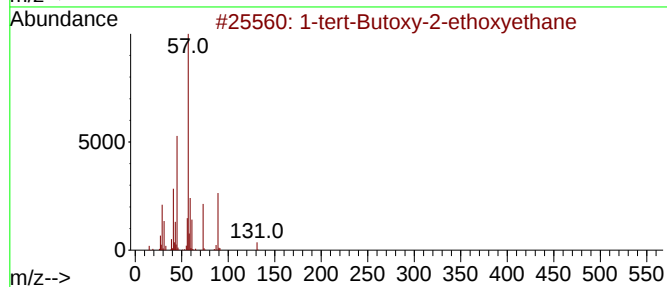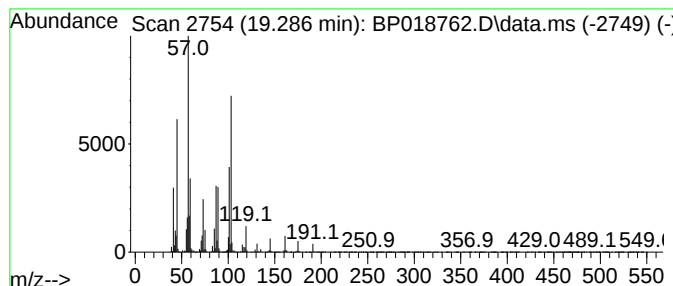

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018762.D
Acq On : 12 Dec 2023 11:47
Operator : MA/JU
Sample : 05675-12
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AB5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	19.286	8.4	ng/ul	1386180	5	21.304	3310180	20.0