

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018767.D
 Acq On : 12 Dec 2023 14:37
 Operator : MA/JU
 Sample : 05675-17
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AC0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018767.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	20	25	28	rBV	72990	116404	2.07%	0.264%
2	3.263	28	30	33	rVV	40368	47001	0.84%	0.107%
3	3.299	33	36	45	rVB	40023	55624	0.99%	0.126%
4	3.687	98	102	114	rBV	205693	326446	5.82%	0.742%
5	3.916	137	141	147	rVB2	15278	24822	0.44%	0.056%
6	4.010	154	157	161	rVB	10555	11591	0.21%	0.026%
7	4.546	241	248	257	rBV	584042	897215	15.99%	2.038%
8	4.940	310	315	318	rBV5	4154	7172	0.13%	0.016%
9	5.546	414	418	425	rVB9	3029	5638	0.10%	0.013%
10	7.010	660	667	674	rVB	140775	212159	3.78%	0.482%
11	7.175	688	695	708	rVB	572770	879157	15.66%	1.997%
12	7.369	720	728	736	rBV	544135	850125	15.15%	1.931%
13	7.469	740	745	753	rVB	3545	7373	0.13%	0.017%
14	7.840	798	808	816	rBV	626046	965292	17.20%	2.193%
15	8.551	922	929	937	rBV	388378	622147	11.09%	1.413%
16	8.998	996	1005	1012	rBV	665384	1069373	19.05%	2.429%
17	9.416	1069	1076	1083	rVB	5213	11135	0.20%	0.025%
18	9.722	1120	1128	1138	rBV	483045	805158	14.35%	1.829%
19	10.257	1211	1219	1233	rBV	742995	1267829	22.59%	2.880%
20	10.634	1275	1283	1296	rBV	760258	1257257	22.40%	2.856%
21	10.775	1298	1307	1317	rBV	713189	1178327	21.00%	2.677%
22	12.057	1522	1525	1530	rVB3	7245	10812	0.19%	0.025%
23	12.222	1545	1553	1560	rVB2	15835	27382	0.49%	0.062%
24	13.298	1732	1736	1743	rVB3	9551	14313	0.26%	0.033%
25	13.375	1744	1749	1756	rVB5	8698	16142	0.29%	0.037%
26	13.439	1756	1760	1764	rBV7	3693	6182	0.11%	0.014%
27	13.886	1828	1836	1849	rBV	1506584	2094242	37.32%	4.758%
28	14.163	1874	1883	1893	rBV	1607893	2405972	42.87%	5.466%
29	14.469	1927	1935	1942	rBV	1179578	1715036	30.56%	3.896%
30	14.675	1963	1970	1981	rBV	88792	170750	3.04%	0.388%
31	14.886	2001	2006	2013	rVB	5879	13089	0.23%	0.030%
32	15.186	2052	2057	2065	rBV7	4817	11712	0.21%	0.027%
33	15.463	2097	2104	2117	rBV	2181293	3172334	56.53%	7.207%
34	15.580	2118	2124	2136	rVV	604865	830992	14.81%	1.888%
35	15.698	2140	2144	2152	rVB2	13446	24306	0.43%	0.055%
36	16.622	2297	2301	2307	rVB9	4551	6404	0.11%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018767.D
 Acq On : 12 Dec 2023 14:37
 Operator : MA/JU
 Sample : 05675-17
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AC0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	17.216	2395	2402	2409	rBV	1591513	2245139	40.00%	5.101%
38	17.316	2412	2419	2430	rVV	2650646	3596902	64.09%	8.171%
39	17.610	2467	2469	2477	rVB9	6724	10265	0.18%	0.023%
40	18.104	2549	2553	2562	rBV	91075	124946	2.23%	0.284%
41	18.186	2563	2567	2573	rVV4	16222	25461	0.45%	0.058%
42	18.427	2605	2608	2612	rVB5	9654	13272	0.24%	0.030%
43	18.521	2622	2624	2629	rVB5	8814	9011	0.16%	0.020%
44	18.574	2630	2633	2638	rVV6	10046	12322	0.22%	0.028%
45	18.886	2683	2686	2690	rVB5	6802	9185	0.16%	0.021%
46	19.127	2724	2727	2733	rBV2	38246	52499	0.94%	0.119%
47	19.198	2735	2739	2744	rBV	47755	71533	1.27%	0.163%
48	19.339	2760	2763	2768	rBV4	47686	58221	1.04%	0.132%
49	19.551	2793	2799	2805	rBV	3671651	4768689	84.97%	10.834%
50	21.027	3047	3050	3056	rVB6	53522	84014	1.50%	0.191%
51	21.304	3092	3097	3105	rBV	2321661	2946732	52.51%	6.694%
52	23.515	3466	3473	3489	rVB2	2785441	5612254	100.00%	12.750%
53	23.668	3492	3499	3509	rVB	1733624	3240368	57.74%	7.362%




Sum of corrected areas: 44017726

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018767.D
Acq On : 12 Dec 2023 14:37
Operator : MA/JU
Sample : 05675-17
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

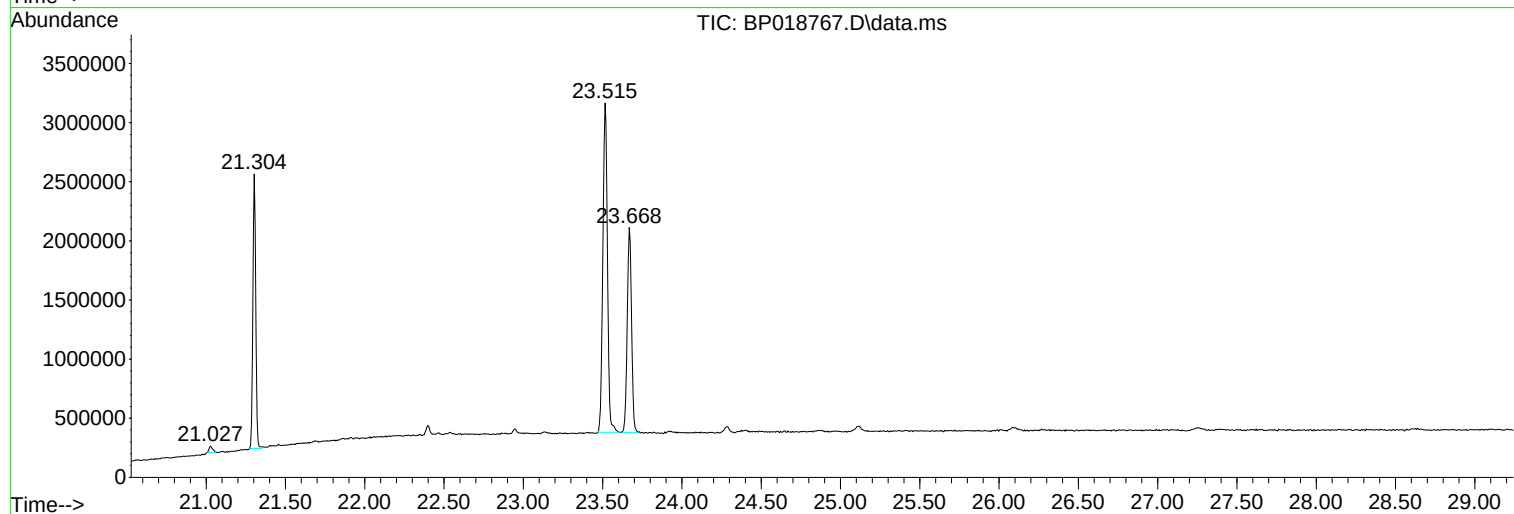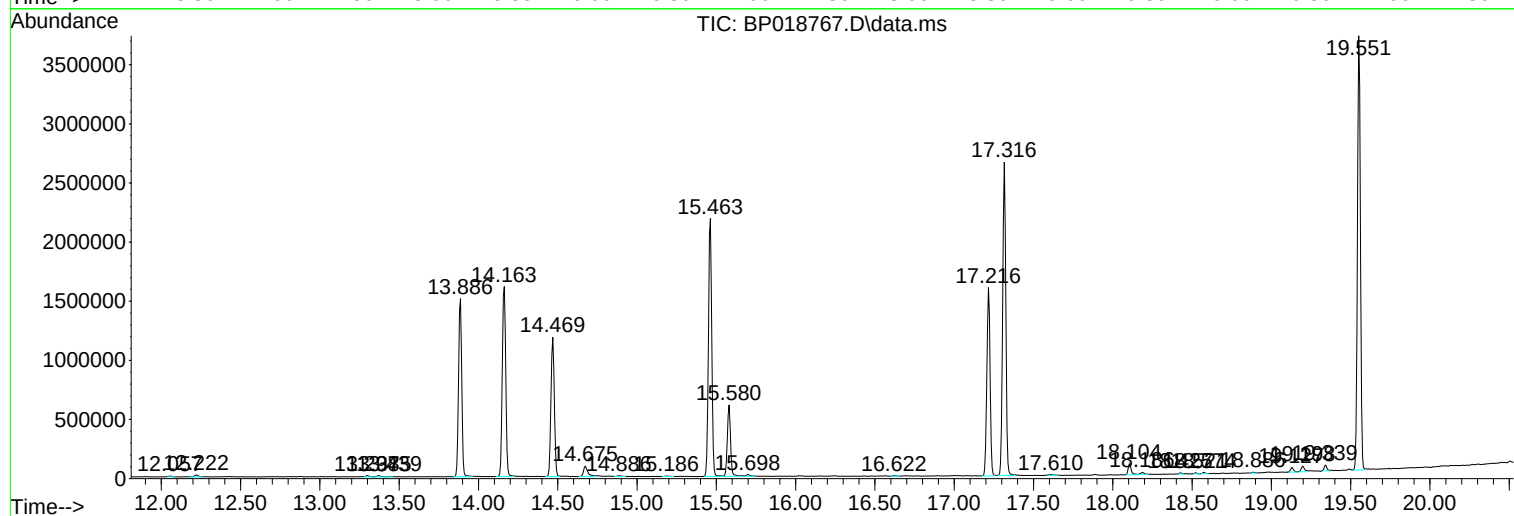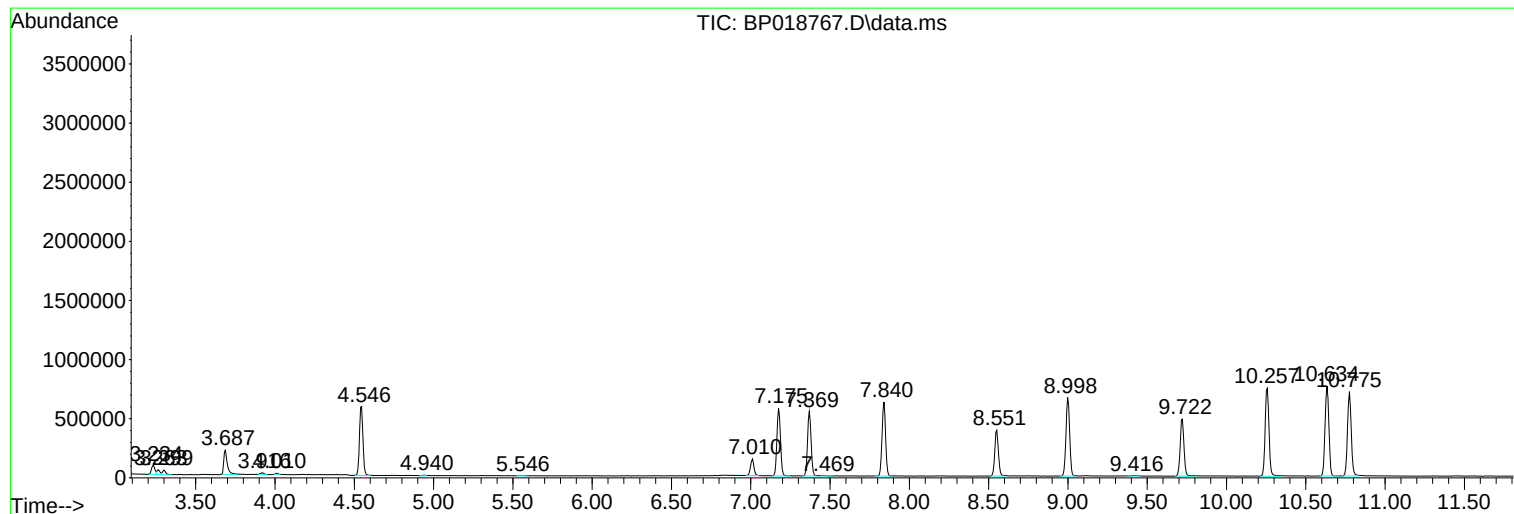

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018767.D
Acq On : 12 Dec 2023 14:37
Operator : MA/JU
Sample : 05675-17
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018767.D
Acq On : 12 Dec 2023 14:37
Operator : MA/JU
Sample : 05675-17
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc