

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018777.D
 Acq On : 12 Dec 2023 20:51
 Operator : MA/JU
 Sample : 05675-01
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AA0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018777.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	34	rBV	48079	60238	0.90%	0.108%
2	3.299	34	36	41	rVB	19977	23689	0.35%	0.043%
3	3.687	98	102	111	rBV	168195	264619	3.95%	0.476%
4	3.793	118	120	125	rVB5	6724	7532	0.11%	0.014%
5	3.917	138	141	145	rVB	15144	23779	0.35%	0.043%
6	4.017	153	158	163	rVB2	14836	22622	0.34%	0.041%
7	4.246	193	197	200	rVB4	6139	9492	0.14%	0.017%
8	4.434	228	229	239	rVB	14931	30570	0.46%	0.055%
9	4.546	244	248	251	rBV4	7047	9498	0.14%	0.017%
10	4.746	275	282	290	rVB4	2159	7048	0.11%	0.013%
11	4.940	310	315	322	rVB9	5938	12717	0.19%	0.023%
12	7.011	660	667	677	rVB	184162	305559	4.56%	0.550%
13	7.175	688	695	705	rVB	700747	1060258	15.81%	1.909%
14	7.369	721	728	739	rBV	694852	1086867	16.21%	1.956%
15	7.840	798	808	818	rBV	804193	1282501	19.12%	2.309%
16	8.552	922	929	937	rBV	543279	864799	12.89%	1.557%
17	8.999	996	1005	1016	rBV	827060	1319336	19.67%	2.375%
18	9.416	1071	1076	1082	rVB10	7326	15104	0.23%	0.027%
19	9.716	1120	1127	1143	rBV	631208	1040043	15.51%	1.872%
20	10.252	1211	1218	1228	rBV	989286	1697442	25.31%	3.055%
21	10.634	1272	1283	1292	rBV	1043391	1722634	25.69%	3.101%
22	10.775	1299	1307	1326	rBV	759657	1339318	19.97%	2.411%
23	12.034	1518	1521	1530	rVB6	5533	14403	0.21%	0.026%
24	12.222	1545	1553	1559	rVB2	20796	34609	0.52%	0.062%
25	12.404	1579	1584	1589	rBV2	12748	20687	0.31%	0.037%
26	13.293	1731	1735	1741	rVB6	7209	12569	0.19%	0.023%
27	13.375	1741	1749	1753	rBV4	18926	33187	0.49%	0.060%
28	13.887	1829	1836	1846	rBV	1834241	2641839	39.39%	4.755%
29	14.004	1851	1856	1859	rVB6	8469	12529	0.19%	0.023%
30	14.157	1872	1882	1896	rBV	2116542	3139476	46.81%	5.651%
31	14.469	1928	1935	1945	rBV	1655031	2392488	35.67%	4.307%
32	14.669	1963	1969	1980	rBV	129704	250622	3.74%	0.451%
33	14.757	1981	1984	1991	rVV5	12214	21105	0.31%	0.038%
34	14.822	1991	1995	2001	rVV5	15632	27230	0.41%	0.049%
35	14.881	2001	2005	2010	rVV8	7310	13383	0.20%	0.024%
36	14.998	2022	2025	2031	rVB8	3726	6944	0.10%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018777.D
 Acq On : 12 Dec 2023 20:51
 Operator : MA/JU
 Sample : 05675-01
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AA0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	15.128	2044	2047	2050	rVB5	6987	8464	0.13%	0.015%
38	15.457	2097	2103	2111	rBV	2811005	4117218	61.39%	7.411%
39	15.581	2118	2124	2139	rBV	767398	1083923	16.16%	1.951%
40	15.698	2140	2144	2150	rVB3	16094	24902	0.37%	0.045%
41	15.975	2186	2191	2197	rBV2	14182	20726	0.31%	0.037%
42	16.245	2234	2237	2243	rVB8	5460	7031	0.10%	0.013%
43	16.492	2274	2279	2282	rBV6	9318	14180	0.21%	0.026%
44	16.616	2297	2300	2306	rVB8	11521	14261	0.21%	0.026%
45	16.981	2359	2362	2365	rBV4	6117	9006	0.13%	0.016%
46	17.092	2378	2381	2387	rVB3	9596	13689	0.20%	0.025%
47	17.216	2394	2402	2410	rBV	2139263	3094000	46.13%	5.569%
48	17.316	2412	2419	2428	rVV2	2971386	4450389	66.36%	8.011%
49	17.387	2428	2431	2442	rVB2	12725	28731	0.43%	0.052%
50	17.887	2513	2516	2520	rVB5	12753	15224	0.23%	0.027%
51	17.981	2528	2532	2538	rBV8	14236	25009	0.37%	0.045%
52	18.104	2549	2553	2558	rBV	170194	220367	3.29%	0.397%
53	18.422	2603	2607	2617	rBV2	35355	64287	0.96%	0.116%
54	18.569	2629	2632	2640	rBV4	25418	39010	0.58%	0.070%
55	19.128	2723	2727	2731	rBV	54097	68802	1.03%	0.124%
56	19.192	2734	2738	2742	rBV	62499	97300	1.45%	0.175%
57	19.281	2749	2753	2758	rVB	92085	102400	1.53%	0.184%
58	19.339	2759	2763	2770	rBV3	85517	112605	1.68%	0.203%
59	19.551	2793	2799	2806	rBV	4486715	5924375	88.34%	10.664%
60	19.804	2838	2842	2846	rVB4	40462	51756	0.77%	0.093%
61	21.022	3047	3049	3058	rVB8	48686	87689	1.31%	0.158%
62	21.304	3091	3097	3104	rBV	3009297	3991133	59.51%	7.184%
63	23.510	3465	3472	3487	rVB2	3449523	6706623	100.00%	12.072%
64	23.663	3491	3498	3510	rVB	2123502	4334229	64.63%	7.802%




Sum of corrected areas: 55554065

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018777.D
Acq On : 12 Dec 2023 20:51
Operator : MA/JU
Sample : 05675-01
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

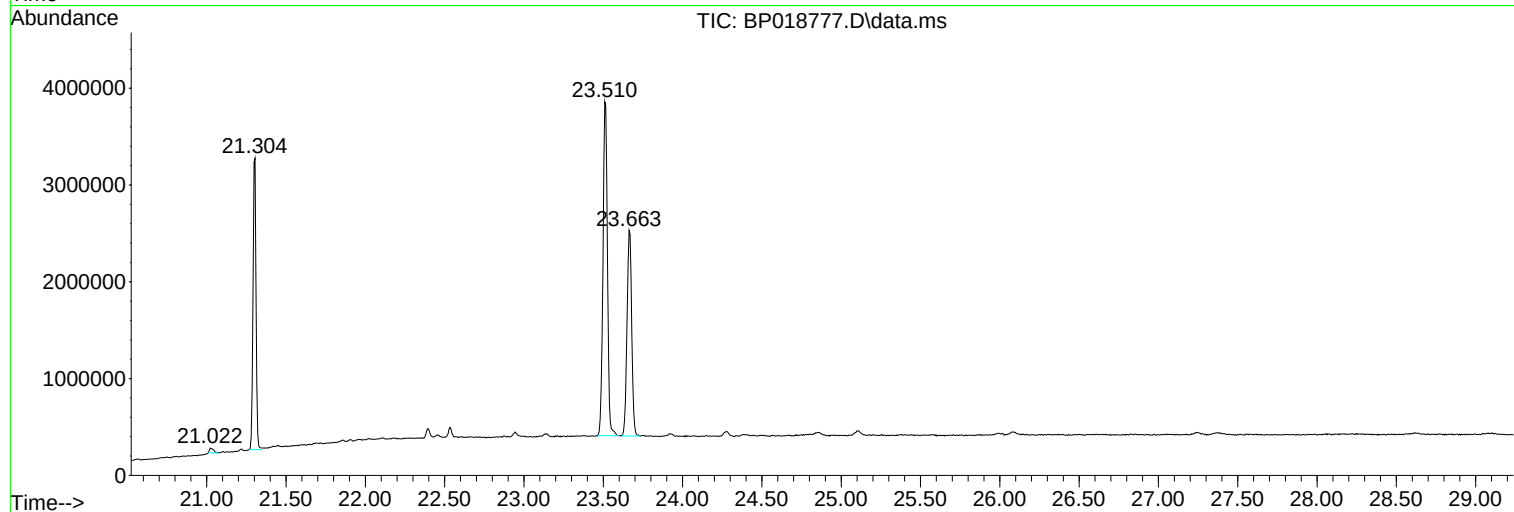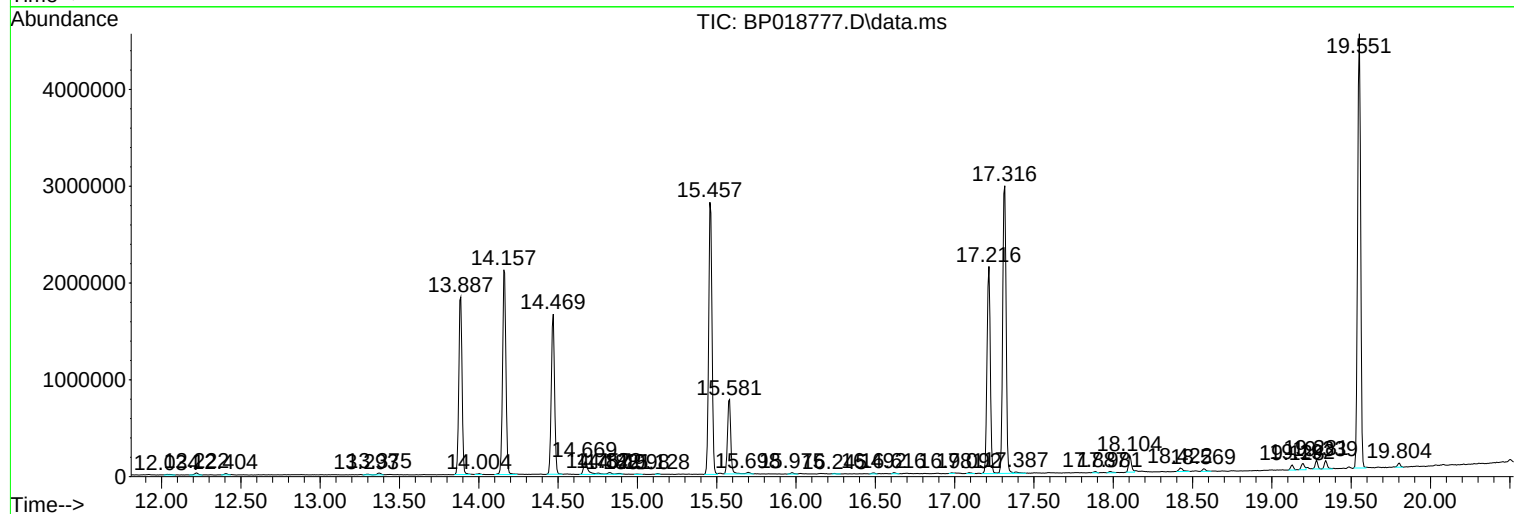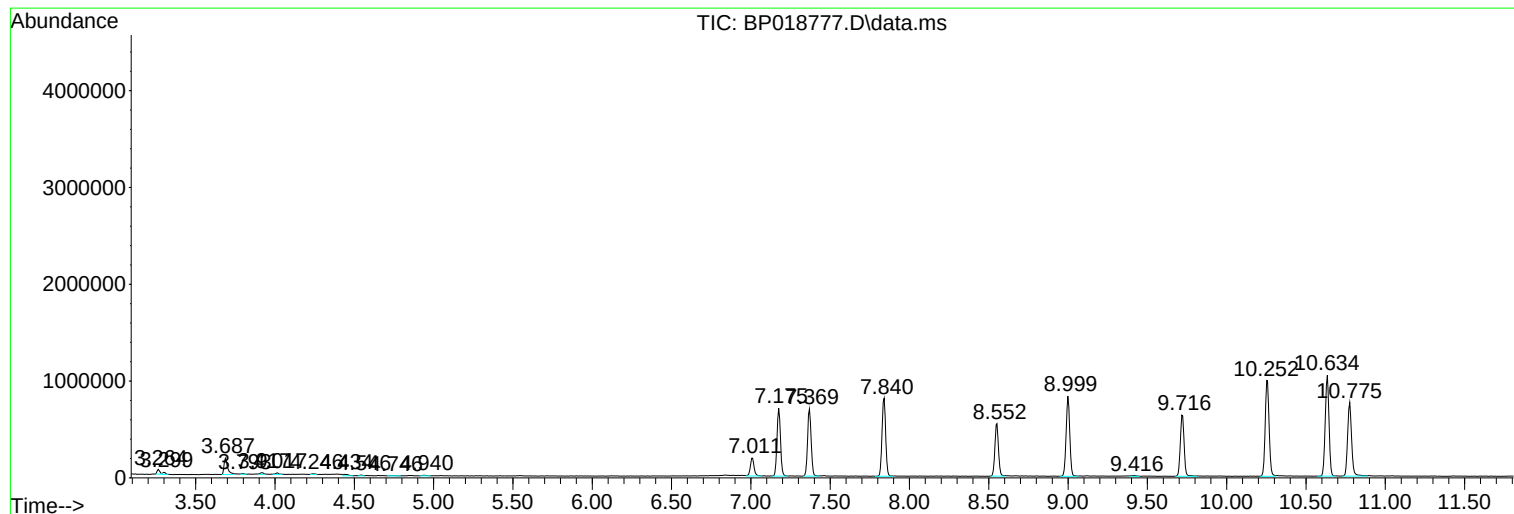

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018777.D
Acq On : 12 Dec 2023 20:51
Operator : MA/JU
Sample : 05675-01
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018777.D
Acq On : 12 Dec 2023 20:51
Operator : MA/JU
Sample : 05675-01
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc