

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018778.D
 Acq On : 12 Dec 2023 21:25
 Operator : MA/JU
 Sample : 05675-18
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AC1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018778.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	20	24	27	rBV	40600	60195	0.90%	0.116%
2	3.264	27	30	33	rVV	44794	56599	0.84%	0.109%
3	3.299	33	36	41	rVB	32426	42635	0.63%	0.082%
4	3.687	98	102	118	rBV	225641	362051	5.39%	0.699%
5	3.916	137	141	147	rVB	17909	28668	0.43%	0.055%
6	4.011	154	157	163	rVB	10415	13964	0.21%	0.027%
7	4.540	241	247	261	rVB	416296	639187	9.51%	1.234%
8	5.552	411	419	423	rVB10	3943	8406	0.13%	0.016%
9	7.010	660	667	675	rVB	165764	264784	3.94%	0.511%
10	7.175	687	695	705	rVB	689306	1048573	15.60%	2.025%
11	7.369	720	728	736	rBV	666288	1033471	15.37%	1.996%
12	7.463	739	744	749	rVB9	4934	9200	0.14%	0.018%
13	7.840	800	808	817	rBV	693743	1089010	16.20%	2.103%
14	8.552	922	929	941	rBV	482727	779410	11.59%	1.505%
15	8.999	997	1005	1019	rBV	801446	1272904	18.94%	2.458%
16	9.116	1020	1025	1030	rVB7	4795	7837	0.12%	0.015%
17	9.716	1116	1127	1136	rBV	597287	987182	14.68%	1.907%
18	10.251	1209	1218	1232	rBV	919071	1551993	23.09%	2.997%
19	10.634	1274	1283	1291	rBV	853183	1440989	21.44%	2.783%
20	10.775	1300	1307	1319	rBV	816671	1397504	20.79%	2.699%
21	12.057	1518	1525	1529	rBV9	5509	10476	0.16%	0.020%
22	12.222	1546	1553	1569	rVB3	17580	35935	0.53%	0.069%
23	13.298	1732	1736	1743	rVB6	7224	10803	0.16%	0.021%
24	13.369	1743	1748	1754	rBV3	16775	28542	0.42%	0.055%
25	13.881	1829	1835	1848	rBV	1779633	2531631	37.66%	4.889%
26	14.163	1875	1883	1891	rBV	1969895	2927233	43.54%	5.653%
27	14.469	1928	1935	1942	rBV	1323631	1969879	29.30%	3.804%
28	14.675	1962	1970	1981	rBV	110964	222481	3.31%	0.430%
29	14.881	2002	2005	2014	rVB	6628	14247	0.21%	0.028%
30	15.457	2096	2103	2115	rBV	2616640	3881654	57.74%	7.497%
31	15.575	2117	2123	2138	rVV	718741	1027095	15.28%	1.984%
32	15.698	2140	2144	2153	rVB3	14239	25569	0.38%	0.049%
33	16.028	2195	2200	2207	rVB8	6206	13615	0.20%	0.026%
34	16.239	2233	2236	2240	rVB5	5448	7602	0.11%	0.015%
35	16.622	2297	2301	2308	rVB10	4265	9830	0.15%	0.019%
36	17.216	2395	2402	2409	rBV	1826788	2539320	37.77%	4.904%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018778.D
 Acq On : 12 Dec 2023 21:25
 Operator : MA/JU
 Sample : 05675-18
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AC1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	17.310	2412	2418	2431	rBV2	2974557	4432708	65.94%	8.561%
38	18.104	2548	2553	2560	rBV	112130	162684	2.42%	0.314%
39	18.186	2563	2567	2572	rVB5	12757	21647	0.32%	0.042%
40	18.422	2604	2607	2611	rBV4	11981	19471	0.29%	0.038%
41	18.575	2630	2633	2637	rVB4	14549	17949	0.27%	0.035%
42	19.127	2723	2727	2732	rBV2	52638	66572	0.99%	0.129%
43	19.192	2734	2738	2742	rBV	56245	82794	1.23%	0.160%
44	19.339	2759	2763	2768	rBV2	77432	100458	1.49%	0.194%
45	19.551	2793	2799	2805	rBV	4412457	5817727	86.54%	11.236%
46	21.304	3092	3097	3102	rBV	2703921	3328532	49.51%	6.428%
47	23.515	3465	3473	3480	rBV2	3531754	6722437	100.00%	12.983%
48	23.668	3492	3499	3509	rVB	1824589	3654411	54.36%	7.058%




Sum of corrected areas: 51777864

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018778.D
Acq On : 12 Dec 2023 21:25
Operator : MA/JU
Sample : 05675-18
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

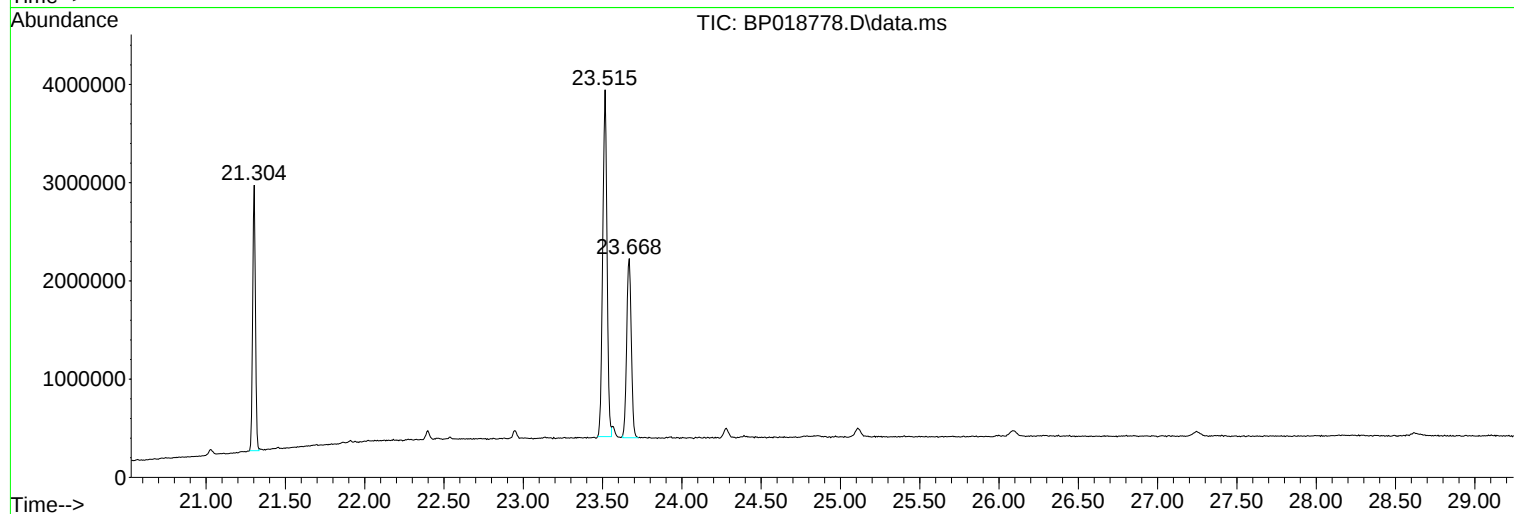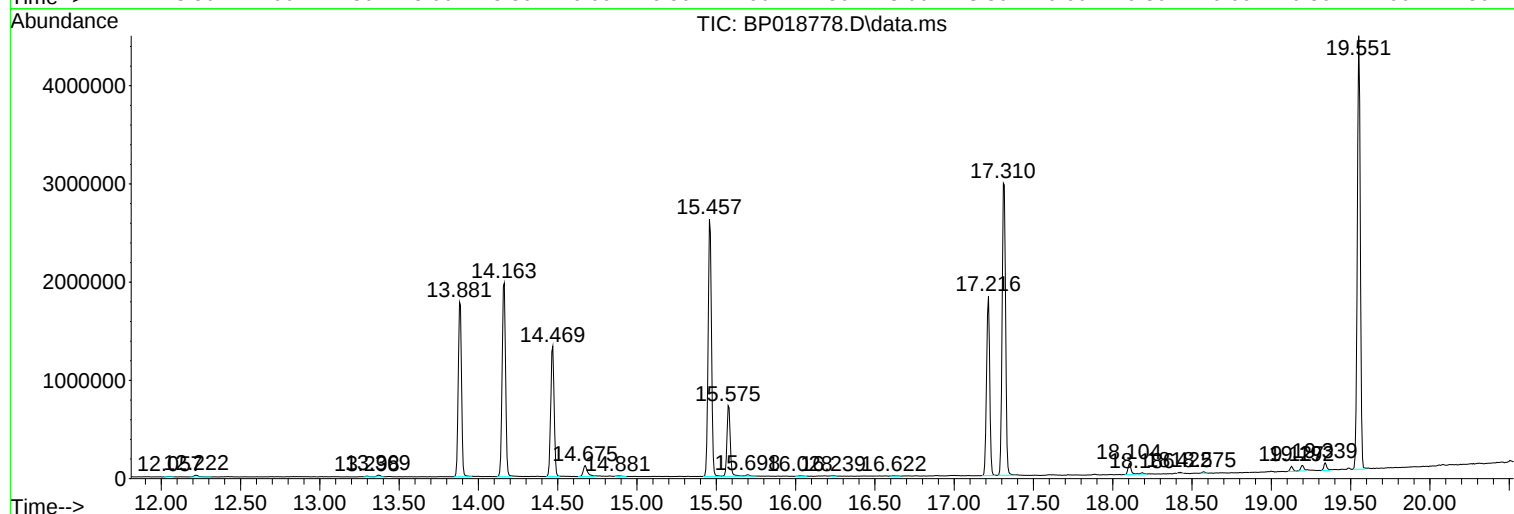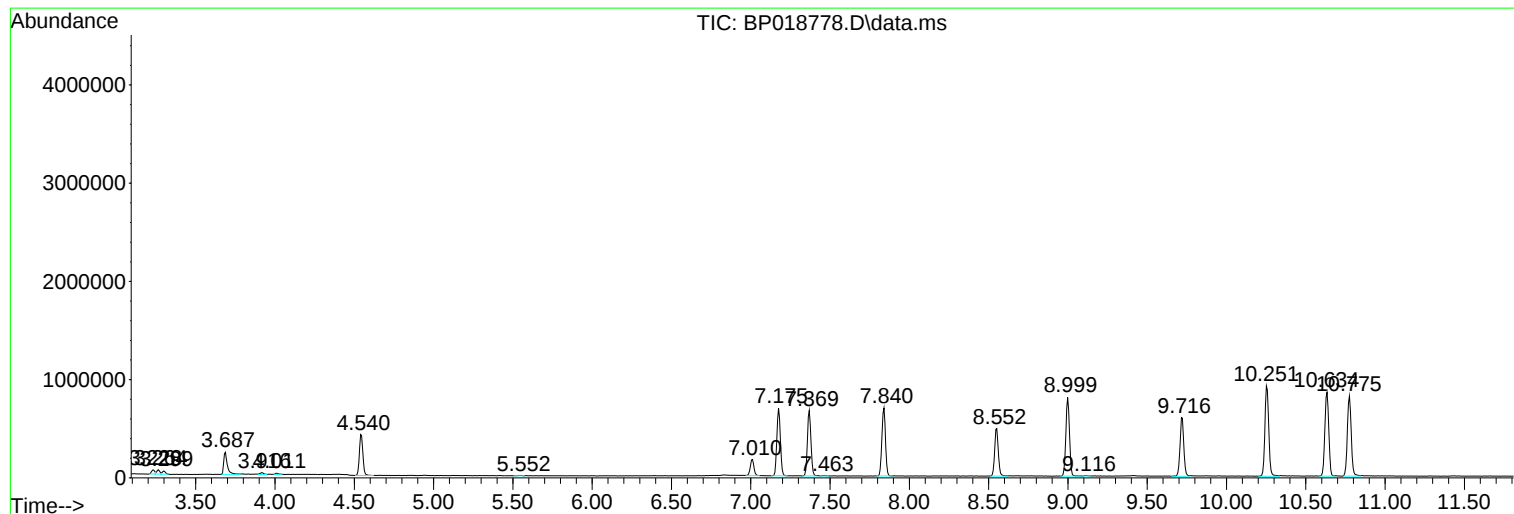

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018778.D
Acq On : 12 Dec 2023 21:25
Operator : MA/JU
Sample : 05675-18
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018778.D
Acq On : 12 Dec 2023 21:25
Operator : MA/JU
Sample : 05675-18
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc