

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018790.D
 Acq On : 13 Dec 2023 04:11
 Operator : MA/JU
 Sample : 05675-03
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AA4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018790.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	35	rBV	38687	49520	0.74%	0.102%
2	3.693	99	103	109	rBV	54221	85542	1.27%	0.177%
3	3.917	138	141	145	rVB2	10129	14045	0.21%	0.029%
4	4.011	154	157	162	rVB2	10421	14619	0.22%	0.030%
5	4.540	244	247	252	rVB6	8123	10754	0.16%	0.022%
6	6.828	633	636	642	rVB7	5248	9023	0.13%	0.019%
7	7.011	659	667	675	rVB	147186	249409	3.71%	0.515%
8	7.175	689	695	704	rVB	660299	1006861	14.98%	2.078%
9	7.369	720	728	736	rBV	646570	991762	14.75%	2.047%
10	7.840	800	808	817	rBV	639765	1018243	15.15%	2.101%
11	8.546	922	928	939	rBV	446953	730355	10.87%	1.507%
12	8.999	996	1005	1017	rBV	792732	1287326	19.15%	2.656%
13	9.416	1072	1076	1081	rVB7	7270	11754	0.17%	0.024%
14	9.716	1119	1127	1136	rBV	624669	1001981	14.91%	2.068%
15	10.252	1210	1218	1231	rBV	923183	1550344	23.06%	3.199%
16	10.634	1275	1283	1297	rVB	809597	1363447	20.28%	2.814%
17	10.775	1302	1307	1313	rBV	20347	40648	0.60%	0.084%
18	11.422	1413	1417	1426	rVB	3911	8408	0.13%	0.017%
19	11.899	1491	1498	1502	rBV10	4178	7924	0.12%	0.016%
20	12.034	1515	1521	1527	rBV2	13212	27127	0.40%	0.056%
21	12.216	1547	1552	1559	rBV2	18774	30477	0.45%	0.063%
22	12.857	1656	1661	1666	rVB9	4712	10842	0.16%	0.022%
23	13.304	1731	1737	1742	rVB9	4079	8507	0.13%	0.018%
24	13.369	1742	1748	1756	rBV6	14911	29829	0.44%	0.062%
25	13.881	1829	1835	1850	rBV	1732705	2529674	37.63%	5.220%
26	14.163	1872	1883	1891	rBV	1921972	2873831	42.75%	5.930%
27	14.469	1926	1935	1943	rBV	1219224	1899987	28.27%	3.921%
28	14.669	1963	1969	1980	rBV	104308	204984	3.05%	0.423%
29	14.751	1980	1983	1990	rVB2	12095	20264	0.30%	0.042%
30	14.881	2003	2005	2012	rVB6	6665	9651	0.14%	0.020%
31	15.457	2096	2103	2117	rBV	2709640	3895508	57.95%	8.038%
32	15.581	2117	2124	2133	rBV	704903	992699	14.77%	2.048%
33	15.698	2139	2144	2148	rVB4	14971	23386	0.35%	0.048%
34	16.034	2194	2201	2206	rVB10	4993	11471	0.17%	0.024%
35	16.245	2232	2237	2240	rBV7	4054	7660	0.11%	0.016%
36	16.887	2342	2346	2350	rBV7	4613	6936	0.10%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018790.D
 Acq On : 13 Dec 2023 04:11
 Operator : MA/JU
 Sample : 05675-03
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AA4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	17.210	2395	2401	2411	rBV	1711598	2447233	36.41%	5.050%
38	17.310	2412	2418	2431	rBV	3031242	4417534	65.72%	9.116%
39	17.886	2513	2516	2519	rVB5	7048	9560	0.14%	0.020%
40	18.104	2548	2553	2560	rBV	86225	121312	1.80%	0.250%
41	19.128	2723	2727	2732	rBV3	45716	61796	0.92%	0.128%
42	19.192	2734	2738	2743	rBV	51200	78116	1.16%	0.161%
43	19.339	2759	2763	2769	rBV2	63002	81129	1.21%	0.167%
44	19.486	2785	2788	2792	rBV4	18366	19718	0.29%	0.041%
45	19.551	2793	2799	2806	rVV	4475190	5659852	84.20%	11.679%
46	21.304	3091	3097	3103	rBV	2512077	3256795	48.45%	6.720%
47	23.510	3465	3472	3487	rVB	3394266	6721968	100.00%	13.871%
48	23.663	3491	3498	3510	rVB	1763780	3550967	52.83%	7.328%




Sum of corrected areas: 48460778

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018790.D
Acq On : 13 Dec 2023 04:11
Operator : MA/JU
Sample : 05675-03
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

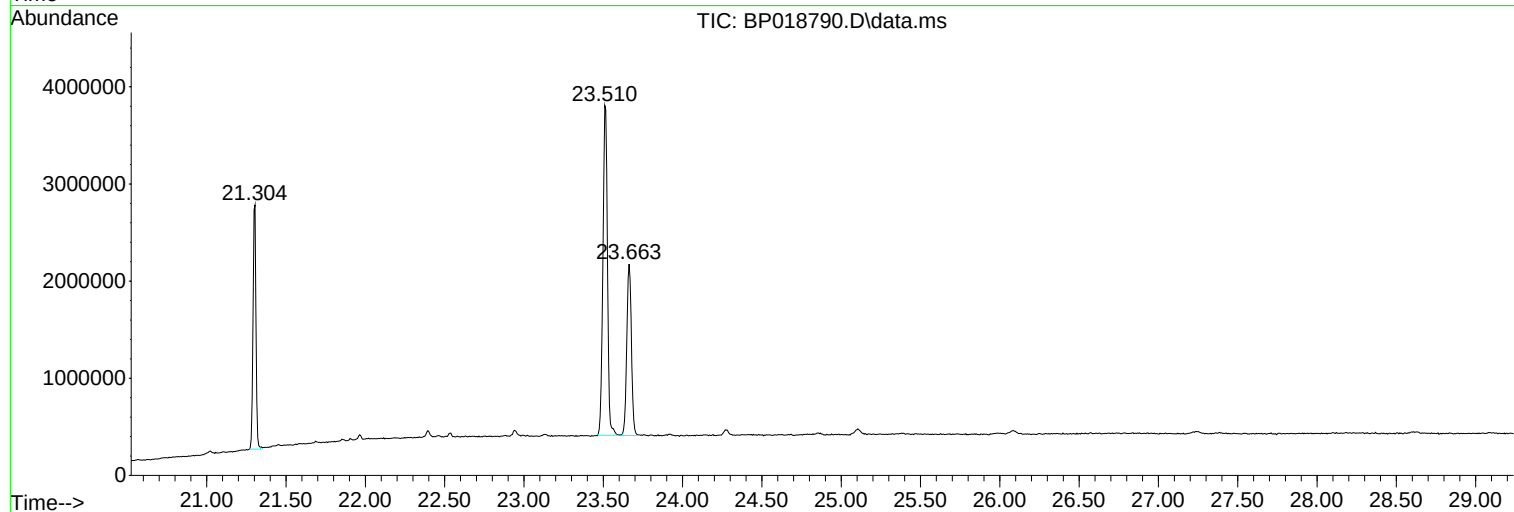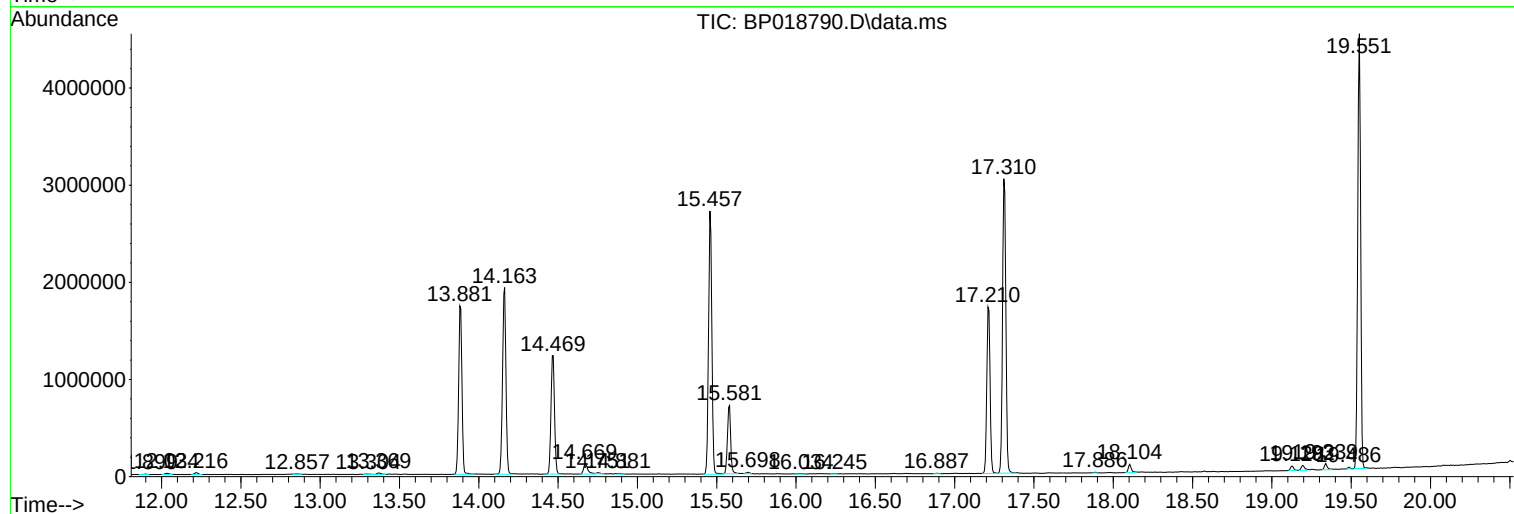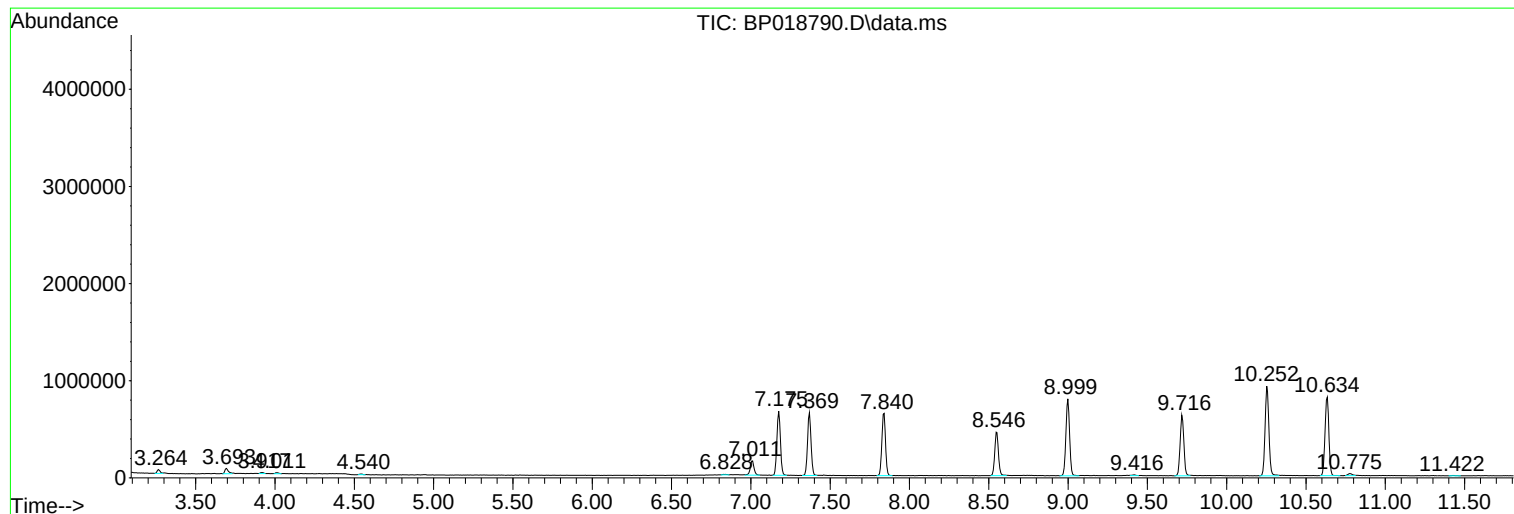

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018790.D
Acq On : 13 Dec 2023 04:11
Operator : MA/JU
Sample : 05675-03
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018790.D
Acq On : 13 Dec 2023 04:11
Operator : MA/JU
Sample : 05675-03
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
