

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018791.D
 Acq On : 13 Dec 2023 04:45
 Operator : MA/JU
 Sample : 05675-04
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018791.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	21	24	27	rBV3	11346	15900	0.31%	0.040%
2	3.264	27	30	33	rVV	36398	43711	0.84%	0.109%
3	3.299	33	36	42	rVB2	15013	21893	0.42%	0.055%
4	3.687	98	102	116	rBV	173141	285119	5.50%	0.714%
5	3.917	138	141	146	rVB	12572	17259	0.33%	0.043%
6	4.011	154	157	162	rVB3	10423	15765	0.30%	0.039%
7	4.540	241	247	252	rBV	67362	100217	1.93%	0.251%
8	6.752	617	623	624	rBV6	3092	5373	0.10%	0.013%
9	6.834	634	637	643	rVB8	3850	7746	0.15%	0.019%
10	7.005	661	666	678	rVB	112494	189882	3.66%	0.475%
11	7.175	687	695	704	rBV	532513	817531	15.76%	2.047%
12	7.369	721	728	739	rVB	499480	781345	15.07%	1.956%
13	7.834	798	807	816	rBV	528950	849641	16.38%	2.127%
14	8.546	922	928	942	rBV	346059	561504	10.83%	1.406%
15	8.999	997	1005	1016	rBV	619351	1020559	19.68%	2.555%
16	9.116	1020	1025	1031	rBV3	20290	31717	0.61%	0.079%
17	9.410	1072	1075	1080	rVB6	7472	12307	0.24%	0.031%
18	9.716	1120	1127	1141	rBV	477903	771150	14.87%	1.931%
19	10.252	1211	1218	1233	rBV	744968	1220074	23.53%	3.055%
20	10.628	1273	1282	1295	rBV	666414	1125955	21.71%	2.819%
21	10.775	1298	1307	1325	rBV	719482	1254232	24.18%	3.140%
22	11.434	1412	1419	1426	rBV	2963	8155	0.16%	0.020%
23	11.910	1493	1500	1502	rBV8	3190	5963	0.11%	0.015%
24	12.034	1516	1521	1523	rBV6	5106	6561	0.13%	0.016%
25	12.216	1547	1552	1558	rVB2	14774	27743	0.53%	0.069%
26	13.293	1732	1735	1740	rVB6	4664	6787	0.13%	0.017%
27	13.369	1742	1748	1754	rVV4	15341	26924	0.52%	0.067%
28	13.881	1828	1835	1846	rBV	1435098	1998715	38.54%	5.005%
29	14.157	1874	1882	1892	rBV2	1594673	2326669	44.86%	5.826%
30	14.463	1927	1934	1944	rBV	1065283	1549529	29.88%	3.880%
31	14.675	1964	1970	1978	rBV	68323	138413	2.67%	0.347%
32	14.834	1993	1997	2000	rVB6	4133	5373	0.10%	0.013%
33	14.887	2002	2006	2012	rVV8	7158	13875	0.27%	0.035%
34	15.457	2096	2103	2110	rBV	2174010	3033593	58.49%	7.596%
35	15.575	2117	2123	2133	rBV	565770	752232	14.50%	1.884%
36	15.698	2140	2144	2151	rVB4	12326	22290	0.43%	0.056%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018791.D
 Acq On : 13 Dec 2023 04:45
 Operator : MA/JU
 Sample : 05675-04
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	16.022	2194	2199	2204	rBV9	4162	8711	0.17%	0.022%
38	16.692	2310	2313	2316	rBV5	3694	5198	0.10%	0.013%
39	16.992	2361	2364	2367	rBV5	3760	5622	0.11%	0.014%
40	17.210	2394	2401	2411	rBV	1385374	2011943	38.79%	5.038%
41	17.310	2412	2418	2429	rVV2	2509324	3484846	67.20%	8.726%
42	18.104	2548	2553	2558	rBV3	71183	97098	1.87%	0.243%
43	18.569	2630	2632	2637	rVB6	7942	12165	0.23%	0.030%
44	19.128	2722	2727	2731	rBV	39828	55105	1.06%	0.138%
45	19.192	2734	2738	2742	rBV	39494	56195	1.08%	0.141%
46	19.339	2759	2763	2767	rBV3	43473	53876	1.04%	0.135%
47	19.551	2793	2799	2807	rBV	3502951	4525385	87.26%	11.331%
48	21.298	3091	3096	3102	rBV	2013219	2571599	49.59%	6.439%
49	23.510	3465	3472	3485	rVB	2657494	5186145	100.00%	12.986%
50	23.663	3491	3498	3509	rVB	1425030	2791983	53.84%	6.991%




Sum of corrected areas: 39937573

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018791.D
Acq On : 13 Dec 2023 04:45
Operator : MA/JU
Sample : 05675-04
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

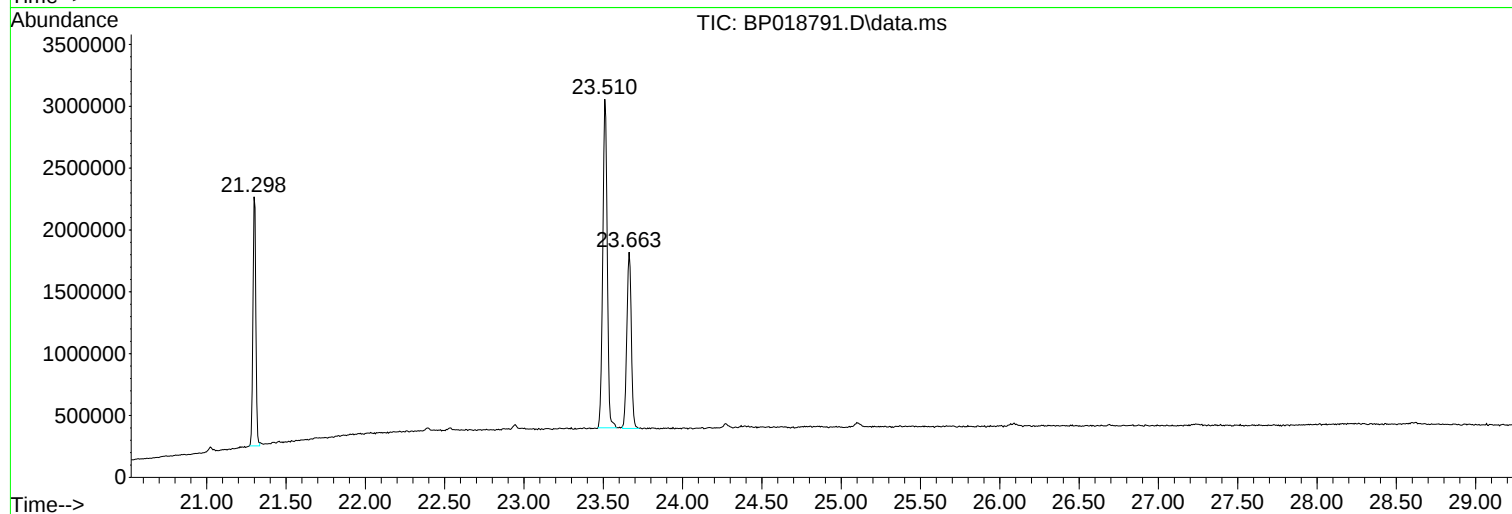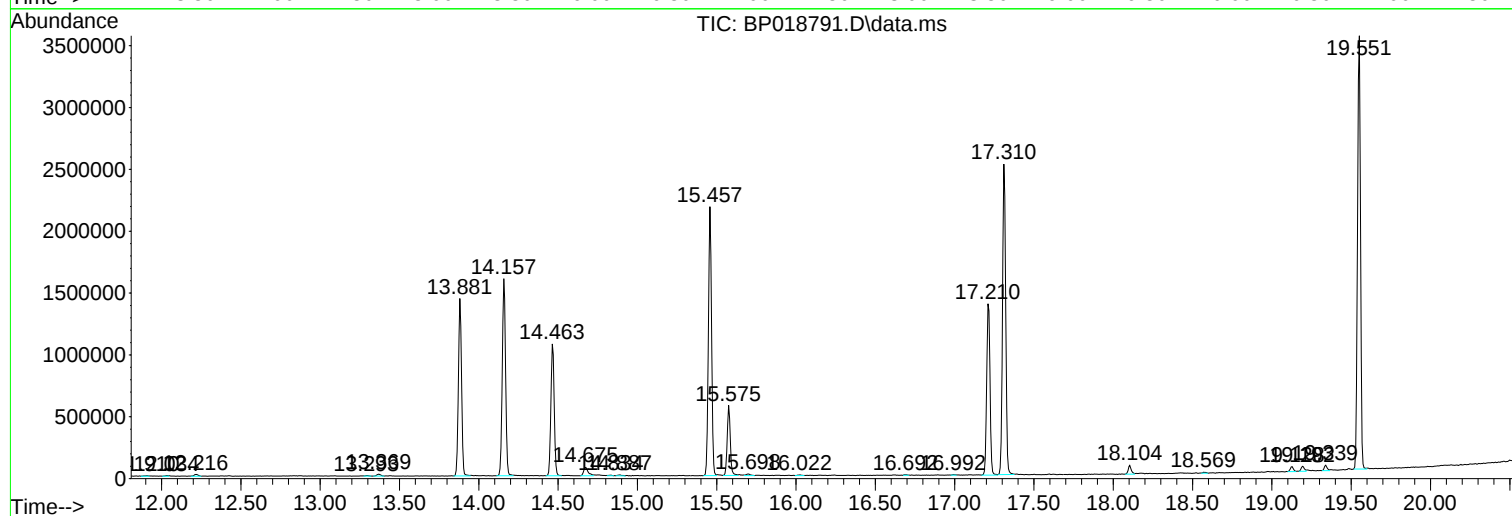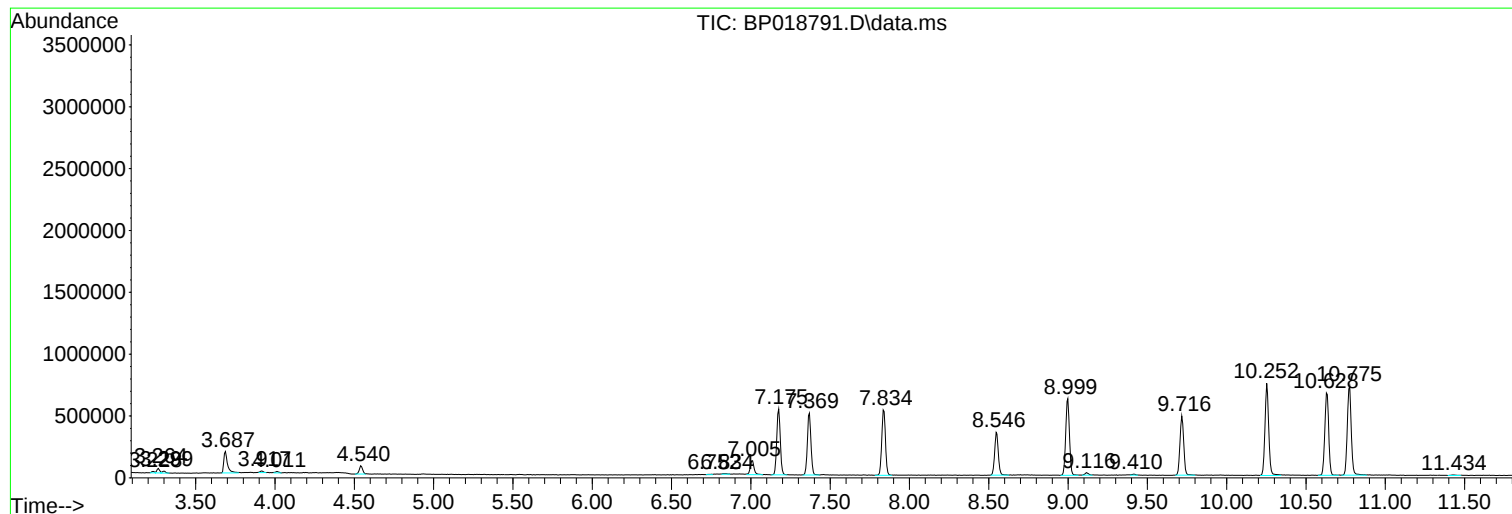

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018791.D
Acq On : 13 Dec 2023 04:45
Operator : MA/JU
Sample : 05675-04
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018791.D
Acq On : 13 Dec 2023 04:45
Operator : MA/JU
Sample : 05675-04
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------