

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018794.D
 Acq On : 13 Dec 2023 07:00
 Operator : MA/JU
 Sample : PB157653BL
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK653

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018794.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	36	rVB	53104	71161	1.41%	0.161%
2	3.681	97	101	119	rBV	597681	915170	18.19%	2.072%
3	4.005	154	156	163	rVB4	9954	14916	0.30%	0.034%
4	7.005	660	666	678	rVB	671766	1056933	21.01%	2.393%
5	7.175	689	695	706	rVB	540862	820813	16.31%	1.858%
6	7.369	721	728	736	rBV	694737	1082416	21.51%	2.450%
7	7.834	799	807	817	rBV	586047	935551	18.60%	2.118%
8	8.546	921	928	939	rBV	807449	1309674	26.03%	2.965%
9	8.999	996	1005	1012	rBV	619621	1005942	19.99%	2.277%
10	9.716	1120	1127	1136	rBV	507817	812128	16.14%	1.839%
11	10.252	1209	1218	1229	rBV	825640	1376384	27.36%	3.116%
12	10.628	1274	1282	1291	rVB	729731	1231874	24.48%	2.789%
13	10.775	1297	1307	1316	rBV	759308	1334303	26.52%	3.021%
14	12.222	1547	1553	1562	rVB3	15706	26965	0.54%	0.061%
15	13.375	1743	1749	1756	rVV7	7678	13674	0.27%	0.031%
16	13.434	1756	1759	1767	rVB9	3116	6290	0.13%	0.014%
17	13.881	1826	1835	1843	rBV	1438176	1978365	39.32%	4.479%
18	14.157	1875	1882	1892	rBV	1554425	2304002	45.79%	5.216%
19	14.463	1927	1934	1942	rBV	1117161	1709892	33.99%	3.871%
20	14.669	1962	1969	1989	rBV	601117	986605	19.61%	2.234%
21	14.887	2001	2006	2009	rVB7	4122	7050	0.14%	0.016%
22	15.128	2043	2047	2052	rVB8	4382	9319	0.19%	0.021%
23	15.457	2096	2103	2110	rBV	2115478	2971177	59.06%	6.726%
24	15.575	2117	2123	2135	rBV	529600	731529	14.54%	1.656%
25	15.698	2140	2144	2151	rVV7	12177	22301	0.44%	0.050%
26	16.028	2194	2200	2202	rBV6	5082	8910	0.18%	0.020%
27	16.240	2233	2236	2243	rVB9	3129	6485	0.13%	0.015%
28	16.892	2341	2347	2353	rBV10	4431	9598	0.19%	0.022%
29	17.004	2361	2366	2368	rBV4	4155	6149	0.12%	0.014%
30	17.210	2395	2401	2412	rBV	1569980	2228718	44.30%	5.046%
31	17.310	2412	2418	2428	rBV2	2480297	3463897	68.85%	7.842%
32	18.104	2550	2553	2559	rBV7	7904	13806	0.27%	0.031%
33	19.128	2723	2727	2731	rVB2	34234	46772	0.93%	0.106%
34	19.192	2734	2738	2746	rBV	39200	61339	1.22%	0.139%
35	19.339	2760	2763	2766	rBV4	11396	13365	0.27%	0.030%
36	19.551	2793	2799	2805	rBV	3182217	4417459	87.80%	10.001%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018794.D
Acq On : 13 Dec 2023 07:00
Operator : MA/JU
Sample : PB157653BL
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK653

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	21.298	3091	3096	3104	rBV	2359195	2948462	58.60%	6.675%
38	23.510	3465	3472	3479	rBV	2796739	5031153	100.00%	11.390%
39	23.663	3491	3498	3510	rVB	1602385	3181120	63.23%	7.202%




Sum of corrected areas: 44171667

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018794.D
Acq On : 13 Dec 2023 07:00
Operator : MA/JU
Sample : PB157653BL
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK653

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

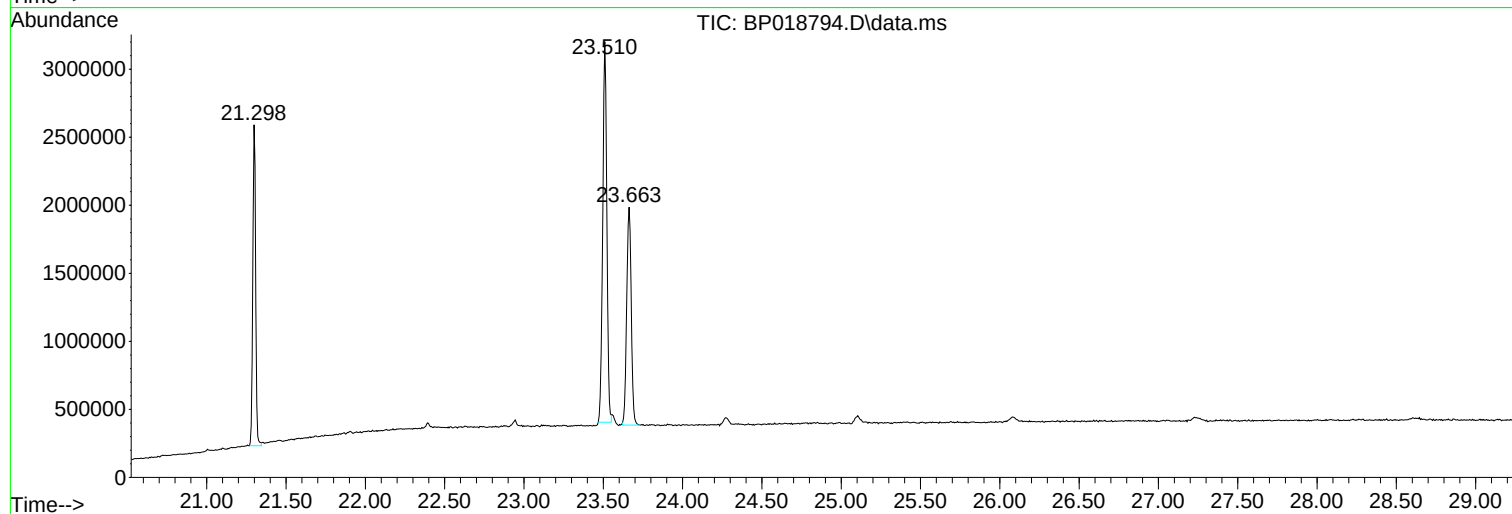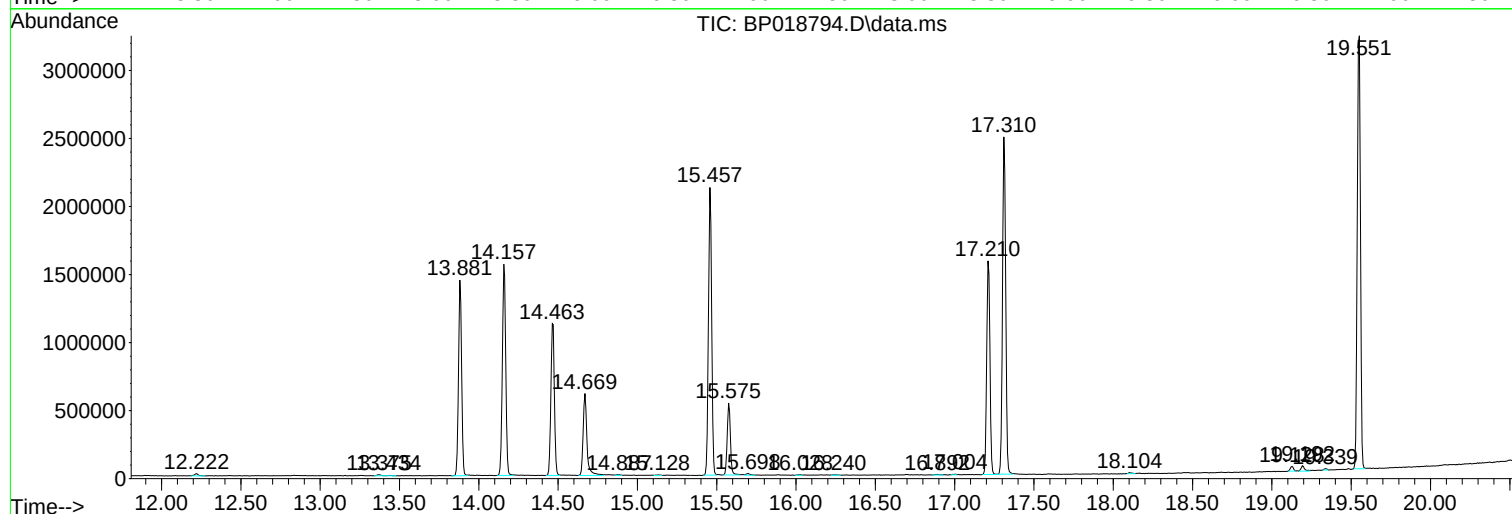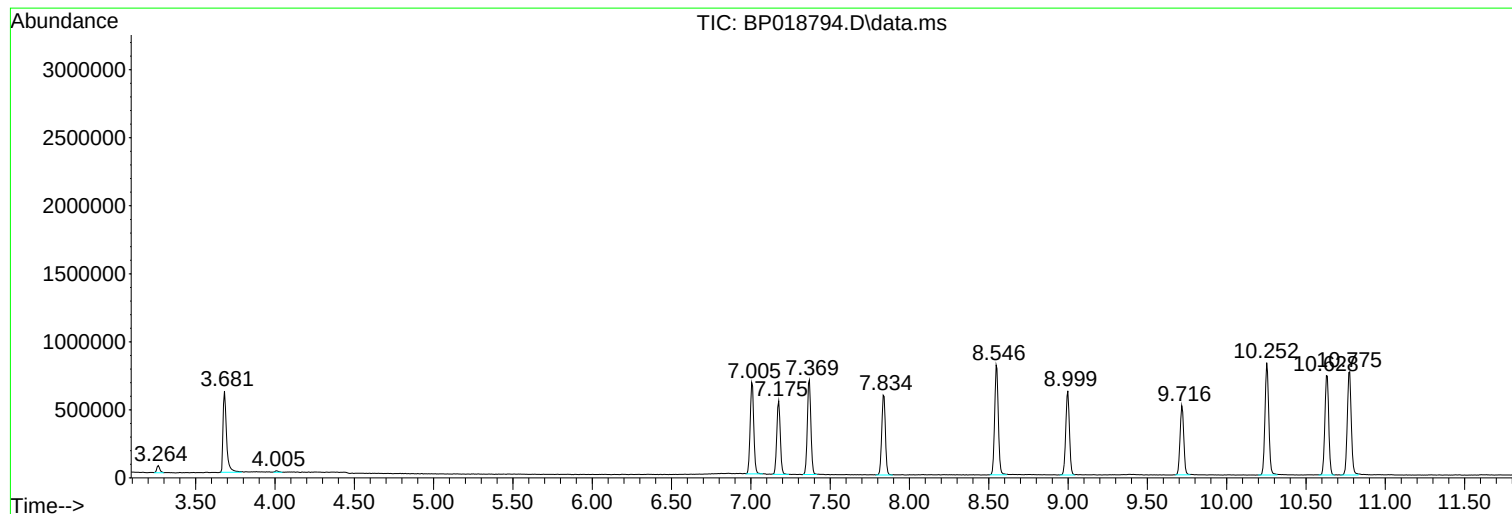

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018794.D
Acq On : 13 Dec 2023 07:00
Operator : MA/JU
Sample : PB157653BL
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK653

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018794.D
Acq On : 13 Dec 2023 07:00
Operator : MA/JU
Sample : PB157653BL
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK653

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------