

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018796.D
 Acq On : 13 Dec 2023 08:08
 Operator : MA/JU
 Sample : PB157666BL
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK666

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018796.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	37	rVB	54172	71720	1.33%	0.151%
2	3.681	97	101	116	rBV	647792	975269	18.10%	2.060%
3	4.011	154	157	163	rVB4	12656	19788	0.37%	0.042%
4	7.005	660	666	679	rVB	716370	1136601	21.09%	2.400%
5	7.175	689	695	708	rVB	584225	894515	16.60%	1.889%
6	7.369	721	728	737	rBV	741591	1159285	21.51%	2.448%
7	7.834	801	807	814	rBV	632053	1011331	18.77%	2.136%
8	8.546	920	928	939	rBV	875246	1417400	26.30%	2.993%
9	8.999	997	1005	1013	rBV	678176	1078324	20.01%	2.277%
10	9.716	1120	1127	1136	rBV	541670	861220	15.98%	1.819%
11	10.251	1208	1218	1227	rBV	890952	1459035	27.08%	3.081%
12	10.634	1274	1283	1290	rBV	815199	1361570	25.27%	2.875%
13	10.775	1299	1307	1323	rBV	807574	1424467	26.44%	3.008%
14	12.222	1547	1553	1562	rBV2	16826	30550	0.57%	0.065%
15	13.369	1741	1748	1753	rBV3	15523	27741	0.51%	0.059%
16	13.440	1756	1760	1766	rVB7	3797	6769	0.13%	0.014%
17	13.881	1829	1835	1846	rVV	1558898	2110629	39.17%	4.457%
18	14.157	1874	1882	1895	rBV	1690764	2492610	46.26%	5.264%
19	14.463	1927	1934	1945	rBV	1278357	1877513	34.84%	3.965%
20	14.669	1963	1969	1988	rBV	621711	1026889	19.06%	2.169%
21	15.457	2097	2103	2111	rBV	2289393	3214387	59.65%	6.788%
22	15.575	2117	2123	2139	rBV	550370	781471	14.50%	1.650%
23	15.698	2139	2144	2148	rVB2	9824	13834	0.26%	0.029%
24	16.016	2196	2198	2204	rBV7	3048	5567	0.10%	0.012%
25	16.998	2361	2365	2370	rBV4	4375	7470	0.14%	0.016%
26	17.216	2395	2402	2408	rBV	1694763	2434263	45.18%	5.141%
27	17.310	2411	2418	2430	rBV	2581577	3718574	69.01%	7.853%
28	18.104	2550	2553	2556	rBV4	6067	7039	0.13%	0.015%
29	18.569	2630	2632	2636	rBV4	5221	7952	0.15%	0.017%
30	19.127	2723	2727	2733	rVB2	37250	51767	0.96%	0.109%
31	19.192	2734	2738	2743	rBV	35594	52650	0.98%	0.111%
32	19.551	2793	2799	2806	rBV	3505559	4719439	87.59%	9.967%
33	21.298	3091	3096	3105	rBV	2407779	3123813	57.97%	6.597%
34	23.510	3465	3472	3486	rVB2	2813948	5388370	100.00%	11.380%
35	23.662	3491	3498	3513	rVB	1702642	3381172	62.75%	7.141%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018796.D
Acq On : 13 Dec 2023 08:08
Operator : MA/JU
Sample : PB157666BL
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK666

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 47350994

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018796.D
Acq On : 13 Dec 2023 08:08
Operator : MA/JU
Sample : PB157666BL
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK666

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

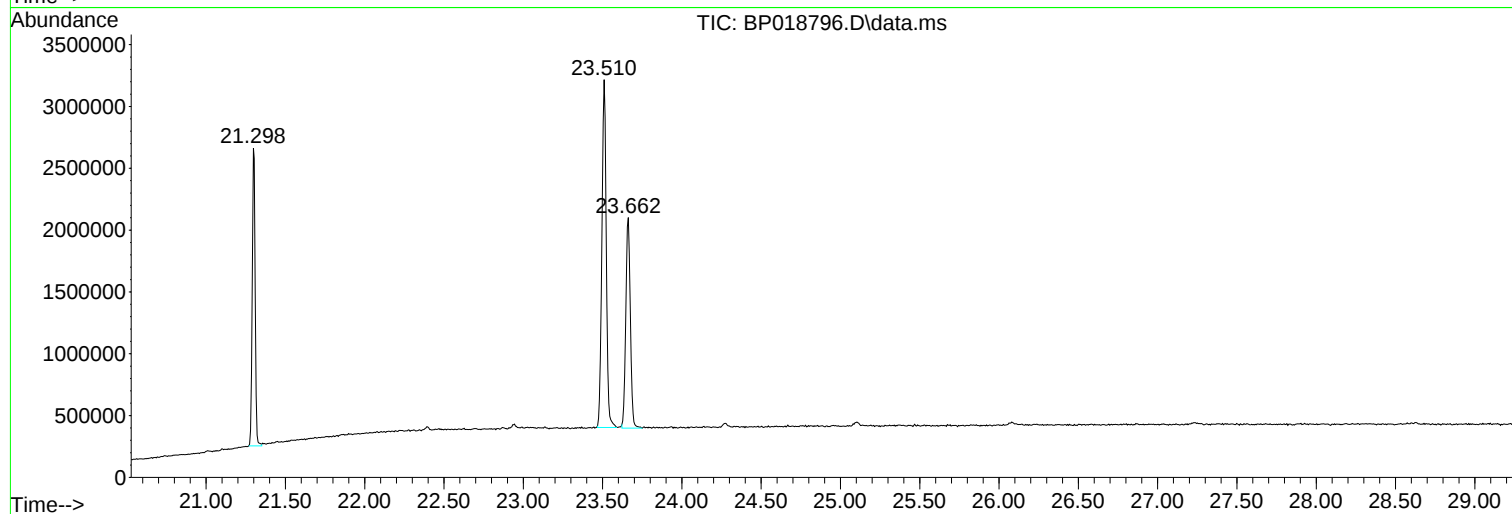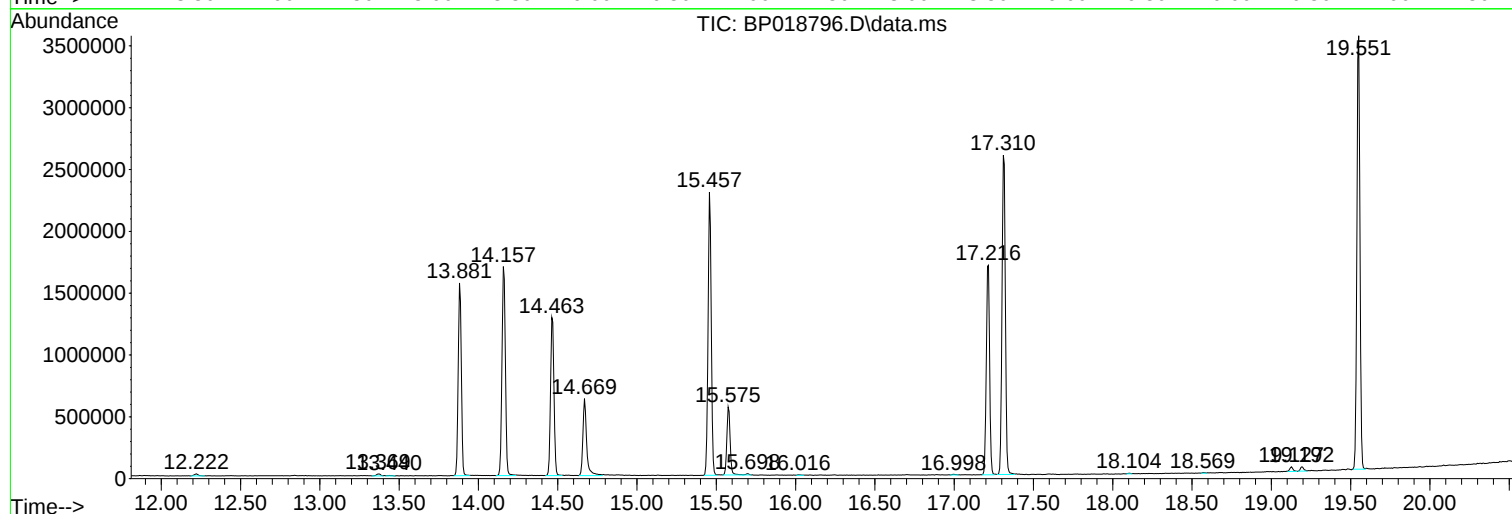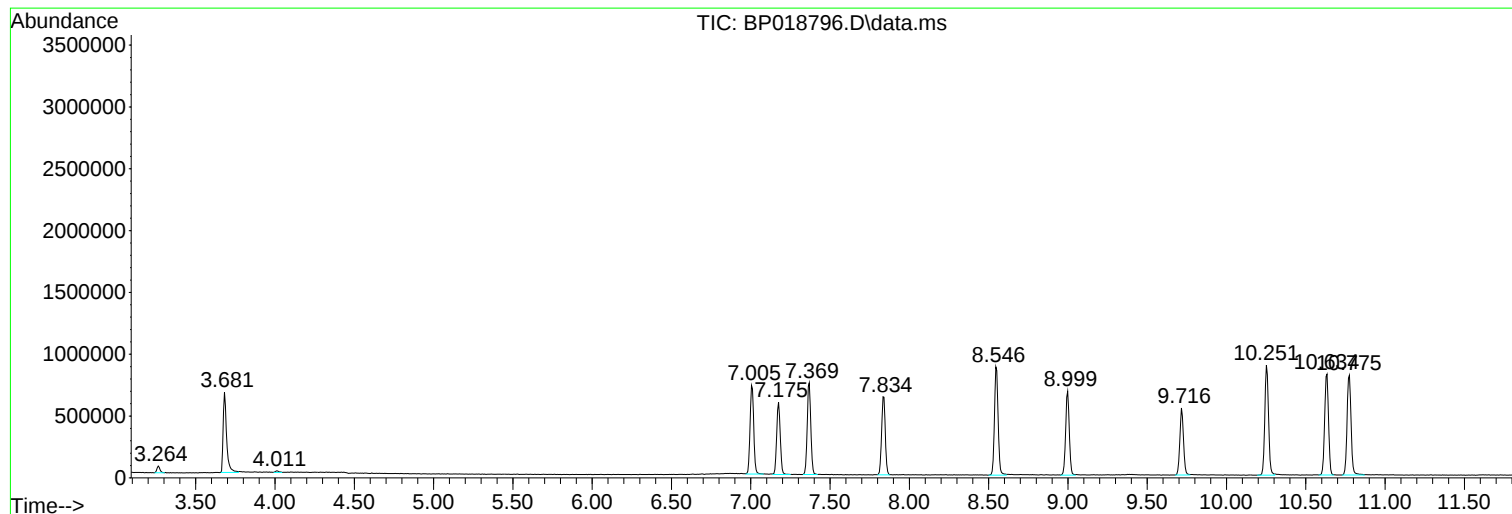

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018796.D
Acq On : 13 Dec 2023 08:08
Operator : MA/JU
Sample : PB157666BL
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK666

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018796.D
Acq On : 13 Dec 2023 08:08
Operator : MA/JU
Sample : PB157666BL
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK666

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------