

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018797.D
 Acq On : 13 Dec 2023 08:42
 Operator : MA/JU
 Sample : 05673-01
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHEH8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018797.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	20	25	27	rBV	28623	45279	0.70%	0.087%
2	3.264	27	30	40	rVB	43293	62704	0.96%	0.121%
3	3.687	98	102	118	rBV	207267	339223	5.21%	0.654%
4	3.916	138	141	146	rVB4	13717	19144	0.29%	0.037%
5	4.016	154	158	162	rVB2	12979	17436	0.27%	0.034%
6	4.540	240	247	263	rVB	3112116	4910747	75.38%	9.470%
7	7.005	661	666	678	rVB	153160	246640	3.79%	0.476%
8	7.175	688	695	703	rBV	585862	885116	13.59%	1.707%
9	7.369	720	728	740	rBV	580852	901688	13.84%	1.739%
10	7.840	799	808	816	rBV	621487	996683	15.30%	1.922%
11	7.904	816	819	824	rVB6	4765	6646	0.10%	0.013%
12	8.546	920	928	938	rBV	444082	708845	10.88%	1.367%
13	8.999	997	1005	1014	rBV	693820	1094759	16.80%	2.111%
14	9.410	1071	1075	1082	rVB8	5373	11954	0.18%	0.023%
15	9.716	1120	1127	1141	rBV	528421	849840	13.04%	1.639%
16	9.946	1164	1166	1173	rBV8	3092	6765	0.10%	0.013%
17	10.251	1208	1218	1232	rBV	821979	1366355	20.97%	2.635%
18	10.634	1276	1283	1290	rBV	787797	1326379	20.36%	2.558%
19	10.775	1299	1307	1315	rBV	716439	1237019	18.99%	2.386%
20	11.904	1491	1499	1505	rBV6	5808	10377	0.16%	0.020%
21	12.216	1548	1552	1561	rVB	15107	26166	0.40%	0.050%
22	12.434	1583	1589	1593	rBV9	3672	8058	0.12%	0.016%
23	13.298	1732	1736	1741	rVB6	6205	9056	0.14%	0.017%
24	13.369	1741	1748	1753	rVV2	17556	30112	0.46%	0.058%
25	13.434	1754	1759	1764	rVB9	4244	7448	0.11%	0.014%
26	13.881	1827	1835	1846	rBV	1666641	2252859	34.58%	4.345%
27	14.087	1866	1870	1875	rBV7	5927	12084	0.19%	0.023%
28	14.157	1875	1882	1894	rVV	1761052	2544244	39.05%	4.906%
29	14.463	1928	1934	1945	rBV	1215694	1841902	28.27%	3.552%
30	14.669	1964	1969	1982	rBV	103691	203222	3.12%	0.392%
31	14.886	2001	2006	2011	rBV8	8401	16939	0.26%	0.033%
32	15.457	2096	2103	2116	rBV	2427733	3419415	52.49%	6.594%
33	15.575	2117	2123	2139	rVV	704820	977800	15.01%	1.886%
34	15.698	2140	2144	2148	rVB5	12153	17547	0.27%	0.034%
35	17.216	2395	2402	2409	rBV	1653550	2379523	36.52%	4.589%
36	17.310	2412	2418	2436	rVB	3013681	4283977	65.76%	8.262%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018797.D
Acq On : 13 Dec 2023 08:42
Operator : MA/JU
Sample : 05673-01
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHEH8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	18.104	2548	2553	2559	rBV2	81709	116180	1.78%	0.224%
38	19.122	2723	2726	2732	rBV2	45172	59254	0.91%	0.114%
39	19.192	2734	2738	2742	rBV	52683	68325	1.05%	0.132%
40	19.339	2759	2763	2770	rBV3	47344	59933	0.92%	0.116%
41	19.551	2793	2799	2805	rBV	4259474	5571592	85.52%	10.745%
42	21.298	3091	3096	3106	rBV	2373153	3081846	47.30%	5.943%
43	23.510	3465	3472	3489	rVB	3356399	6514931	100.00%	12.564%
44	23.662	3492	3498	3508	rVB	1692602	3308672	50.79%	6.381%




Sum of corrected areas: 51854684

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018797.D
Acq On : 13 Dec 2023 08:42
Operator : MA/JU
Sample : 05673-01
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHEH8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

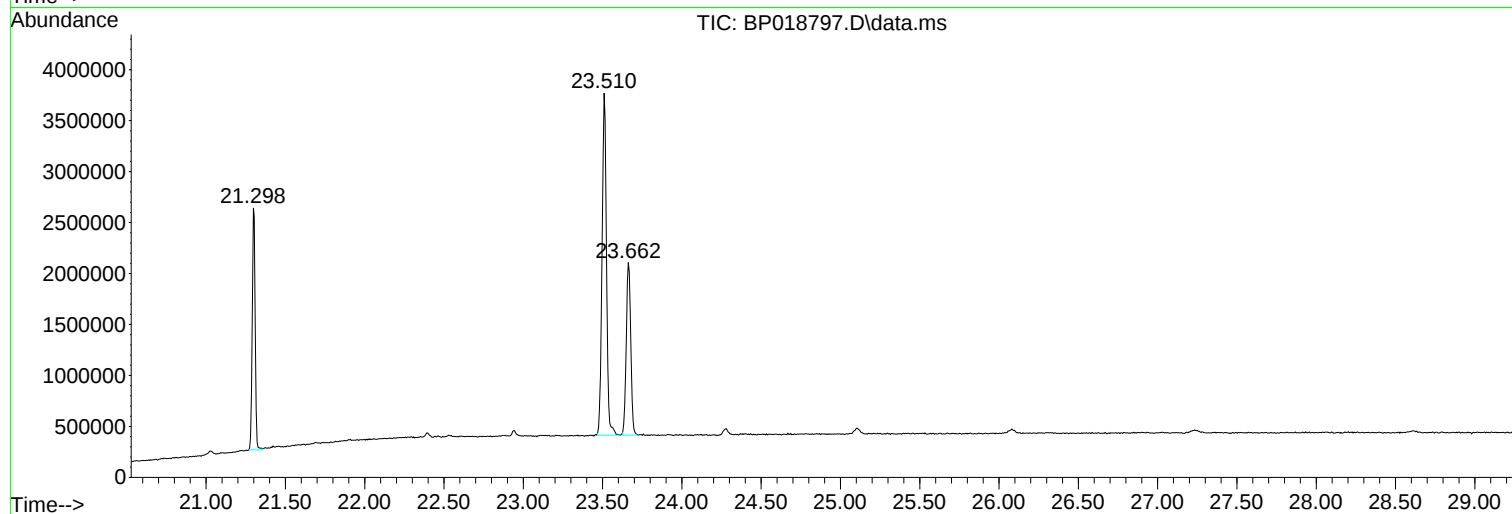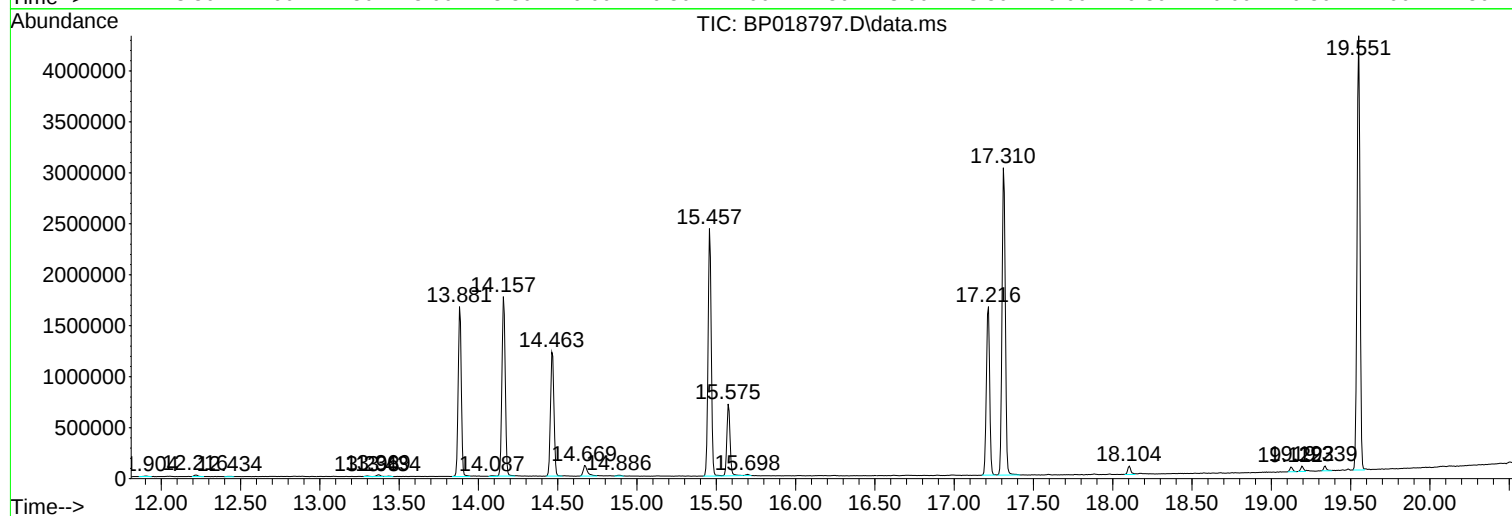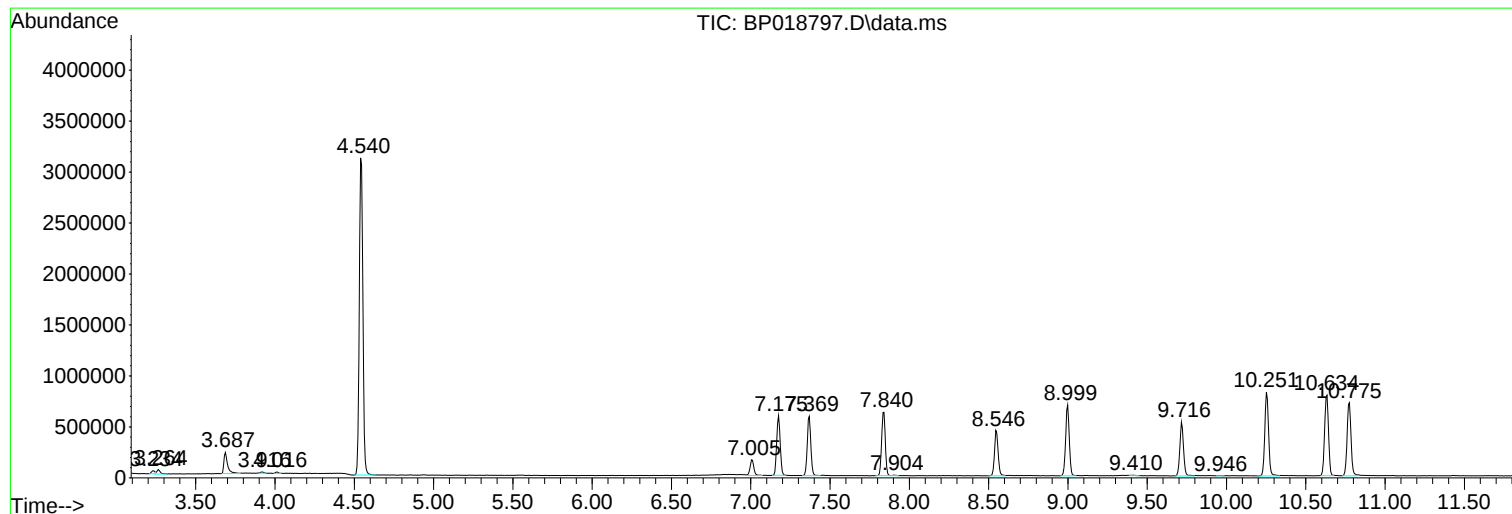

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018797.D
Acq On : 13 Dec 2023 08:42
Operator : MA/JU
Sample : 05673-01
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHEH8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018797.D
Acq On : 13 Dec 2023 08:42
Operator : MA/JU
Sample : 05673-01
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHEH8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc