

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018801.D
 Acq On : 13 Dec 2023 10:57
 Operator : MA/JU
 Sample : 05673-05
 Misc :
 ALS Vial : 81 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHEJ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018801.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	20	25	27	rBV4	26307	43202	0.68%	0.083%
2	3.264	27	30	38	rVB	42083	58534	0.92%	0.113%
3	3.687	98	102	112	rBV	197028	314145	4.94%	0.605%
4	3.917	137	141	145	rVB2	13236	22161	0.35%	0.043%
5	4.011	155	157	163	rVB	12363	13146	0.21%	0.025%
6	4.540	240	247	259	rBV	3245819	4945650	77.72%	9.519%
7	7.005	661	666	677	rVB	156926	248094	3.90%	0.478%
8	7.175	688	695	703	rVB	607614	936272	14.71%	1.802%
9	7.364	720	727	737	rBV	582500	923291	14.51%	1.777%
10	7.464	741	744	750	rVB7	4519	7673	0.12%	0.015%
11	7.834	799	807	816	rBV	628248	979666	15.39%	1.886%
12	8.546	921	928	939	rBV	466779	727277	11.43%	1.400%
13	8.999	995	1005	1012	rBV	713269	1152564	18.11%	2.218%
14	9.340	1057	1063	1064	rBV6	5162	6680	0.10%	0.013%
15	9.411	1067	1075	1083	rVB	26132	51275	0.81%	0.099%
16	9.716	1119	1127	1138	rBV	536698	869502	13.66%	1.674%
17	10.252	1209	1218	1231	rBV	866324	1416504	22.26%	2.726%
18	10.628	1275	1282	1289	rBV	773204	1289379	20.26%	2.482%
19	10.769	1298	1306	1318	rBV	753410	1312247	20.62%	2.526%
20	11.905	1491	1499	1505	rBV2	33341	51443	0.81%	0.099%
21	12.040	1512	1522	1528	rVB2	4753	11245	0.18%	0.022%
22	12.222	1546	1553	1559	rVB3	15652	30393	0.48%	0.059%
23	13.369	1742	1748	1753	rBV2	14808	23479	0.37%	0.045%
24	13.881	1828	1835	1847	rBV	1713287	2358027	37.05%	4.539%
25	14.093	1865	1871	1874	rBV8	5728	11094	0.17%	0.021%
26	14.157	1875	1882	1900	rVB	1874068	2721328	42.76%	5.238%
27	14.463	1927	1934	1943	rBV	1191660	1763215	27.71%	3.394%
28	14.675	1963	1970	1982	rBV	93639	191575	3.01%	0.369%
29	14.893	2005	2007	2012	rVB6	6527	7074	0.11%	0.014%
30	15.140	2043	2049	2053	rVB9	3346	7040	0.11%	0.014%
31	15.457	2096	2103	2116	rBV	2504556	3609254	56.72%	6.947%
32	15.575	2117	2123	2137	rVV	684610	951407	14.95%	1.831%
33	15.698	2139	2144	2149	rVB3	13760	25190	0.40%	0.048%
34	16.240	2230	2236	2240	rBV9	5357	10753	0.17%	0.021%
35	16.992	2359	2364	2366	rBV5	4872	8610	0.14%	0.017%
36	17.210	2395	2401	2412	rBV	1633571	2301461	36.17%	4.430%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018801.D
 Acq On : 13 Dec 2023 10:57
 Operator : MA/JU
 Sample : 05673-05
 Misc :
 ALS Vial : 81 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHEJ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	17.310	2412	2418	2433	rVV	3016041	4257380	66.90%	8.195%
38	17.981	2528	2532	2535	rBV6	3730	6803	0.11%	0.013%
39	18.104	2548	2553	2559	rBV3	52806	73713	1.16%	0.142%
40	19.128	2723	2727	2732	rVB2	42330	54906	0.86%	0.106%
41	19.192	2734	2738	2742	rBV	46400	66437	1.04%	0.128%
42	19.339	2759	2763	2767	rBV2	29923	42846	0.67%	0.082%
43	19.551	2793	2799	2806	rBV	4100911	5456711	85.75%	10.503%
44	21.298	3091	3096	3102	rBV	2307640	2988097	46.96%	5.751%
45	23.510	3465	3472	3488	rVB2	3233299	6363654	100.00%	12.249%
46	23.663	3491	3498	3509	rVB	1653677	3243030	50.96%	6.242%




Sum of corrected areas: 51953427

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018801.D
Acq On : 13 Dec 2023 10:57
Operator : MA/JU
Sample : 05673-05
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHEJ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

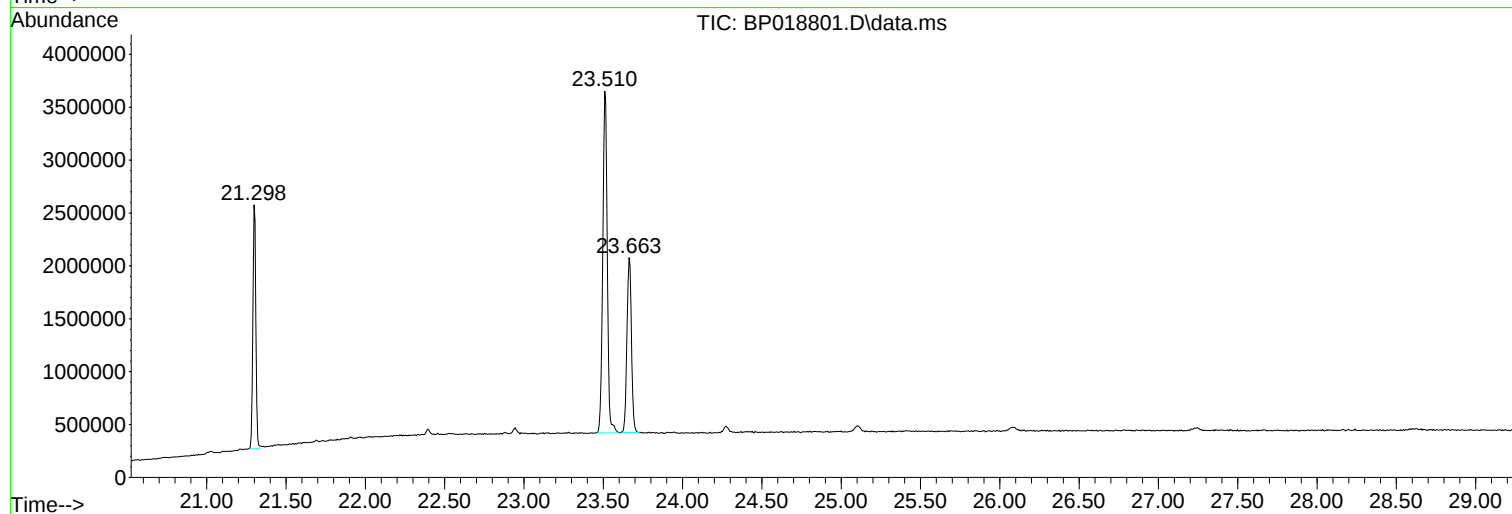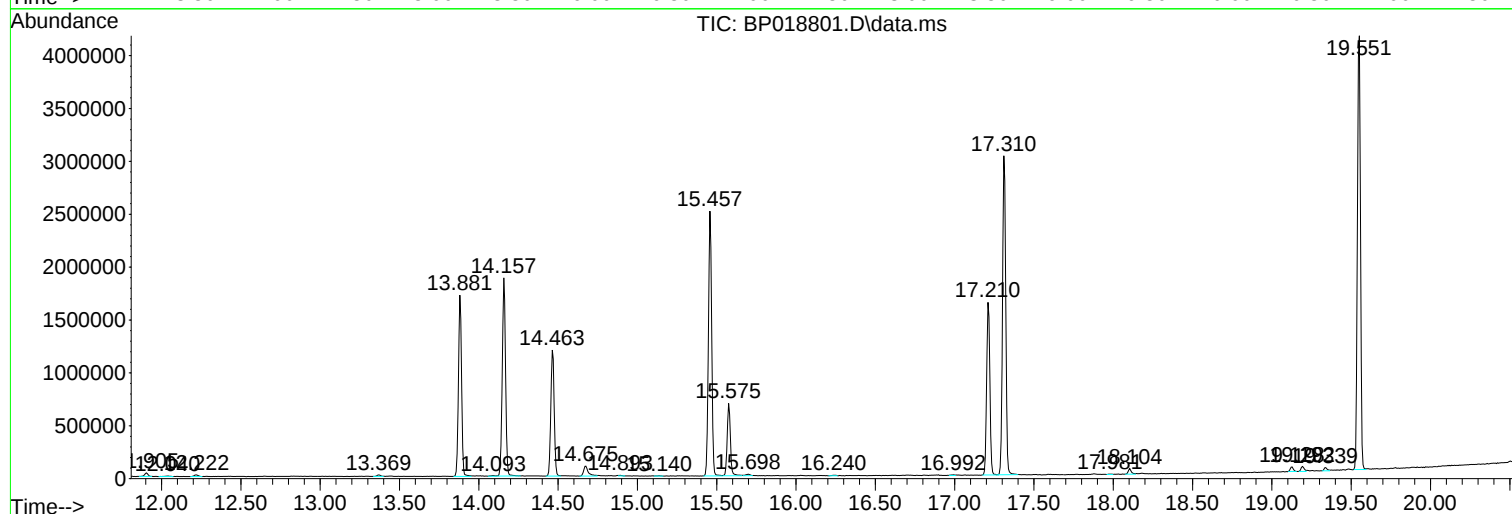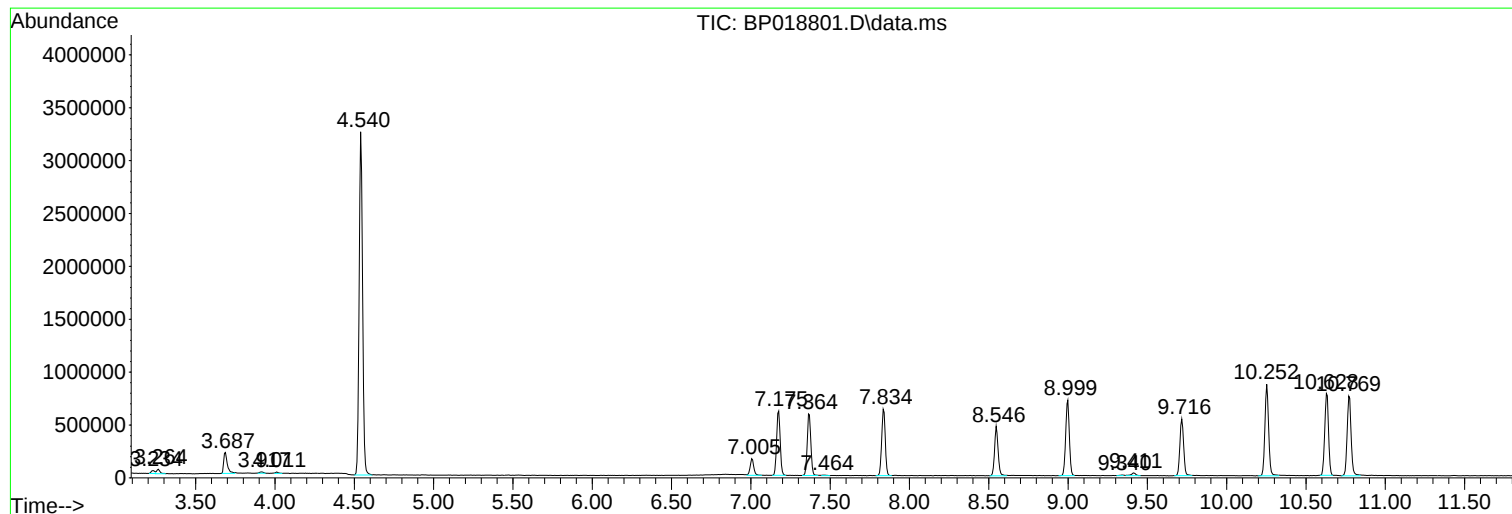

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018801.D
Acq On : 13 Dec 2023 10:57
Operator : MA/JU
Sample : 05673-05
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHEJ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018801.D
Acq On : 13 Dec 2023 10:57
Operator : MA/JU
Sample : 05673-05
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHEJ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc