

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018804.D
 Acq On : 13 Dec 2023 12:39
 Operator : MA/JU
 Sample : 05675-20
 Misc :
 ALS Vial : 84 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018804.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	19	24	28	rBV	77104	123820	1.86%	0.241%
2	3.264	28	30	33	rVV	41556	46158	0.69%	0.090%
3	3.299	33	36	43	rVB	31486	42265	0.64%	0.082%
4	3.687	97	102	115	rBV	205584	340536	5.13%	0.662%
5	3.917	137	141	146	rVB	13456	22026	0.33%	0.043%
6	4.011	153	157	161	rVB	12671	17663	0.27%	0.034%
7	4.540	241	247	256	rBV	575905	843572	12.70%	1.639%
8	4.934	310	314	322	rVB8	4454	11512	0.17%	0.022%
9	7.005	660	666	676	rVB	157443	242900	3.66%	0.472%
10	7.175	688	695	702	rBV	622618	986711	14.85%	1.917%
11	7.363	721	727	739	rBV	598780	955120	14.38%	1.856%
12	7.452	740	742	748	rVB7	4930	7701	0.12%	0.015%
13	7.834	799	807	818	rBV	710408	1111016	16.72%	2.159%
14	8.546	922	928	943	rBV	449847	729587	10.98%	1.417%
15	8.993	998	1004	1012	rBV	730180	1177045	17.72%	2.287%
16	9.405	1071	1074	1082	rVB9	5168	9134	0.14%	0.018%
17	9.716	1119	1127	1138	rBV	540808	876172	13.19%	1.702%
18	10.252	1211	1218	1231	rBV	874329	1427392	21.49%	2.773%
19	10.628	1272	1282	1291	rBV	908756	1487387	22.39%	2.890%
20	10.769	1295	1306	1320	rBV	774873	1371747	20.65%	2.665%
21	11.381	1405	1410	1416	rBV4	8617	19202	0.29%	0.037%
22	12.057	1519	1525	1530	rVB6	6936	13162	0.20%	0.026%
23	12.216	1546	1552	1558	rBV	18204	31130	0.47%	0.060%
24	13.293	1732	1735	1740	rBV4	6791	8180	0.12%	0.016%
25	13.369	1743	1748	1753	rBV3	14580	20644	0.31%	0.040%
26	13.881	1827	1835	1849	rBV	1816096	2460238	37.03%	4.780%
27	14.157	1872	1882	1895	rBV	1851663	2801416	42.17%	5.443%
28	14.463	1928	1934	1944	rBV	1402240	2019849	30.40%	3.924%
29	14.675	1963	1970	1985	rBV	95338	205872	3.10%	0.400%
30	14.881	2002	2005	2012	rVB9	7050	11795	0.18%	0.023%
31	15.457	2096	2103	2117	rBV	2718912	3830865	57.66%	7.443%
32	15.575	2117	2123	2138	rVV	720177	990518	14.91%	1.924%
33	15.692	2138	2143	2149	rVB3	14904	24179	0.36%	0.047%
34	16.887	2343	2346	2351	rBV7	6246	9445	0.14%	0.018%
35	17.210	2395	2401	2410	rBV	1830440	2658275	40.01%	5.165%
36	17.310	2412	2418	2430	rBV2	3215253	4722516	71.09%	9.175%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018804.D
 Acq On : 13 Dec 2023 12:39
 Operator : MA/JU
 Sample : 05675-20
 Misc :
 ALS Vial : 84 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	18.104	2549	2553	2559	rBV	79911	100479	1.51%	0.195%
38	18.186	2563	2567	2572	rVB3	14406	22379	0.34%	0.043%
39	19.128	2723	2727	2731	rBV2	49053	65216	0.98%	0.127%
40	19.192	2734	2738	2742	rBV	47642	66345	1.00%	0.129%
41	19.339	2759	2763	2767	rBV4	47896	63987	0.96%	0.124%
42	19.551	2793	2799	2806	rBV	4639675	5954395	89.63%	11.568%
43	21.304	3091	3097	3103	rBV	2568775	3339525	50.27%	6.488%
44	23.516	3465	3473	3488	rVB	3450080	6643406	100.00%	12.907%
45	23.669	3492	3499	3509	rVB	1782316	3558443	53.56%	6.914%




Sum of corrected areas: 51470925

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018804.D
Acq On : 13 Dec 2023 12:39
Operator : MA/JU
Sample : 05675-20
Misc :
ALS Vial : 84 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

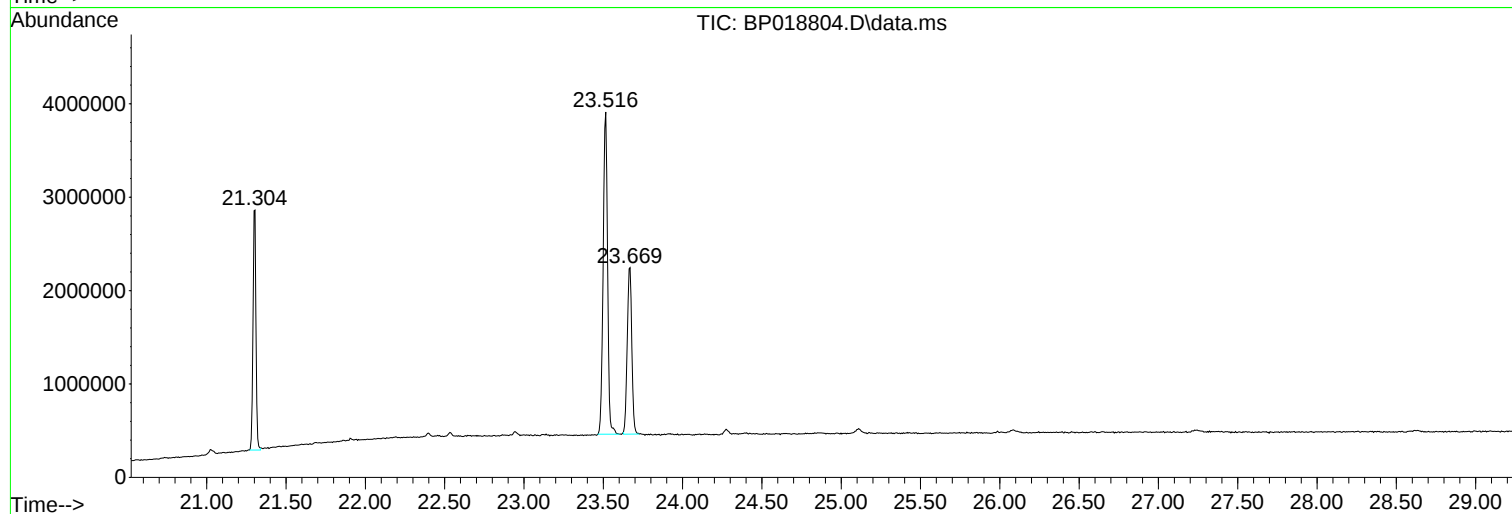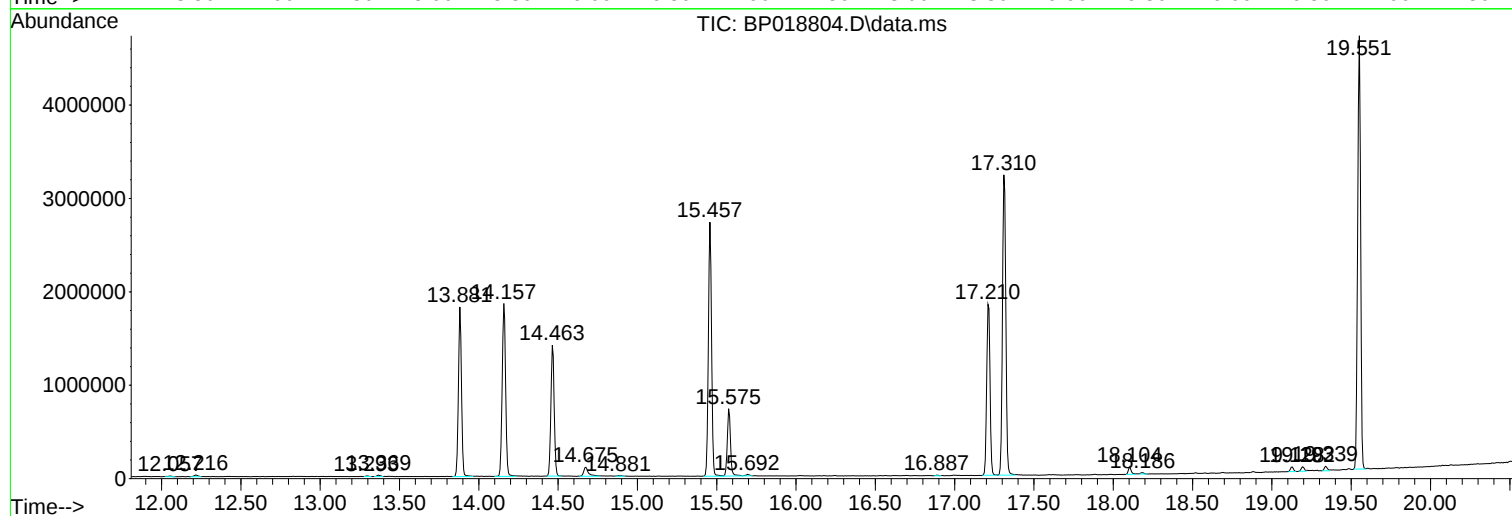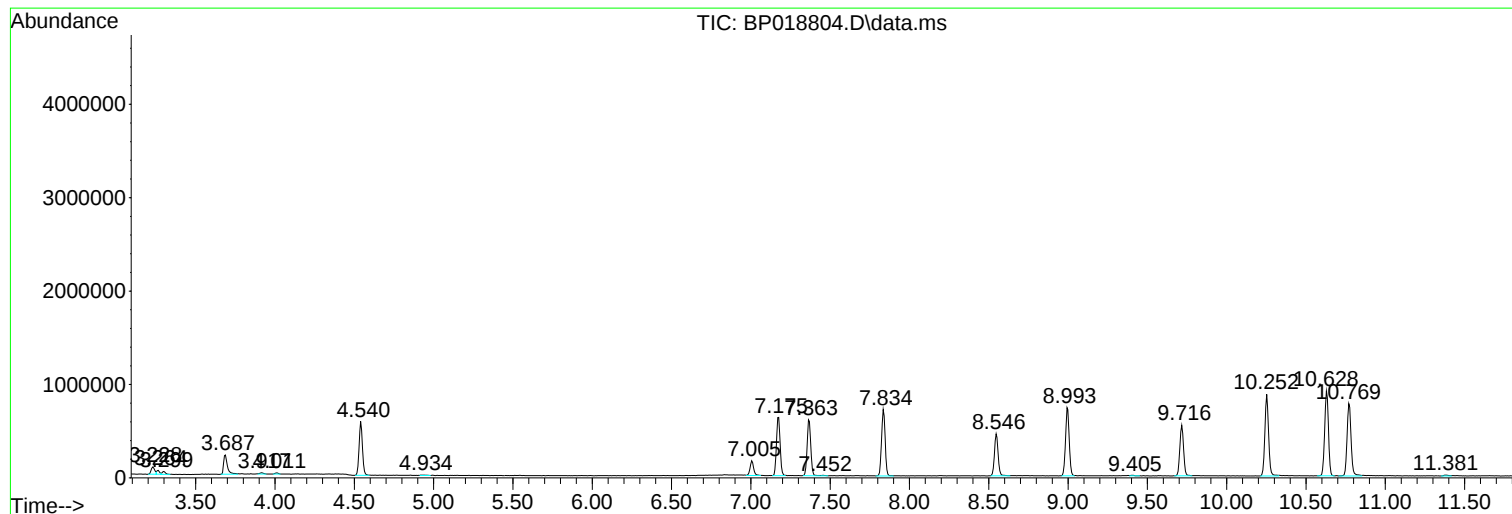

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018804.D
Acq On : 13 Dec 2023 12:39
Operator : MA/JU
Sample : 05675-20
Misc :
ALS Vial : 84 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018804.D
Acq On : 13 Dec 2023 12:39
Operator : MA/JU
Sample : 05675-20
Misc :
ALS Vial : 84 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc