

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018806.D
 Acq On : 13 Dec 2023 13:47
 Operator : MA/JU
 Sample : 05626-23
 Misc :
 ALS Vial : 86 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLG8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018806.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	38	rVB	56724	75164	0.91%	0.119%
2	3.687	98	102	118	rBV	222780	381188	4.62%	0.605%
3	3.917	137	141	147	rVB2	20584	33313	0.40%	0.053%
4	4.011	153	157	162	rBV2	19412	28830	0.35%	0.046%
5	4.934	311	314	321	rVB6	4859	8471	0.10%	0.013%
6	6.487	574	578	584	rVB6	7890	11577	0.14%	0.018%
7	7.005	661	666	675	rVB	229731	348053	4.22%	0.552%
8	7.175	688	695	704	rVB	877339	1367000	16.57%	2.170%
9	7.363	720	727	735	rBV	818487	1281546	15.54%	2.034%
10	7.458	740	743	749	rVB7	6978	9282	0.11%	0.015%
11	7.834	799	807	815	rBV	847179	1324781	16.06%	2.103%
12	8.546	922	928	940	rBV	623920	988680	11.99%	1.569%
13	8.934	991	994	997	rBV5	6221	8904	0.11%	0.014%
14	8.999	997	1005	1013	rVV	957933	1566027	18.99%	2.486%
15	9.716	1120	1127	1140	rBV	694610	1116523	13.54%	1.772%
16	10.251	1211	1218	1230	rBV	1138038	1896862	23.00%	3.011%
17	10.416	1242	1246	1253	rVB9	6120	12375	0.15%	0.020%
18	10.551	1265	1269	1274	rBV8	5521	10714	0.13%	0.017%
19	10.628	1274	1282	1290	rBV	1081517	1818226	22.04%	2.886%
20	10.769	1297	1306	1322	rBV	958489	1683541	20.41%	2.672%
21	11.287	1387	1394	1401	rVB3	10160	20087	0.24%	0.032%
22	12.134	1534	1538	1544	rVB5	5665	8594	0.10%	0.014%
23	12.216	1546	1552	1557	rBV2	22818	39056	0.47%	0.062%
24	12.469	1592	1595	1601	rVB	8191	13011	0.16%	0.021%
25	12.828	1650	1656	1663	rBV7	11601	23273	0.28%	0.037%
26	13.081	1692	1699	1707	rVB4	20532	33711	0.41%	0.054%
27	13.369	1743	1748	1755	rBV	90852	145028	1.76%	0.230%
28	13.440	1755	1760	1766	rVB8	5054	11537	0.14%	0.018%
29	13.881	1828	1835	1847	rBV	2370640	3216780	39.00%	5.106%
30	14.157	1873	1882	1890	rBV	2576000	3758980	45.57%	5.967%
31	14.463	1926	1934	1942	rBV	1677426	2478921	30.05%	3.935%
32	14.675	1964	1970	1983	rBV2	117298	245553	2.98%	0.390%
33	14.892	2004	2007	2012	rBV7	9664	13236	0.16%	0.021%
34	15.139	2045	2049	2054	rVB8	5155	9488	0.12%	0.015%
35	15.292	2071	2075	2077	rVB2	8595	9939	0.12%	0.016%
36	15.457	2095	2103	2117	rBV	3610904	5267070	63.85%	8.360%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018806.D
 Acq On : 13 Dec 2023 13:47
 Operator : MA/JU
 Sample : 05626-23
 Misc :
 ALS Vial : 86 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLG8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	15.575	2117	2123	2132	rBV	744957	1020349	12.37%	1.620%
38	15.698	2140	2144	2149	rVB4	16806	25599	0.31%	0.041%
39	15.828	2162	2166	2173	rVB8	8316	14192	0.17%	0.023%
40	16.022	2192	2199	2206	rBV8	5682	13053	0.16%	0.021%
41	16.698	2309	2314	2316	rBV6	6167	8916	0.11%	0.014%
42	16.757	2320	2324	2327	rVV4	5402	8286	0.10%	0.013%
43	16.998	2359	2365	2370	rBV4	4498	10516	0.13%	0.017%
44	17.210	2395	2401	2410	rBV	1844463	2728964	33.08%	4.332%
45	17.310	2412	2418	2433	rVV	3929250	5578631	67.63%	8.855%
46	17.886	2511	2516	2521	rVB2	66604	85876	1.04%	0.136%
47	18.104	2548	2553	2559	rBV6	24442	45506	0.55%	0.072%
48	18.575	2629	2633	2635	rBV6	8786	11851	0.14%	0.019%
49	19.128	2722	2727	2733	rBV2	64047	93666	1.14%	0.149%
50	19.192	2734	2738	2743	rBV	60499	85158	1.03%	0.135%
51	19.339	2760	2763	2768	rVB5	17148	20381	0.25%	0.032%
52	19.551	2793	2799	2808	rBV	6355585	8011583	97.13%	12.717%
53	21.304	3091	3097	3107	rBV	2798946	3780987	45.84%	6.001%
54	23.515	3465	3473	3480	rBV2	4218014	8248506	100.00%	13.093%
55	23.663	3492	3498	3514	rVB	1981872	3943468	47.81%	6.259%




Sum of corrected areas: 63000809

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018806.D
Acq On : 13 Dec 2023 13:47
Operator : MA/JU
Sample : 05626-23
Misc :
ALS Vial : 86 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLG8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

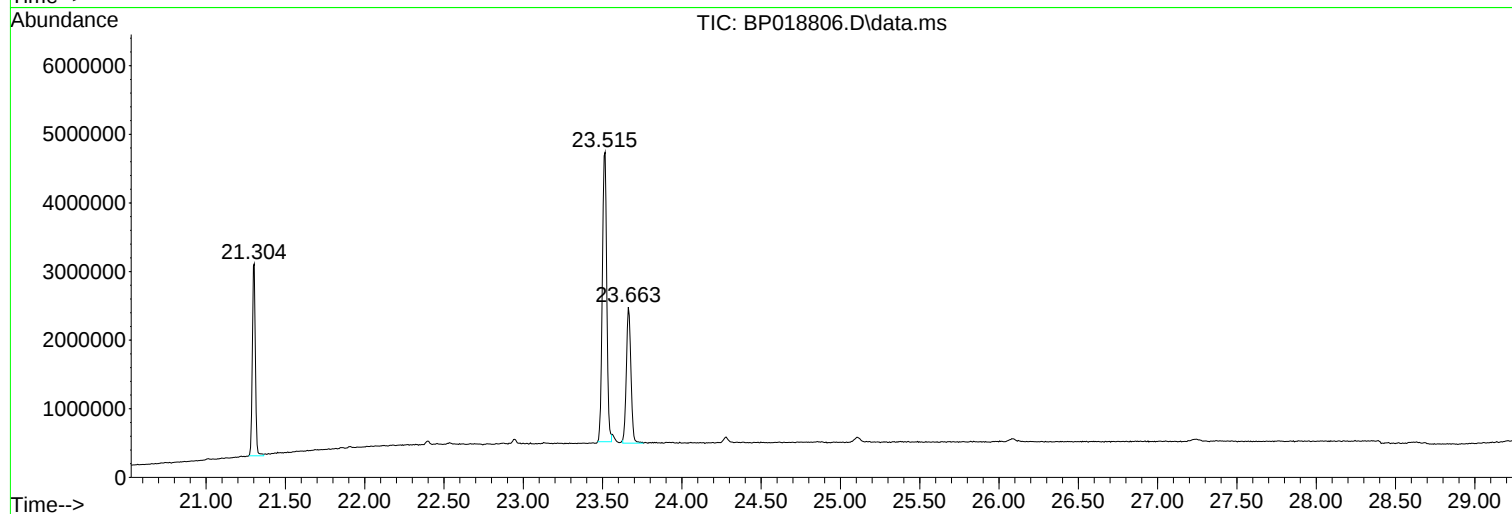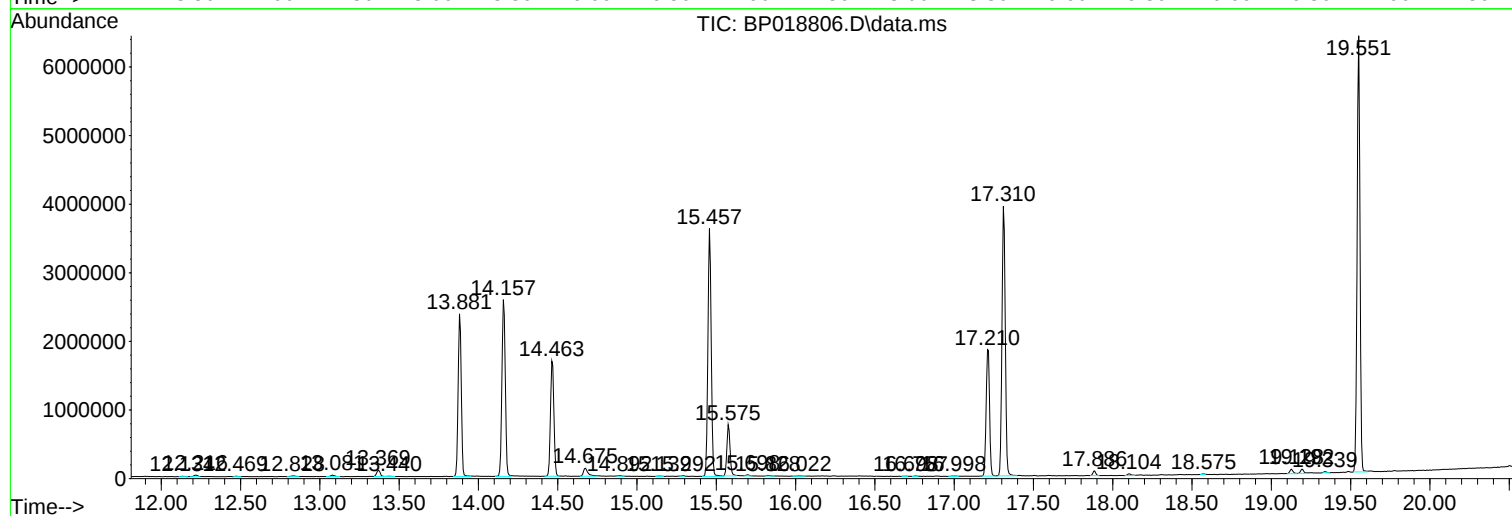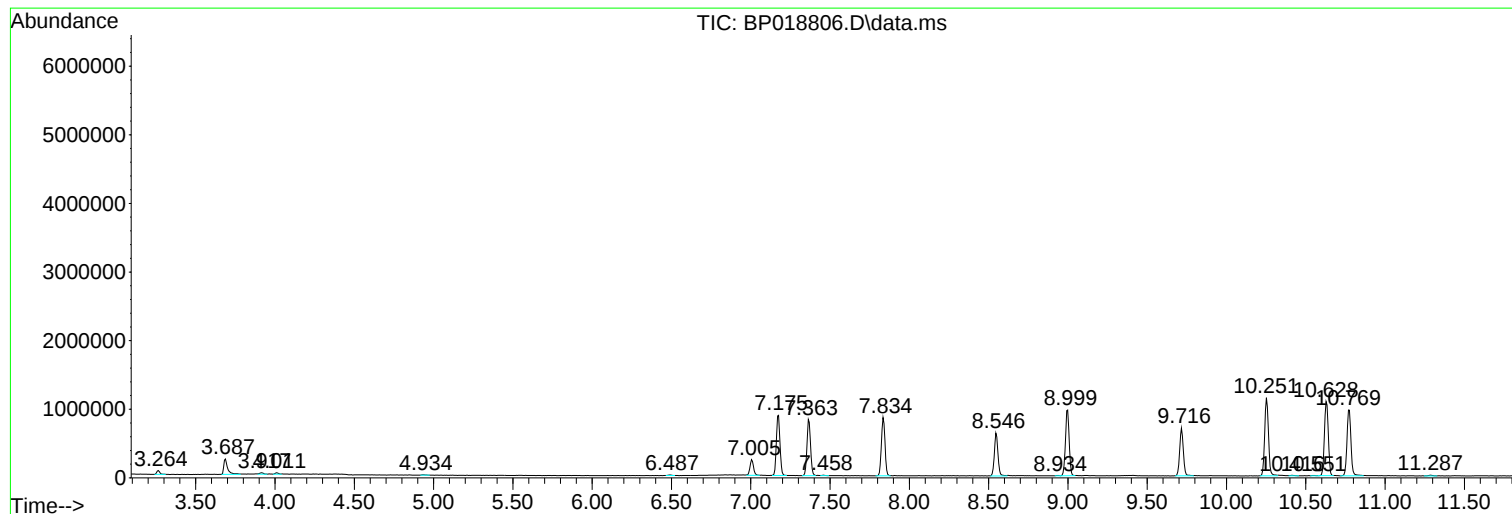

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018806.D
Acq On : 13 Dec 2023 13:47
Operator : MA/JU
Sample : 05626-23
Misc :
ALS Vial : 86 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLG8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018806.D
Acq On : 13 Dec 2023 13:47
Operator : MA/JU
Sample : 05626-23
Misc :
ALS Vial : 86 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLG8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc