
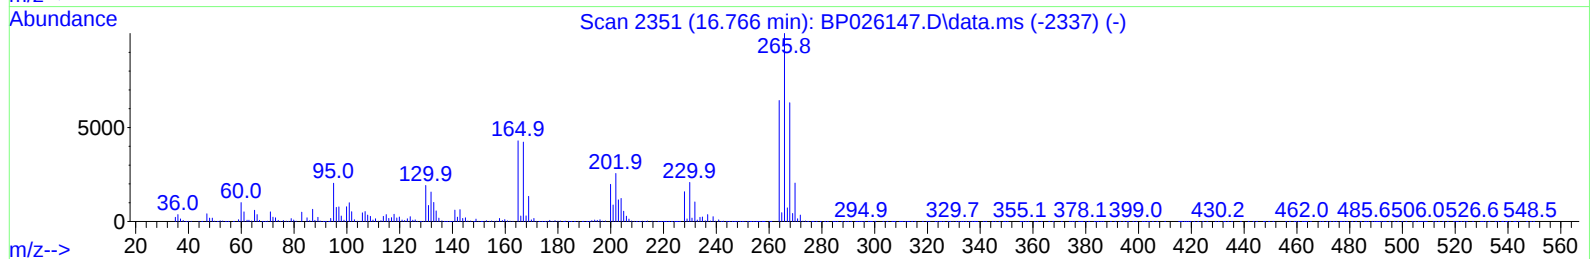
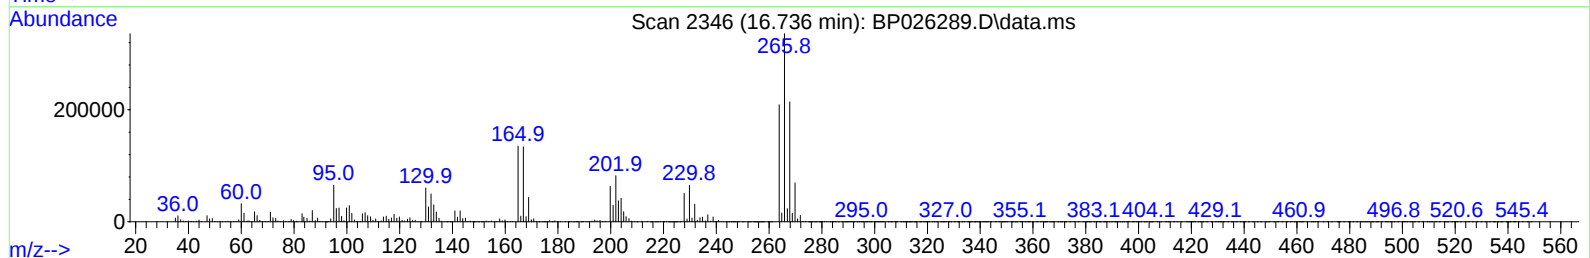


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121125\
Data File : BP026289.D
Acq On : 11 Dec 2025 12:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 11 12:51:22 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 05 14:52:44 2025
Response via : Initial Calibration

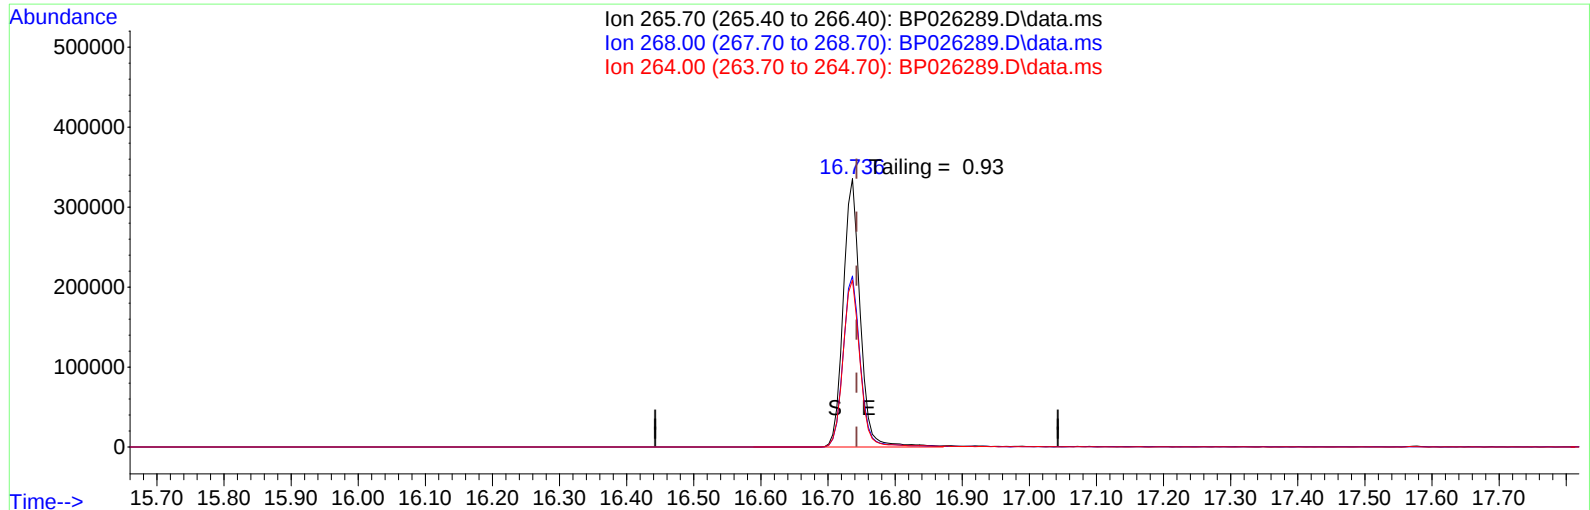

TIC: BP026289.D\data.ms

(70) Pentachlorophenol (C)




16.736min (-0.006) 123831.64 ng

response 584414

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.77
264.00	62.70	62.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121125\
Data File : BP026289.D
Acq On : 11 Dec 2025 12:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 11 12:51:22 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 05 14:52:44 2025
Response via : Initial Calibration

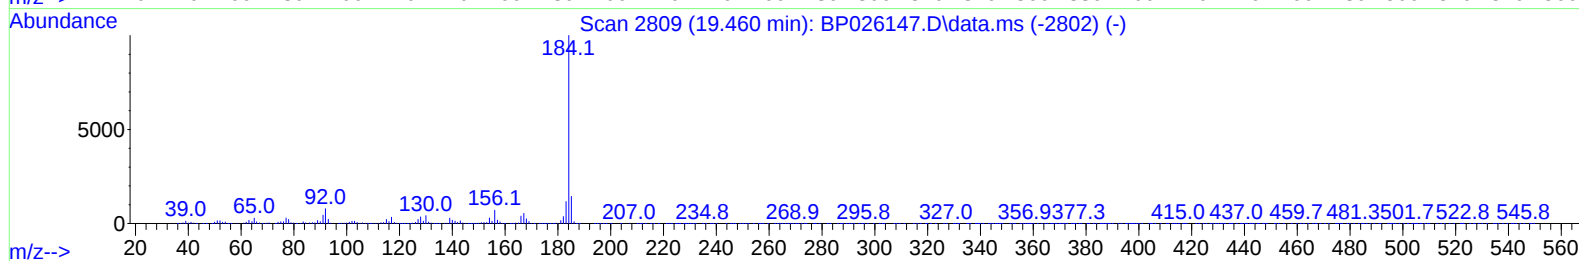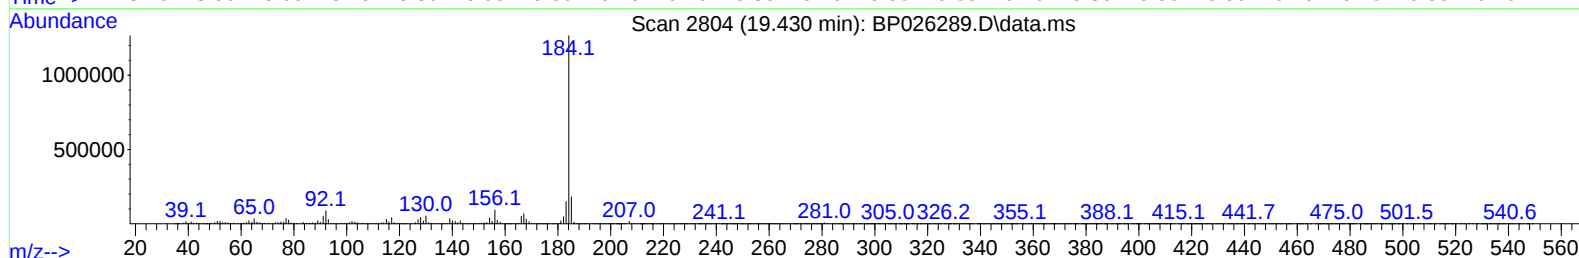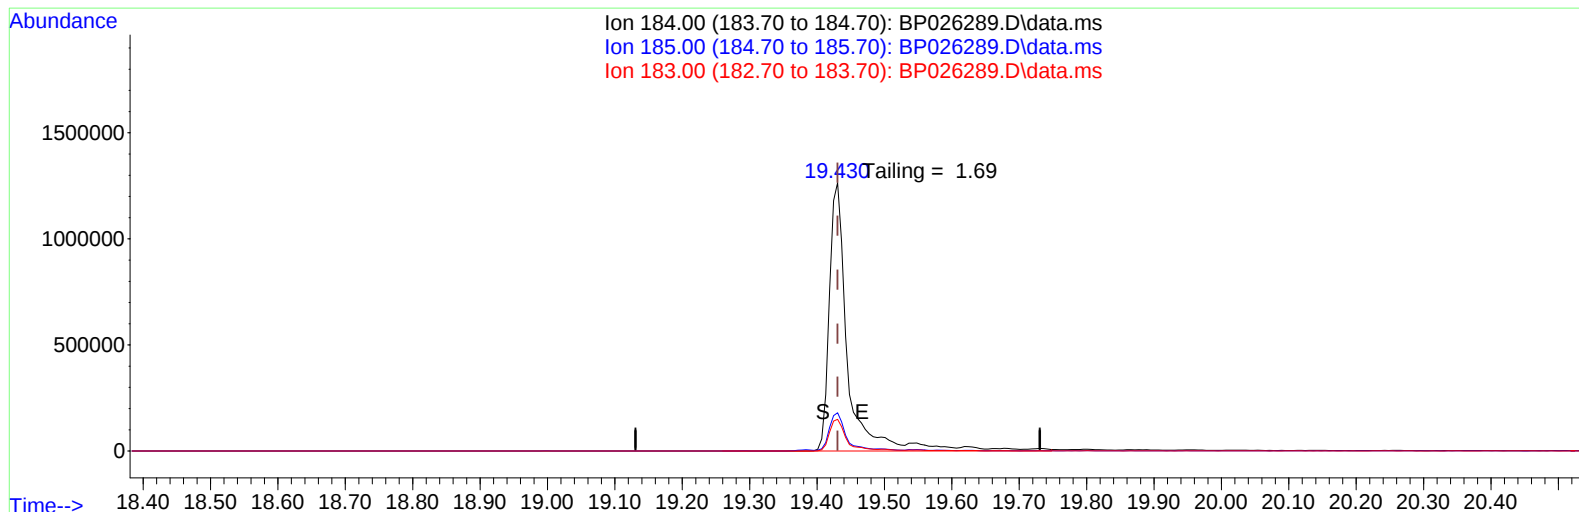

TIC: BP026289.D\data.ms

(77) Benzidine

19.430min (-0.000) 18777.43 ng

response 2264441

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.27
183.00	11.30	11.82
0.00	0.00	0.00