
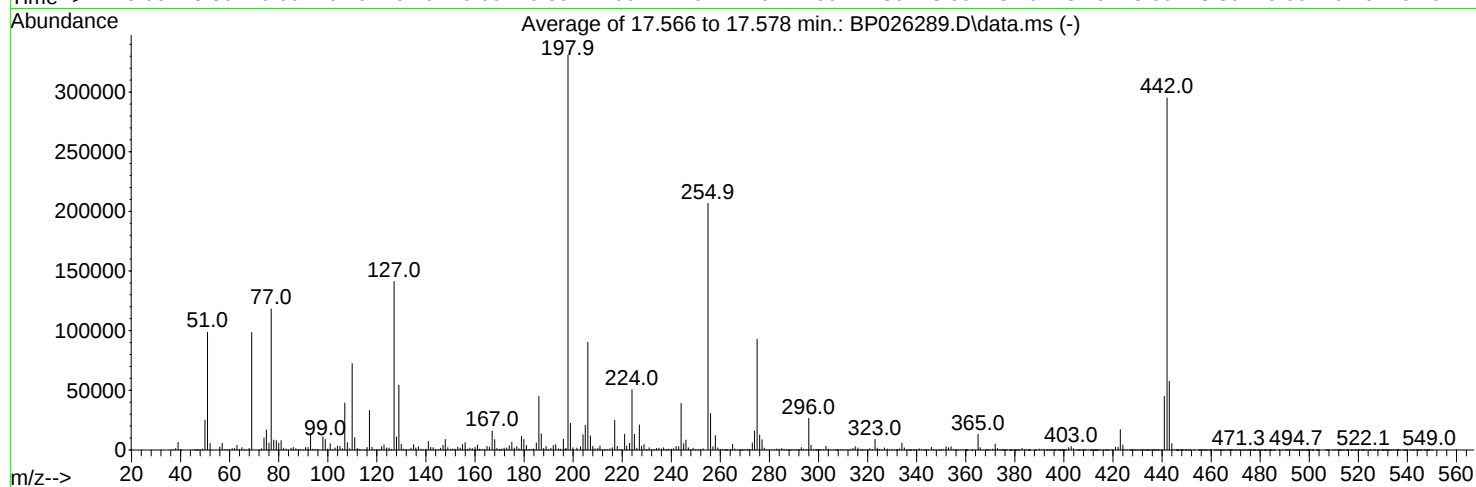


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121125\
Data File : BP026289.D
Acq On : 11 Dec 2025 12:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 05 14:52:44 2025

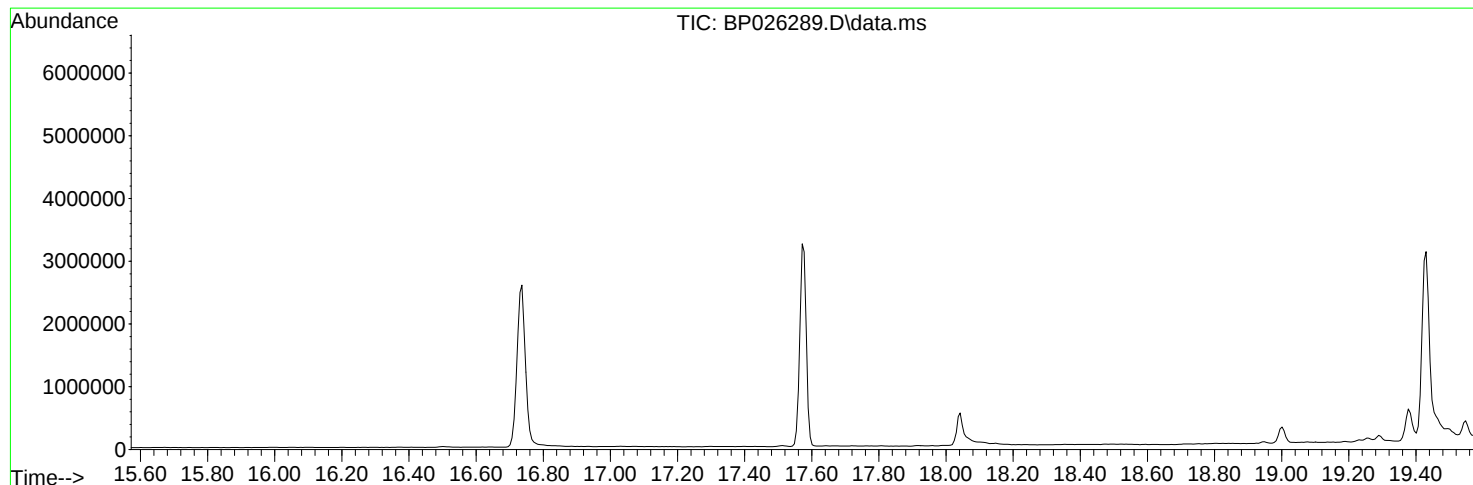




AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2479

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.3	1297	PASS
69	69	100	100	100.0	98463	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.4	1400	PASS
198	198	100	100	100.0	331012	PASS
199	198	5	9	6.7	22338	PASS
365	198	1	100	4.0	13114	PASS
441	443	0.01	150	78.0	44832	PASS
442	442	100	100	100.0	295099	PASS
443	442	15	24	19.5	57466	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121125\
Data File : BP026289.D
Acq On : 11 Dec 2025 12:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 11 12:51:22 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 05 14:52:44 2025
Response via : Initial Calibration

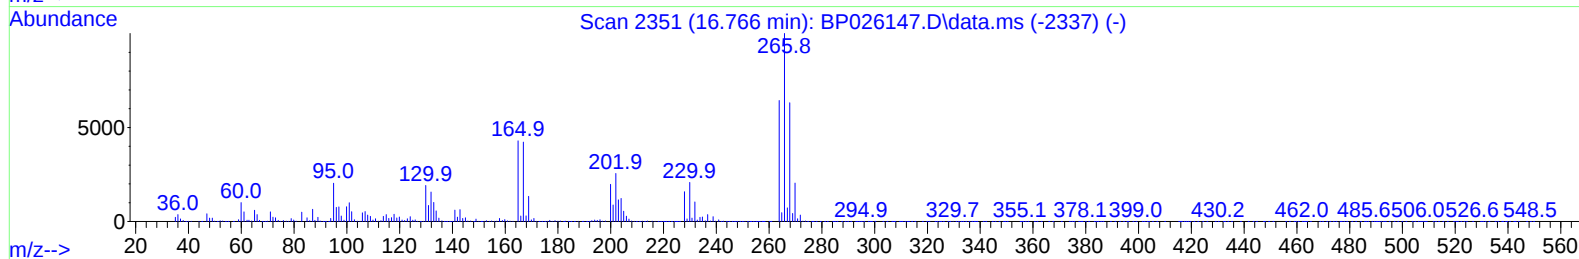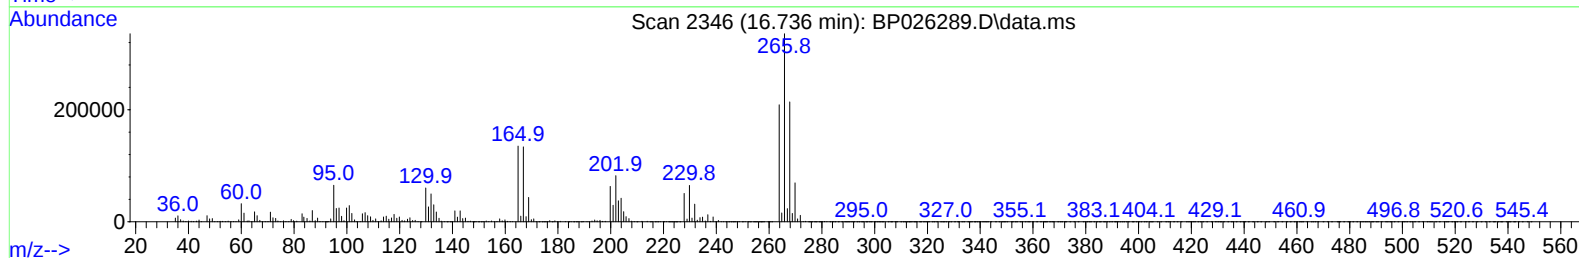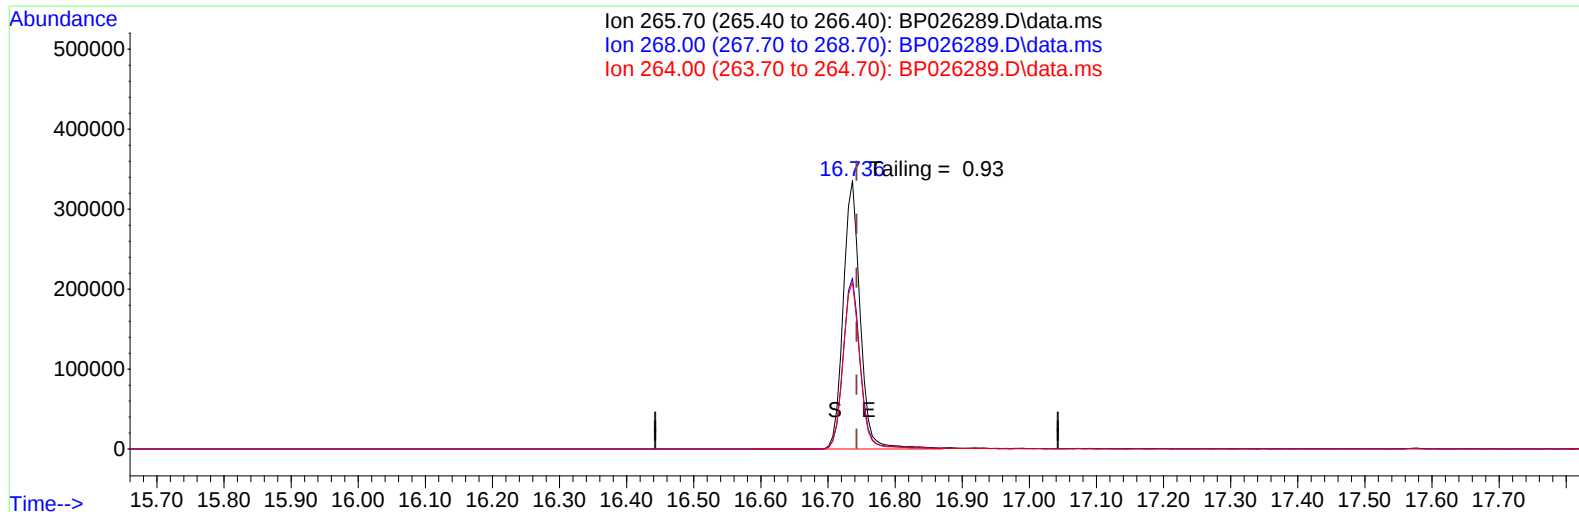

TIC: BP026289.D\data.ms

(70) Pentachlorophenol (C)

16.736min (-0.006) 123831.64 ng


response 584414

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.77
264.00	62.70	62.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121125\
Data File : BP026289.D
Acq On : 11 Dec 2025 12:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 11 12:51:22 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 05 14:52:44 2025
Response via : Initial Calibration

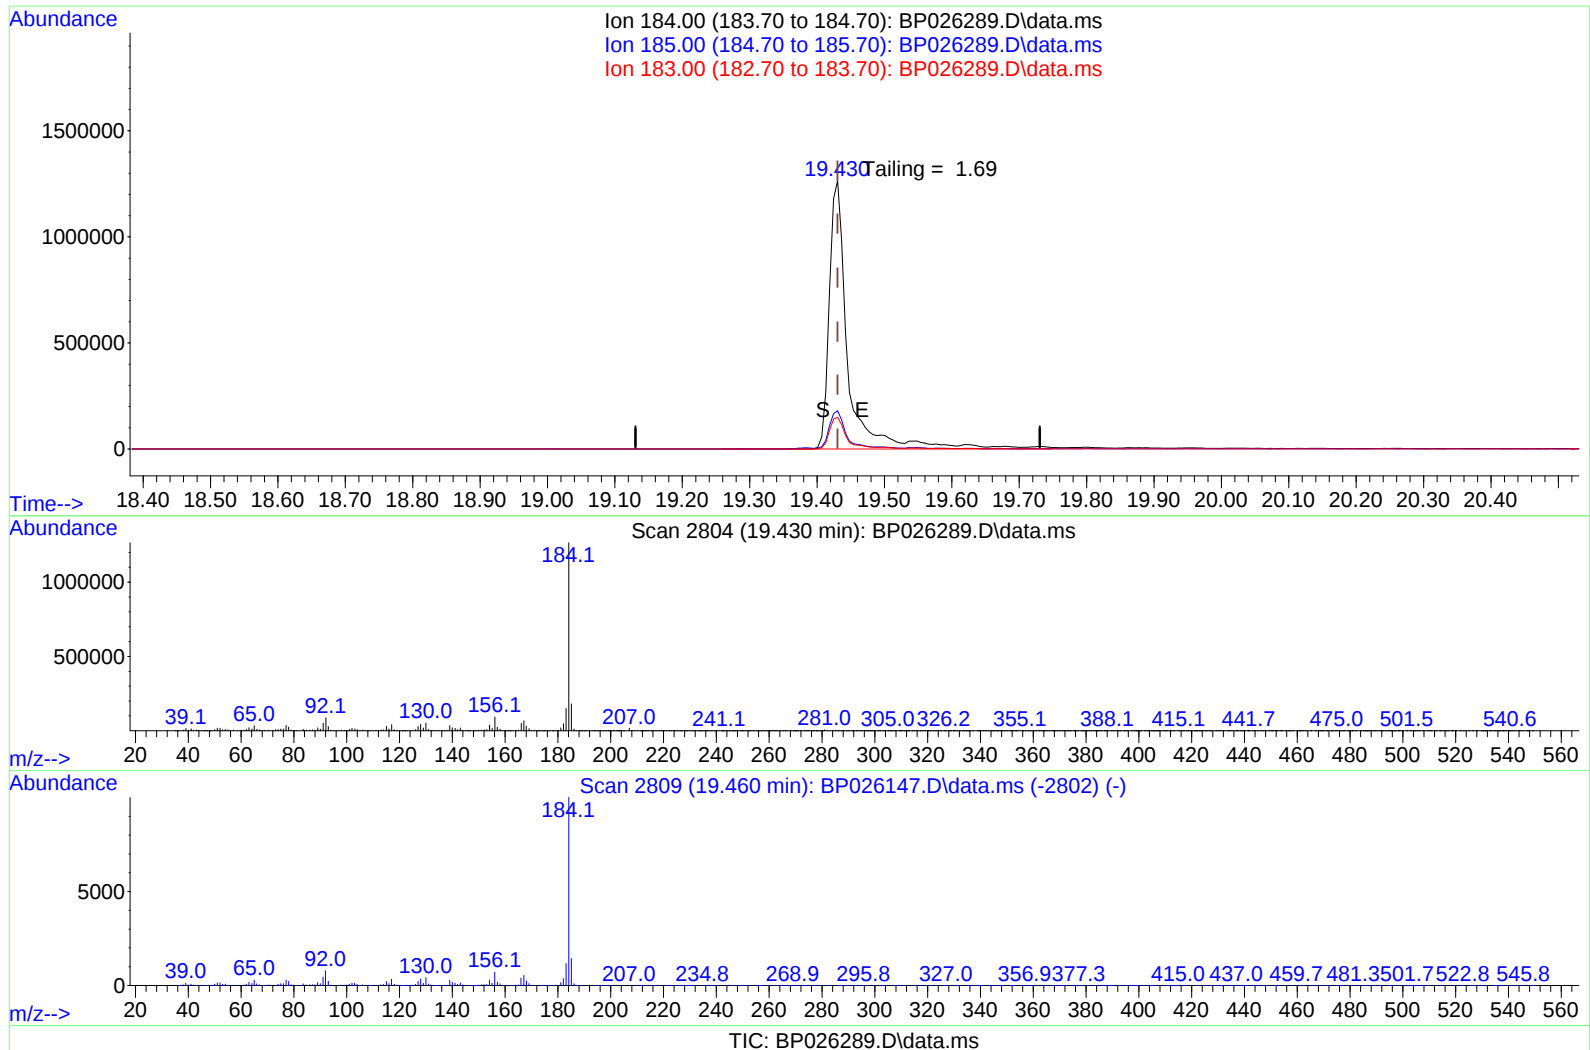

(77) Benzidine

19.430min (-0.000) 18777.43 ng

response 2264441

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.27
183.00	11.30	11.82
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/11/2025	BNA_P	<u>BP026289.D</u>
Compound Name	Response	Retention Time
DDT	1499546	20.724
DDD	46040	20.272
DDE	4378	19.736
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
50418	1549964	3.25

Instrument :
BNA_P
ClientSampleId :
DFTPP