
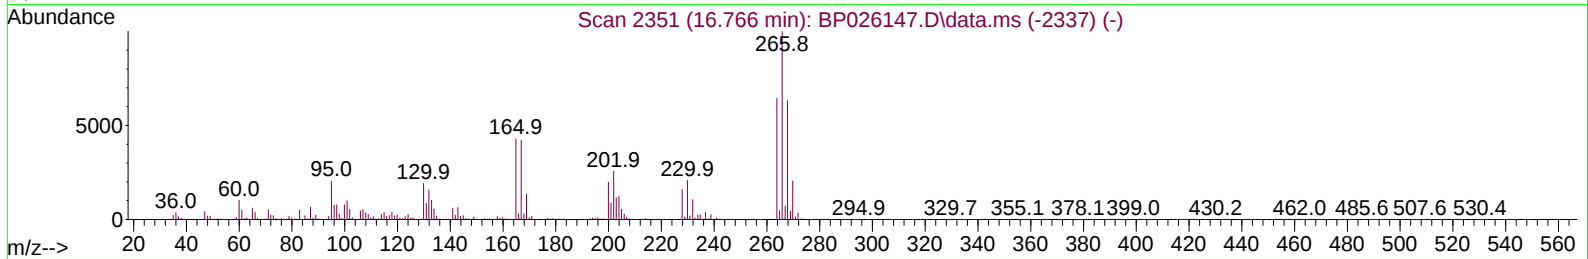
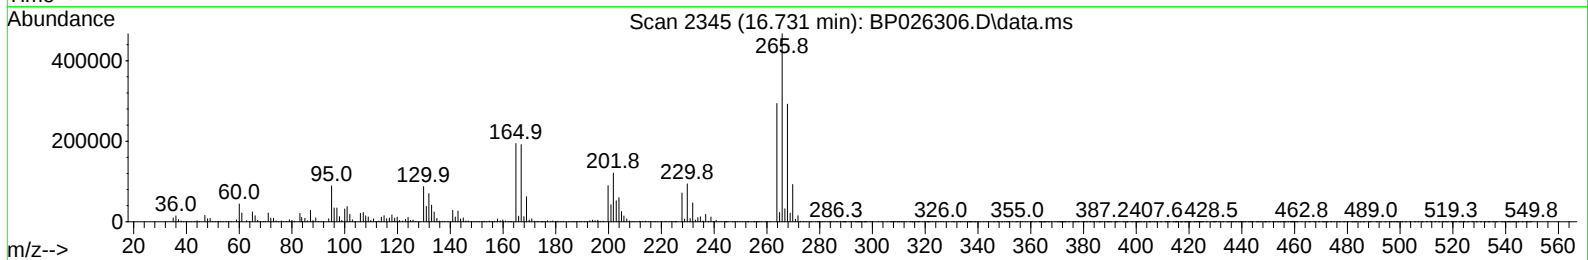


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121225\
Data File : BP026306.D
Acq On : 12 Dec 2025 10:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 12 10:54:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 05 14:52:44 2025
Response via : Initial Calibration

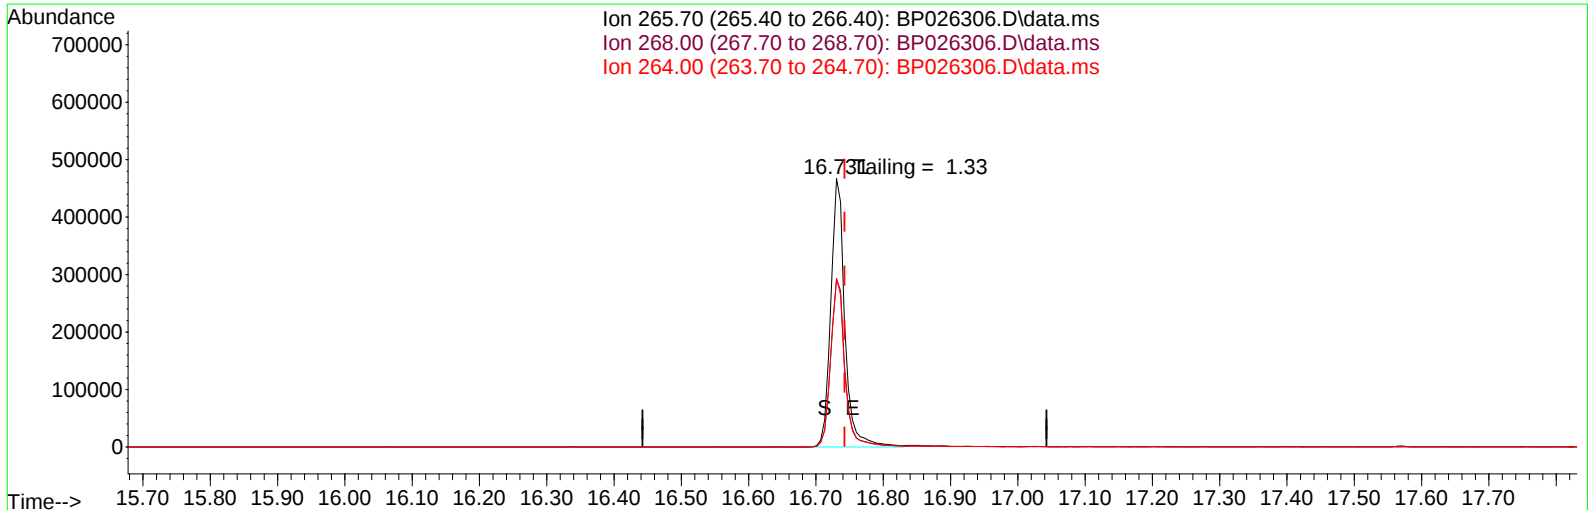

TIC: BP026306.D\data.ms

(70) Pentachlorophenol (C)




16.731min (-0.012) 122101.30 ng

response 677746

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.53
264.00	62.70	62.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121225\
Data File : BP026306.D
Acq On : 12 Dec 2025 10:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 12 10:54:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 05 14:52:44 2025
Response via : Initial Calibration

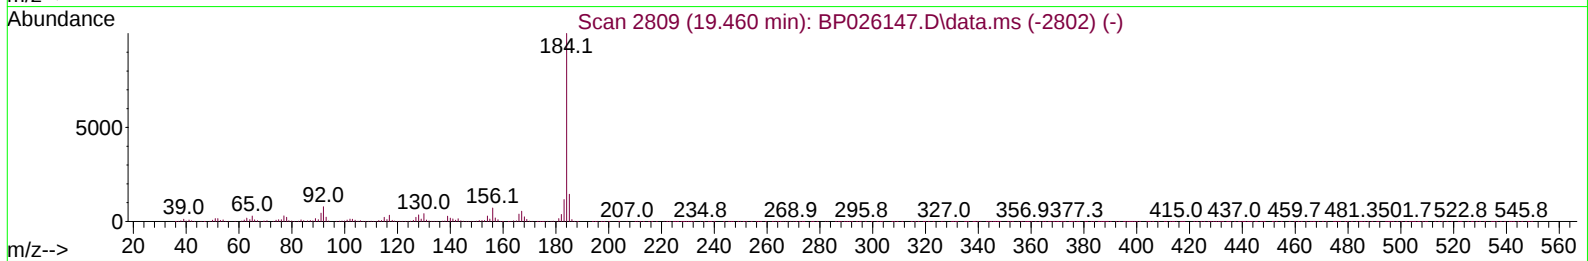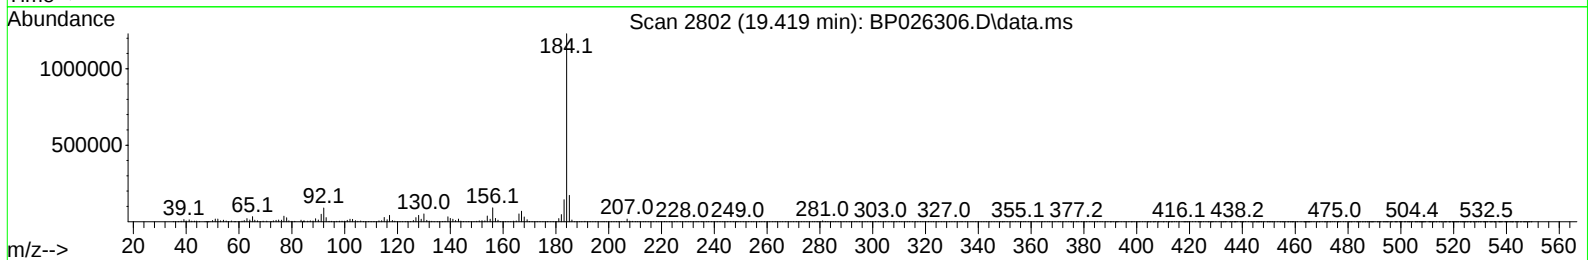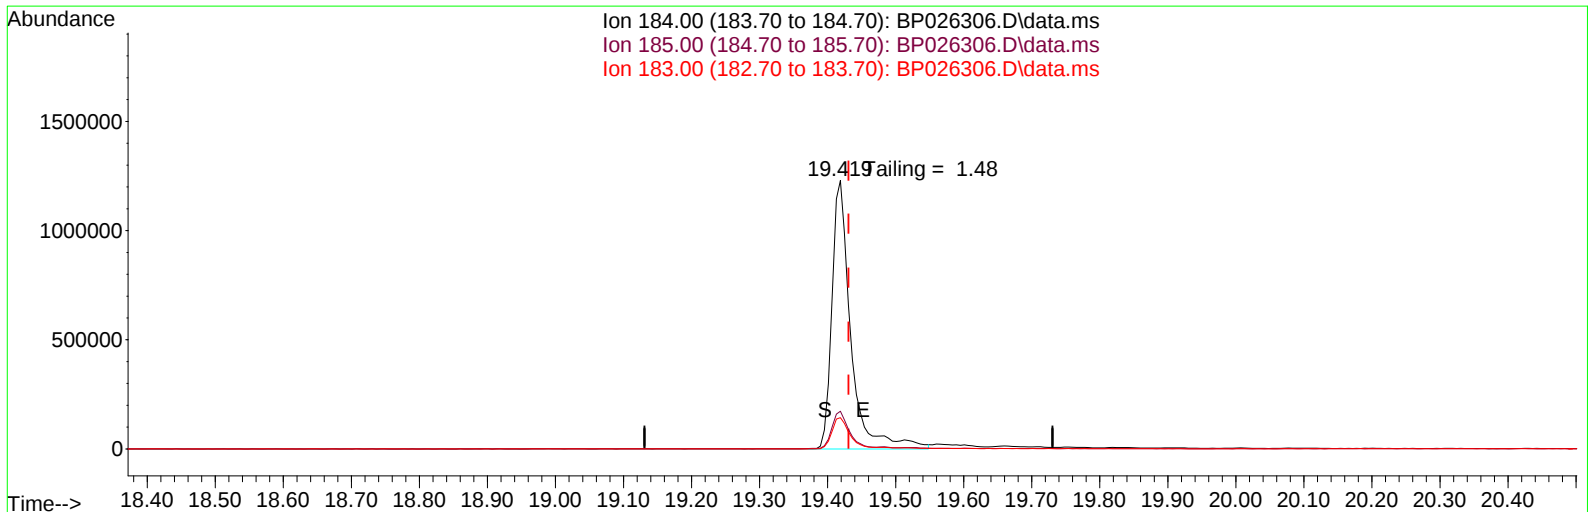

TIC: BP026306.D\data.ms

(77) Benzidine**19.419min (-0.012) 16192.53 ng****response 2291813**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.05
183.00	11.30	11.70
0.00	0.00	0.00