


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121225\
Data File : BP026306.D
Acq On : 12 Dec 2025 10:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Dec 15 01:38:31 2025

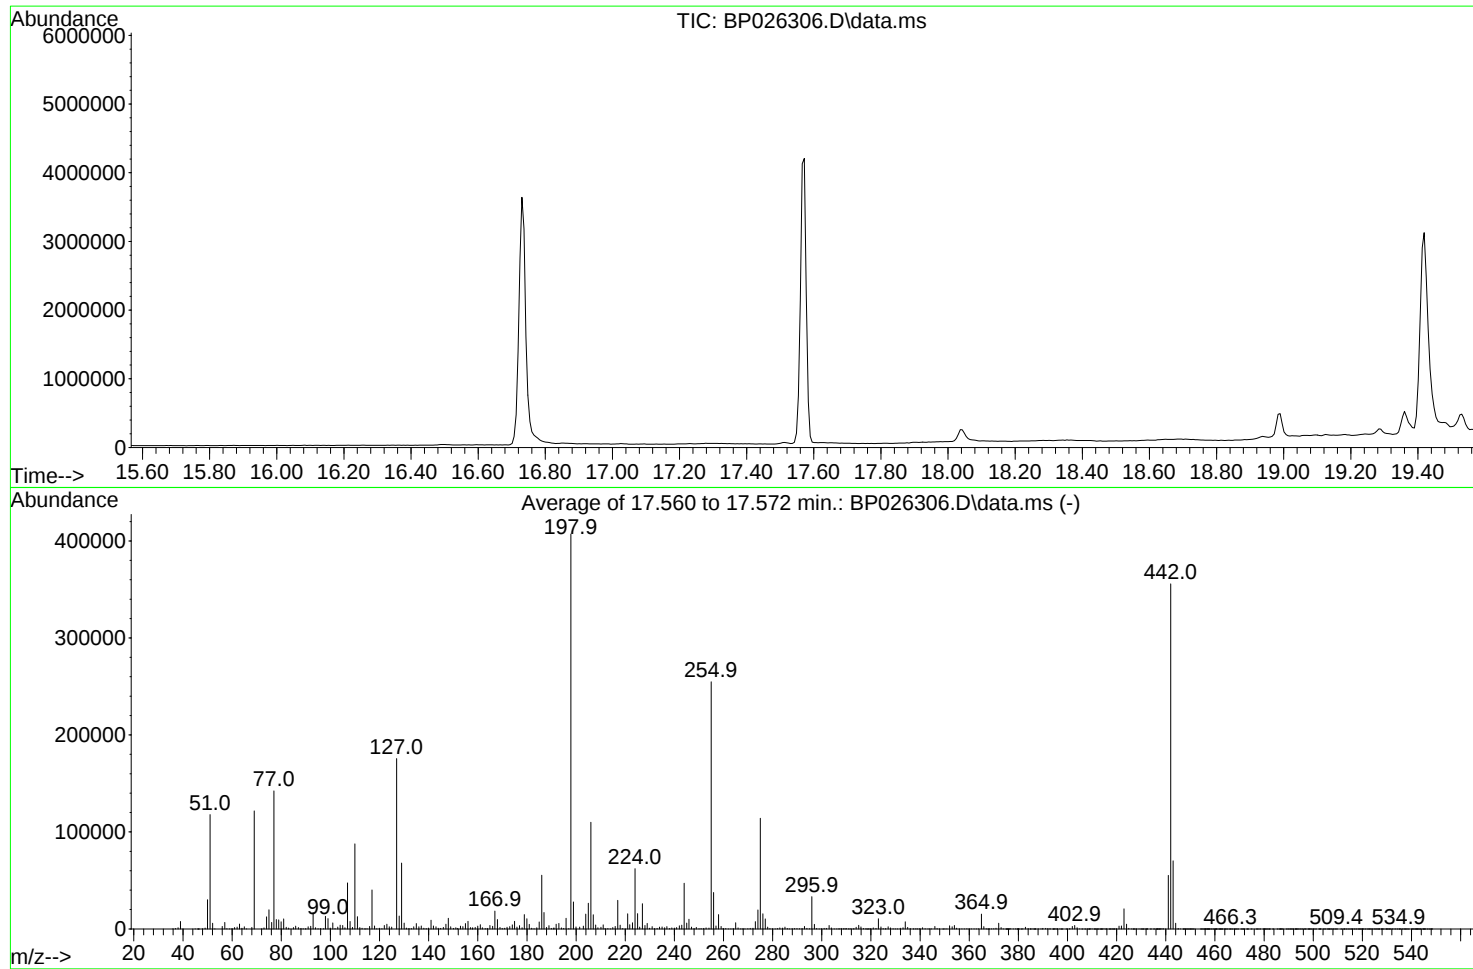




AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2477

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.3	1522	PASS
69	69	100	100	100.0	121683	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.1	453	PASS
198	198	100	100	100.0	407087	PASS
199	198	5	9	6.8	27840	PASS
365	198	1	100	3.7	15190	PASS
441	443	0.01	150	78.7	55216	PASS
442	442	100	100	100.0	355757	PASS
443	442	15	24	19.7	70133	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121225\
Data File : BP026306.D
Acq On : 12 Dec 2025 10:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 12 10:54:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 05 14:52:44 2025
Response via : Initial Calibration

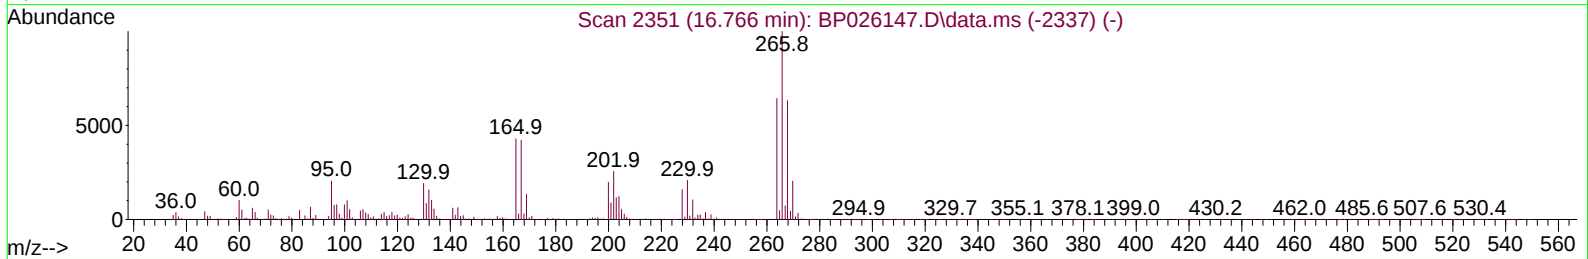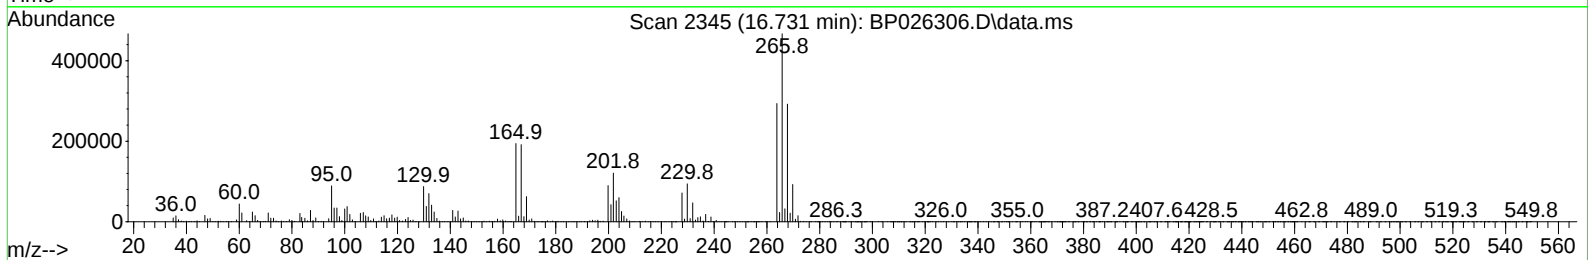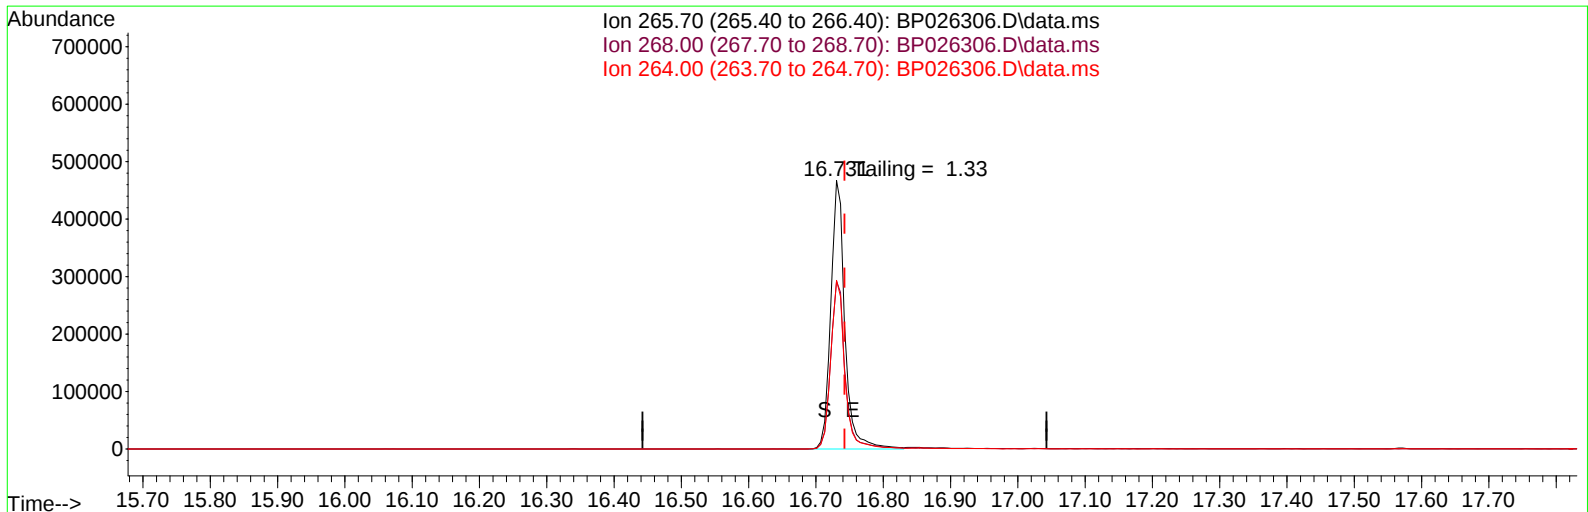

TIC: BP026306.D\data.ms

(70) Pentachlorophenol (C)

16.731min (-0.012) 122101.30 ng




response 677746

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.53
264.00	62.70	62.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121225\
Data File : BP026306.D
Acq On : 12 Dec 2025 10:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 12 10:54:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 05 14:52:44 2025
Response via : Initial Calibration

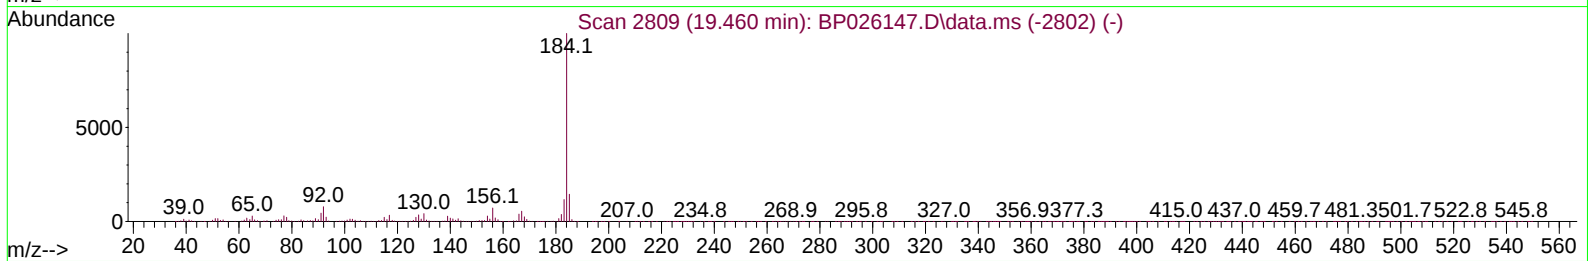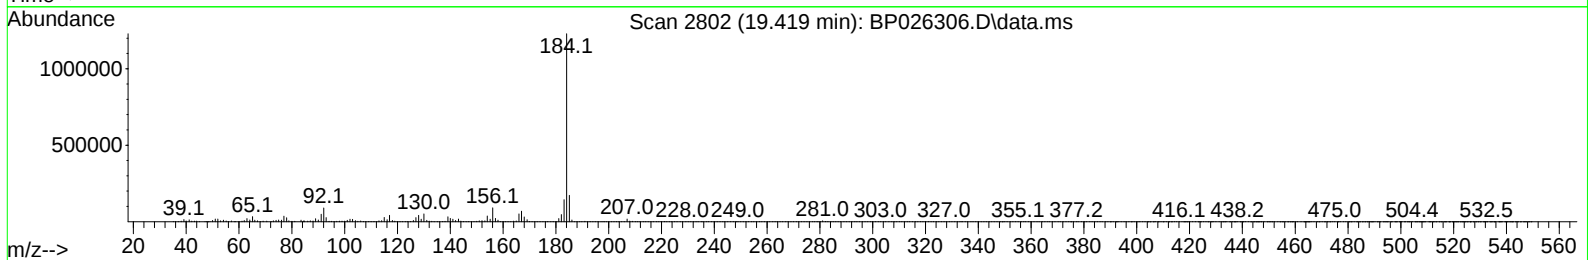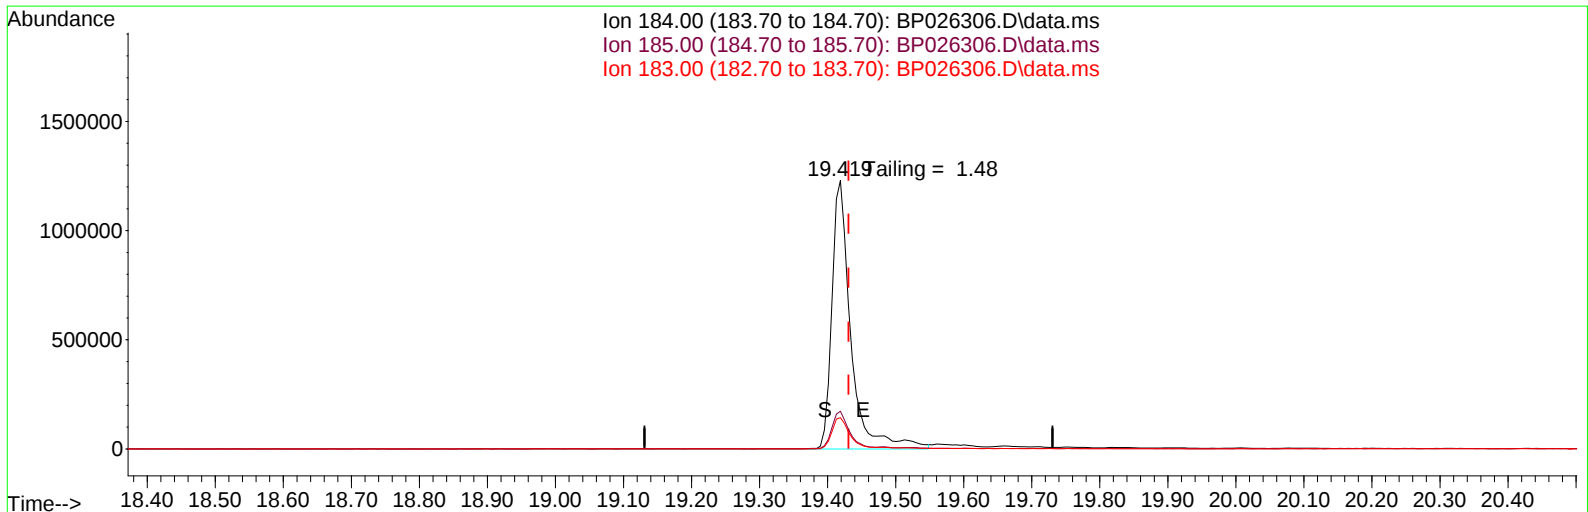

TIC: BP026306.D\data.ms

(77) Benzidine

19.419min (-0.012) 16192.53 ng

response 2291813

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.05
183.00	11.30	11.70
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/12/2025	BNA_P	<u>BP026306.D</u>
Compound Name	Response	Retention Time
DDT	1650269	20.724
DDD	40085	20.26
DDE	7199	19.73
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
47284	1697553	2.79

Instrument :
BNA_P
ClientSampleId :
DFTPP