
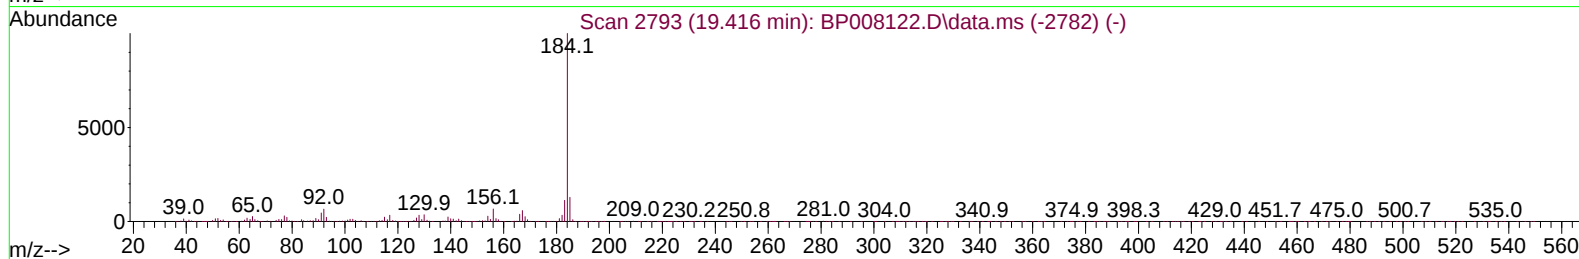
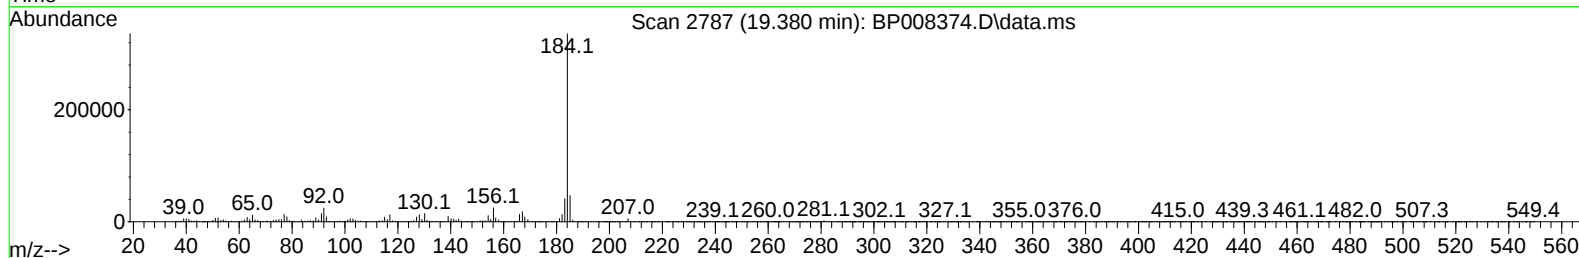


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121321\
Data File : BP008374.D
Acq On : 13 Dec 2021 10:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 13 15:31:18 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 11 03:53:01 2021
Response via : Initial Calibration

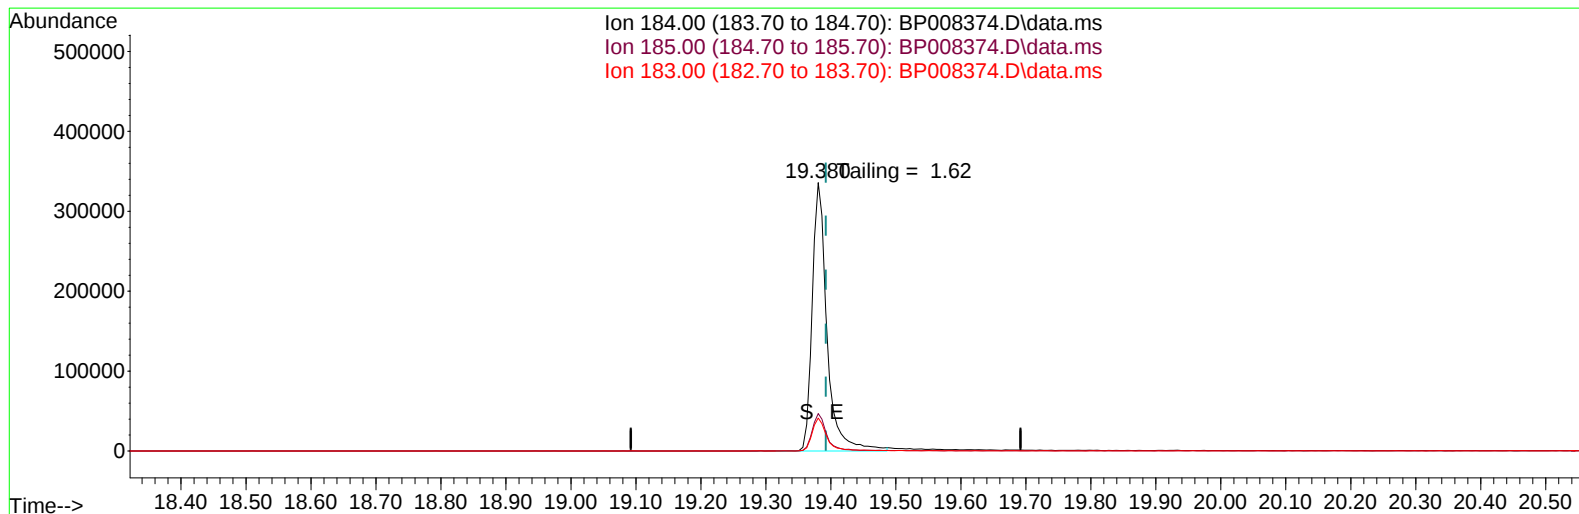

TIC: BP008374.D\data.ms

(77) Benzidine**19.380min (-0.012) 23100.11 ng****response 542797**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	13.99
183.00	11.40	12.29
0.00	0.00	0.00