

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121321\
 Data File : BP008387.D
 Acq On : 13 Dec 2021 21:15
 Operator : CG/JU
 Sample : M5051-03 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P-3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008387.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.946	161	163	172	rVB3	7340	10847	1.08%	0.203%
2	5.358	398	403	406	rBV	33800	52241	5.19%	0.979%
3	5.393	406	409	419	rVB2	18278	38377	3.81%	0.719%
4	5.763	468	472	477	rVB2	12192	18304	1.82%	0.343%
5	6.840	650	655	659	rBV2	10892	15549	1.54%	0.291%
6	6.893	659	664	671	rVB5	9581	17210	1.71%	0.322%
7	6.969	671	677	684	rBV3	29240	63197	6.27%	1.184%
8	7.393	742	749	754	rBV2	18970	37933	3.77%	0.711%
9	7.746	801	809	819	rBV	241734	393483	39.06%	7.371%
10	8.299	896	903	906	rBV8	5931	13539	1.34%	0.254%
11	8.922	1004	1009	1015	rBV3	16714	37828	3.75%	0.709%
12	8.975	1015	1018	1023	rVB	12264	17494	1.74%	0.328%
13	10.546	1276	1285	1291	rBV	282684	499730	49.60%	9.362%
14	13.022	1700	1706	1712	rBV	53402	86479	8.58%	1.620%
15	14.316	1918	1926	1930	rBV6	7607	20390	2.02%	0.382%
16	14.404	1934	1941	1948	rVV	422009	650621	64.58%	12.188%
17	15.916	2191	2198	2205	rBV2	39054	69277	6.88%	1.298%
18	16.134	2231	2235	2238	rBV6	7115	11336	1.13%	0.212%
19	17.169	2404	2411	2416	rBV	539853	791598	78.57%	14.830%
20	18.069	2560	2564	2573	rBV2	61761	97364	9.66%	1.824%
21	18.757	2677	2681	2686	rVB2	41481	50547	5.02%	0.947%
22	19.192	2751	2755	2761	rBV	56670	94397	9.37%	1.768%
23	19.304	2771	2774	2779	rBV3	44081	66507	6.60%	1.246%
24	19.545	2812	2815	2818	rBV	30253	35875	3.56%	0.672%
25	19.739	2844	2848	2853	rBV	115900	144173	14.31%	2.701%
26	21.274	3104	3109	3114	rBV	775323	1007477	100.00%	18.874%
27	23.651	3508	3513	3521	rVB2	517497	996220	98.88%	18.663%




Sum of corrected areas: 5337993

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121321\
Data File : BP008387.D
Acq On : 13 Dec 2021 21:15
Operator : CG/JU
Sample : M5051-03 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

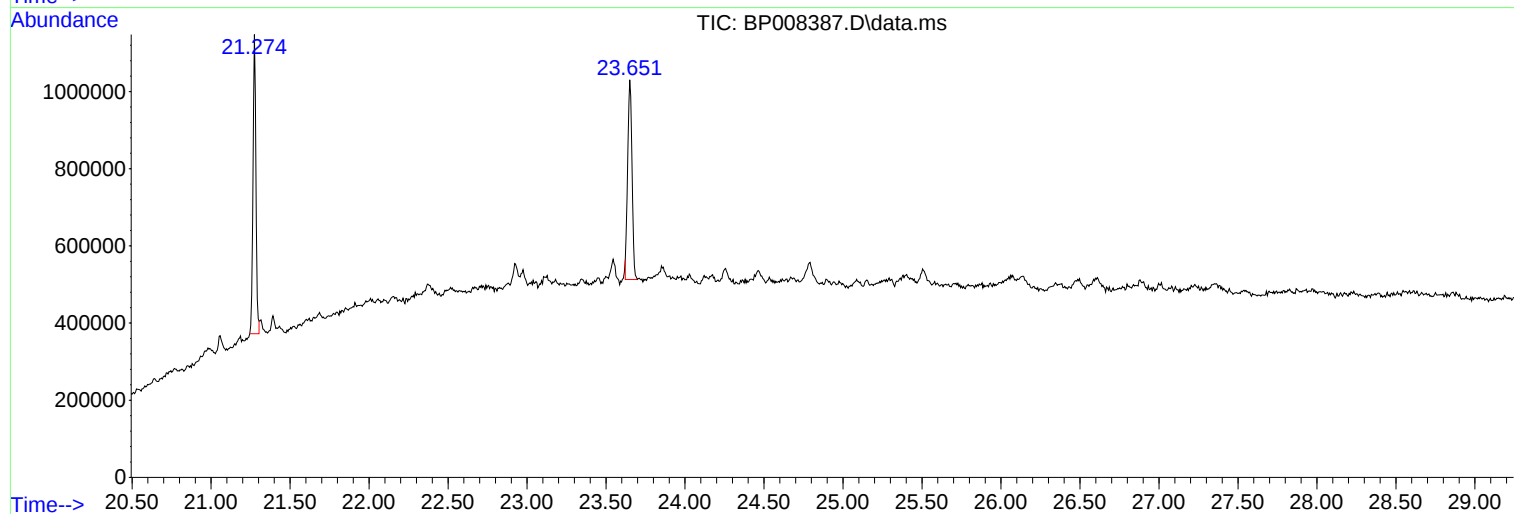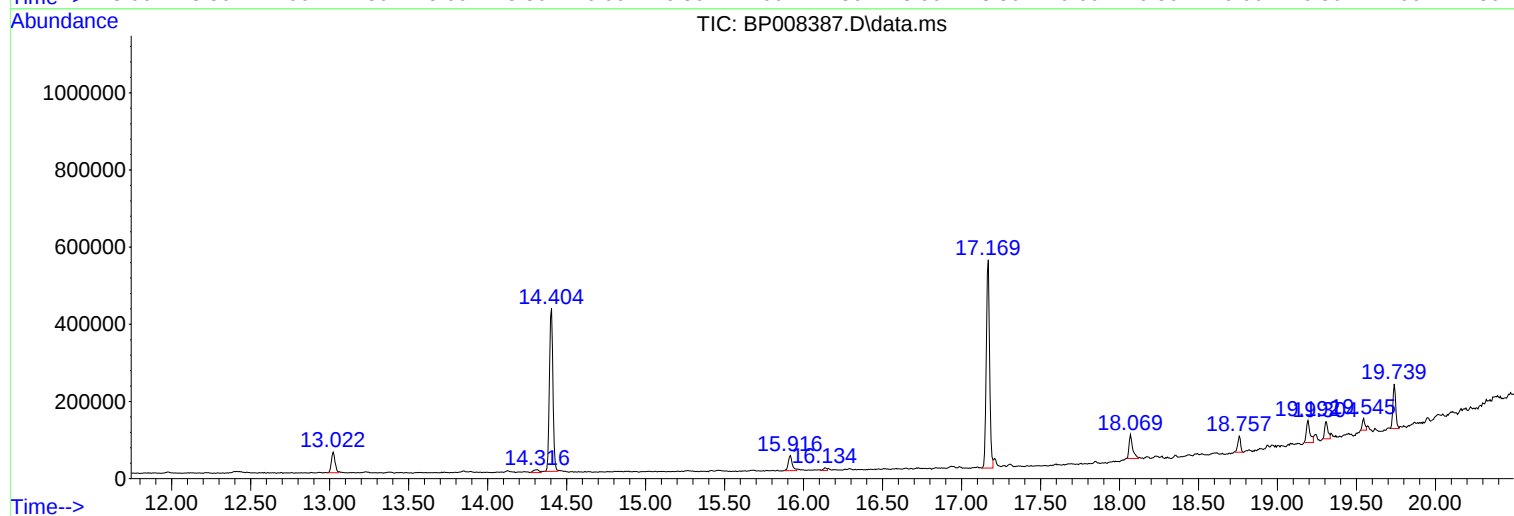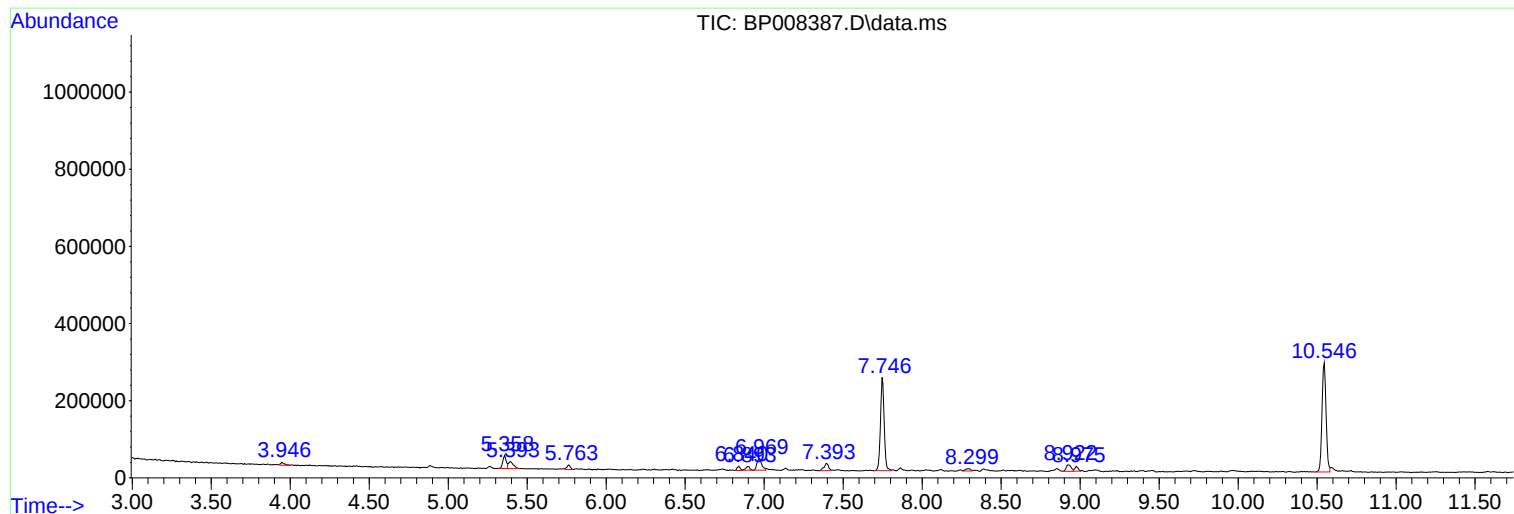

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121321\
Data File : BP008387.D
Acq On : 13 Dec 2021 21:15
Operator : CG/JU
Sample : M5051-03 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121321\
Data File : BP008387.D
Acq On : 13 Dec 2021 21:15
Operator : CG/JU
Sample : M5051-03 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------