


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121321\
 Data File : BP008374.D
 Acq On : 13 Dec 2021 10:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 11 03:53:01 2021

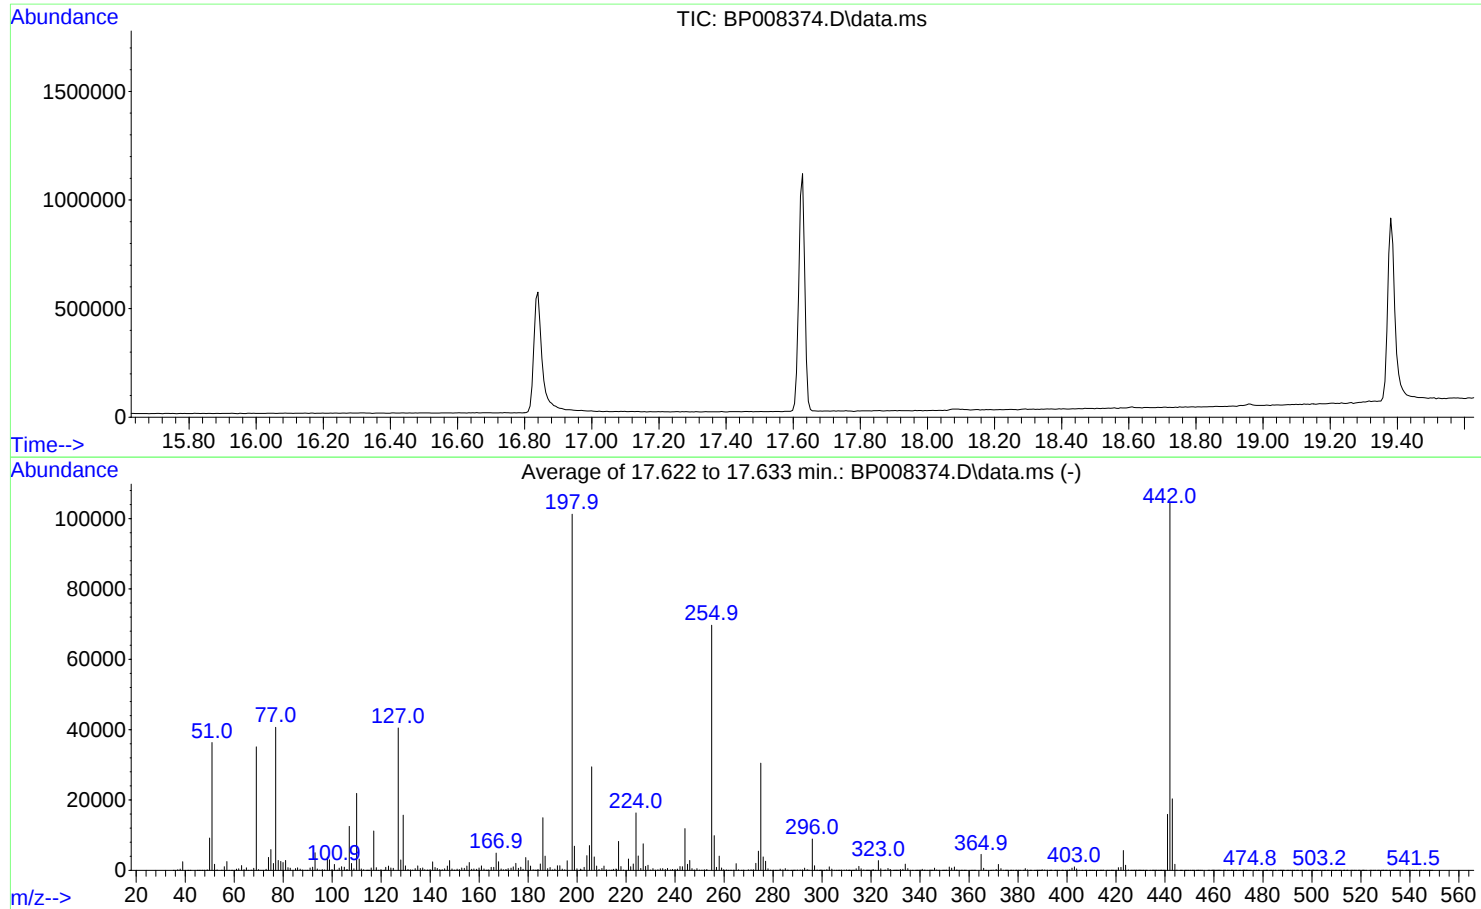




AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	36350	PASS
68	69	0.00	2	1.7	583	PASS
69	198	0.00	100	34.7	35118	PASS
70	69	0.00	2	0.7	250	PASS
127	198	10	80	40.0	40478	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	101245	PASS
199	198	5	9	6.8	6856	PASS
275	198	10	60	30.1	30485	PASS
365	198	1	100	4.5	4535	PASS
441	198	0.01	100	15.7	15932	PASS
442	442	100	100	100.0	104579	PASS
443	442	15	24	19.5	20357	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121321\
 Data File : BP008374.D
 Acq On : 13 Dec 2021 10:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 13 15:31:18 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 11 03:53:01 2021
 Response via : Initial Calibration

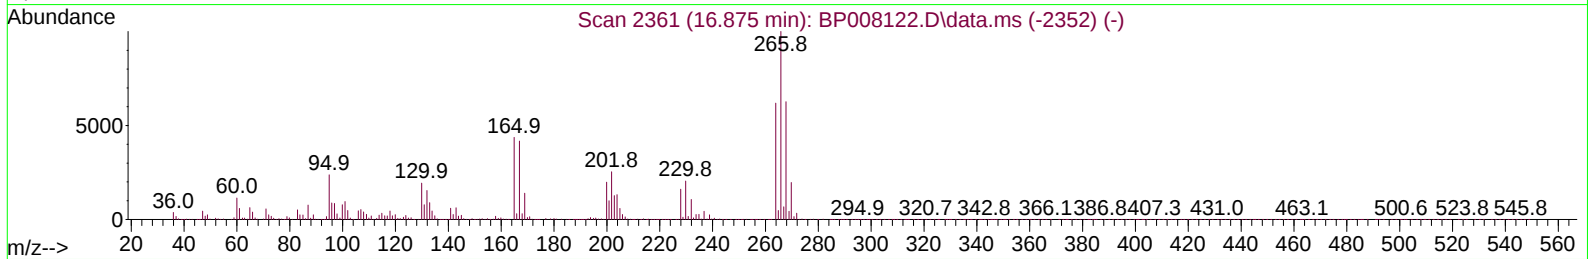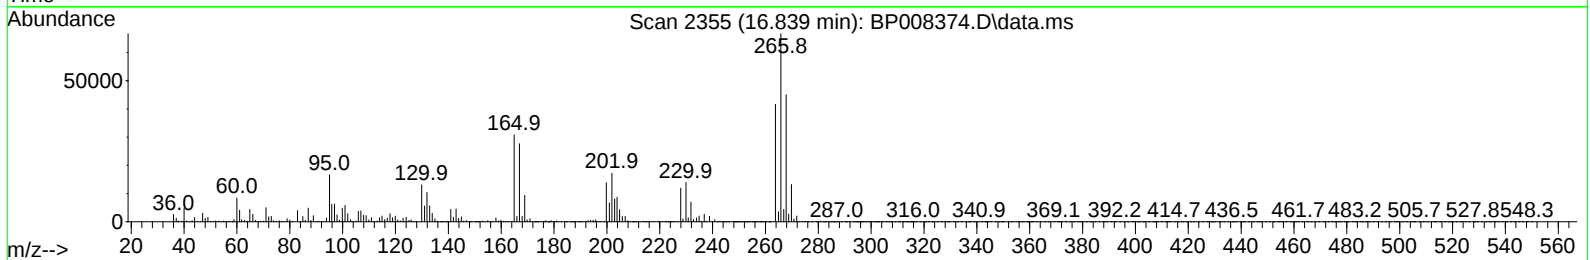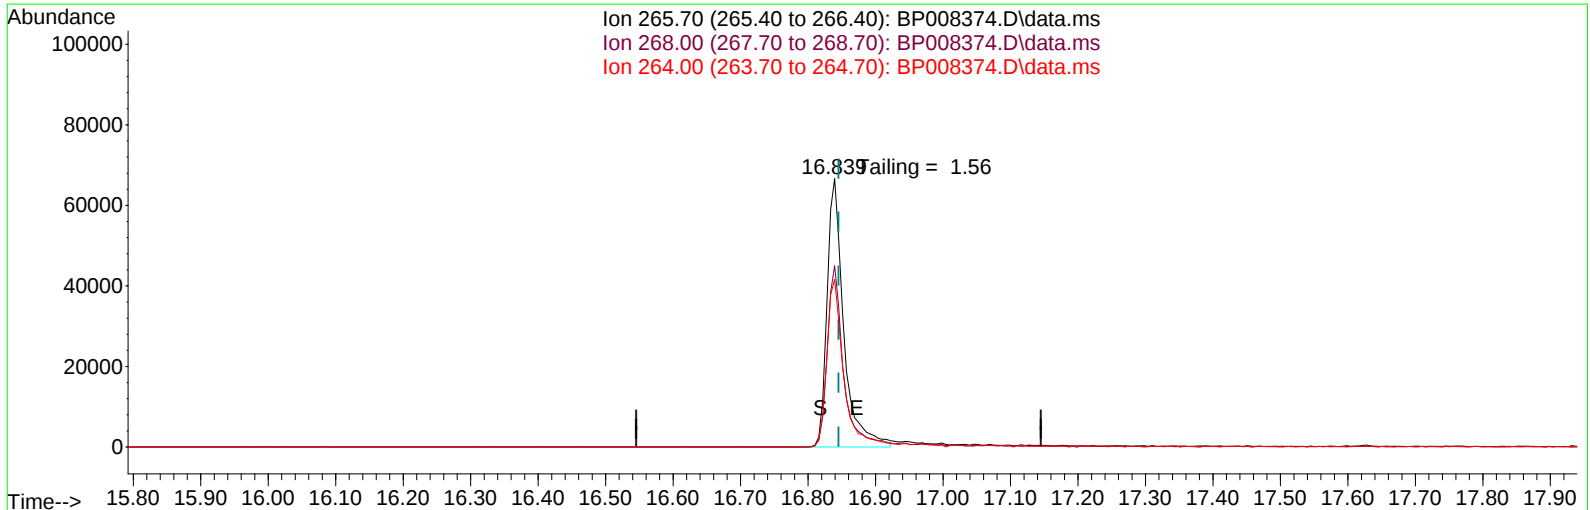

TIC: BP008374.D\data.ms

(70) Pentachlorophenol (C)

16.839min (-0.006) 748043.84 ng




response 116319

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	67.57
264.00	61.90	62.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121321\
 Data File : BP008374.D
 Acq On : 13 Dec 2021 10:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 13 15:31:18 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 11 03:53:01 2021
 Response via : Initial Calibration

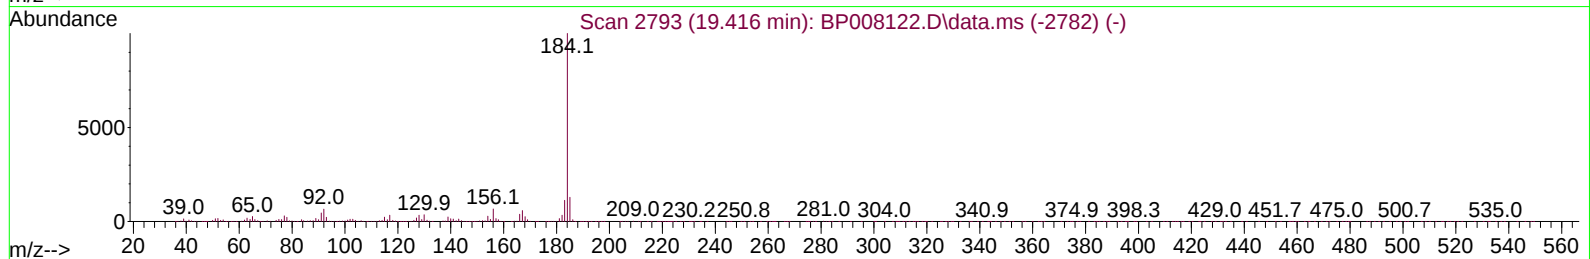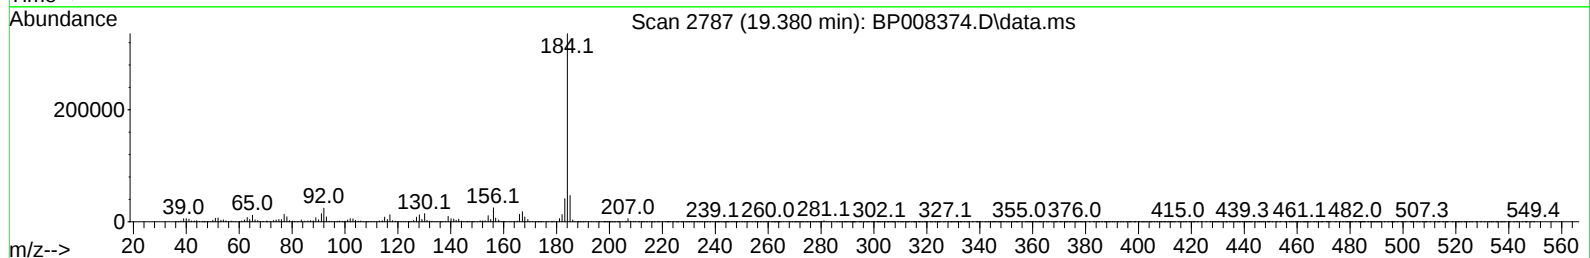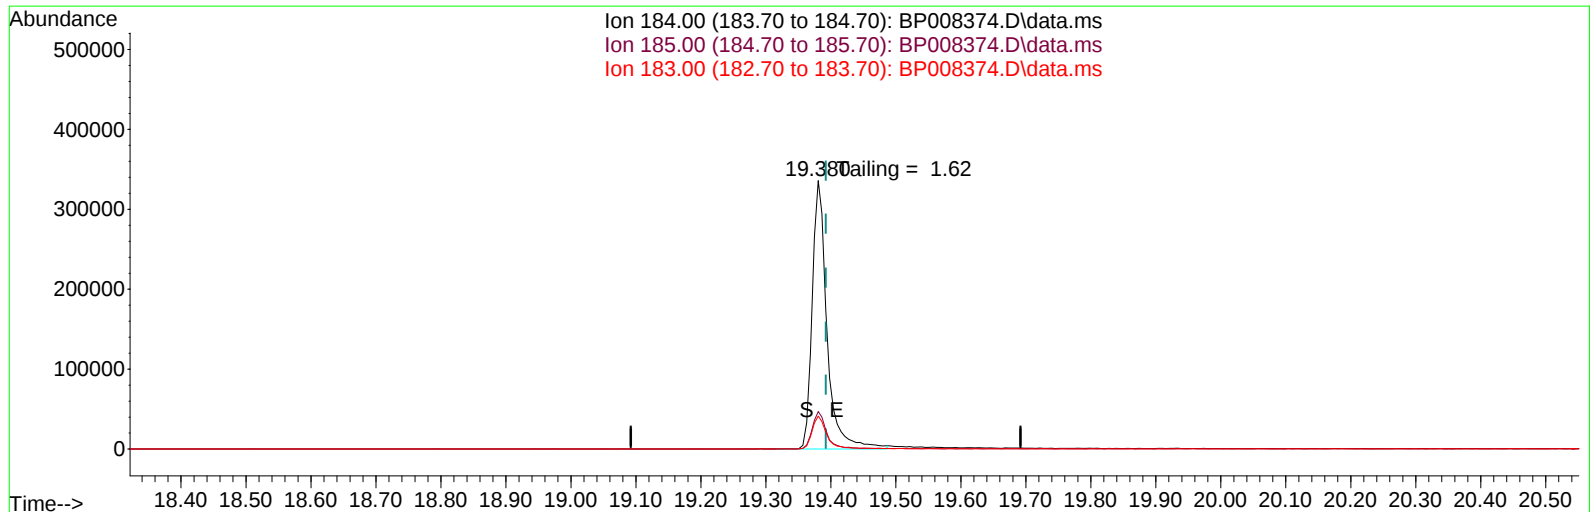

TIC: BP008374.D\data.ms

(77) Benzidine

19.380min (-0.012) 23100.11 ng

response 542797

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	13.99
183.00	11.40	12.29
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/13/2021	BNA_P	<u>BP008374.D</u>
Compound Name	Response	Retention Time
DDT	349231	20.58
DDD	4181	20.15
DDE	608	19.65
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4789	354020	1.35

Instrument :
BNA_P
ClientSampleId :
DFTPP