

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121323\
 Data File : BM043330.D
 Acq On : 14 Dec 2023 08:59
 Operator : MA/JU
 Sample : 05686-07
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCH81

Quant Time: Dec 14 22:56:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 13 22:33:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.998	152	439134	20.000	ng/ul	0.00
20) Naphthalene-d8	10.804	136	2086944	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.622	164	1243940	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.363	188	2397196	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.533	240	1617884	20.000	ng/ul	# 0.00
88) Perylene-d12	23.950	264	1516088	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	45989	4.110	ng/uL	0.00
4) Pyridine-d5	3.816	84	373633	11.254	ng/ul	0.00
7) Phenol-d5	7.157	99	270255	6.199	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	923173	34.206	ng/ul	0.00
11) 2-Chlorophenol-d4	7.522	132	820311	24.682	ng/ul	0.00
15) 4-Methylphenol-d8	8.704	113	526699	15.271	ng/ul	0.00
21) Nitrobenzene-d5	9.169	128	595542	33.480	ng/ul	0.00
24) 2-Nitrophenol-d4	9.887	143	596913	34.800	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.422	165	1010195	26.423	ng/ul	0.00
31) 4-Chloroaniline-d4	10.945	131	1375623	25.007	ng/ul	0.00
46) Dimethylphthalate-d6	14.045	166	3453682	31.673	ng/ul	0.00
49) Acenaphthylene-d8	14.322	160	4211212	33.381	ng/ul	0.00
54) 4-Nitrophenol-d4	14.816	143	91120	4.663	ng/ul	0.00
60) Fluorene-d10	15.616	176	3018631	31.757	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.733	200	252605	19.146	ng/ul	0.00
73) Anthracene-d10	17.463	188	4307647	33.215	ng/ul	0.00
81) Pyrene-d10	19.751	212	4311746	41.651	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.797	264	3039576	34.359	ng/ul	0.00
Target Compounds						
					Qvalue	
34) Caprolactam	11.733	113	76456	6.929	ng/ul	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121323\
Data File : BM043330.D
Acq On : 14 Dec 2023 08:59
Operator : MA/JU
Sample : 05686-07
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCH81

Quant Time: Dec 14 22:56:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 13 22:33:14 2023
Response via : Initial Calibration

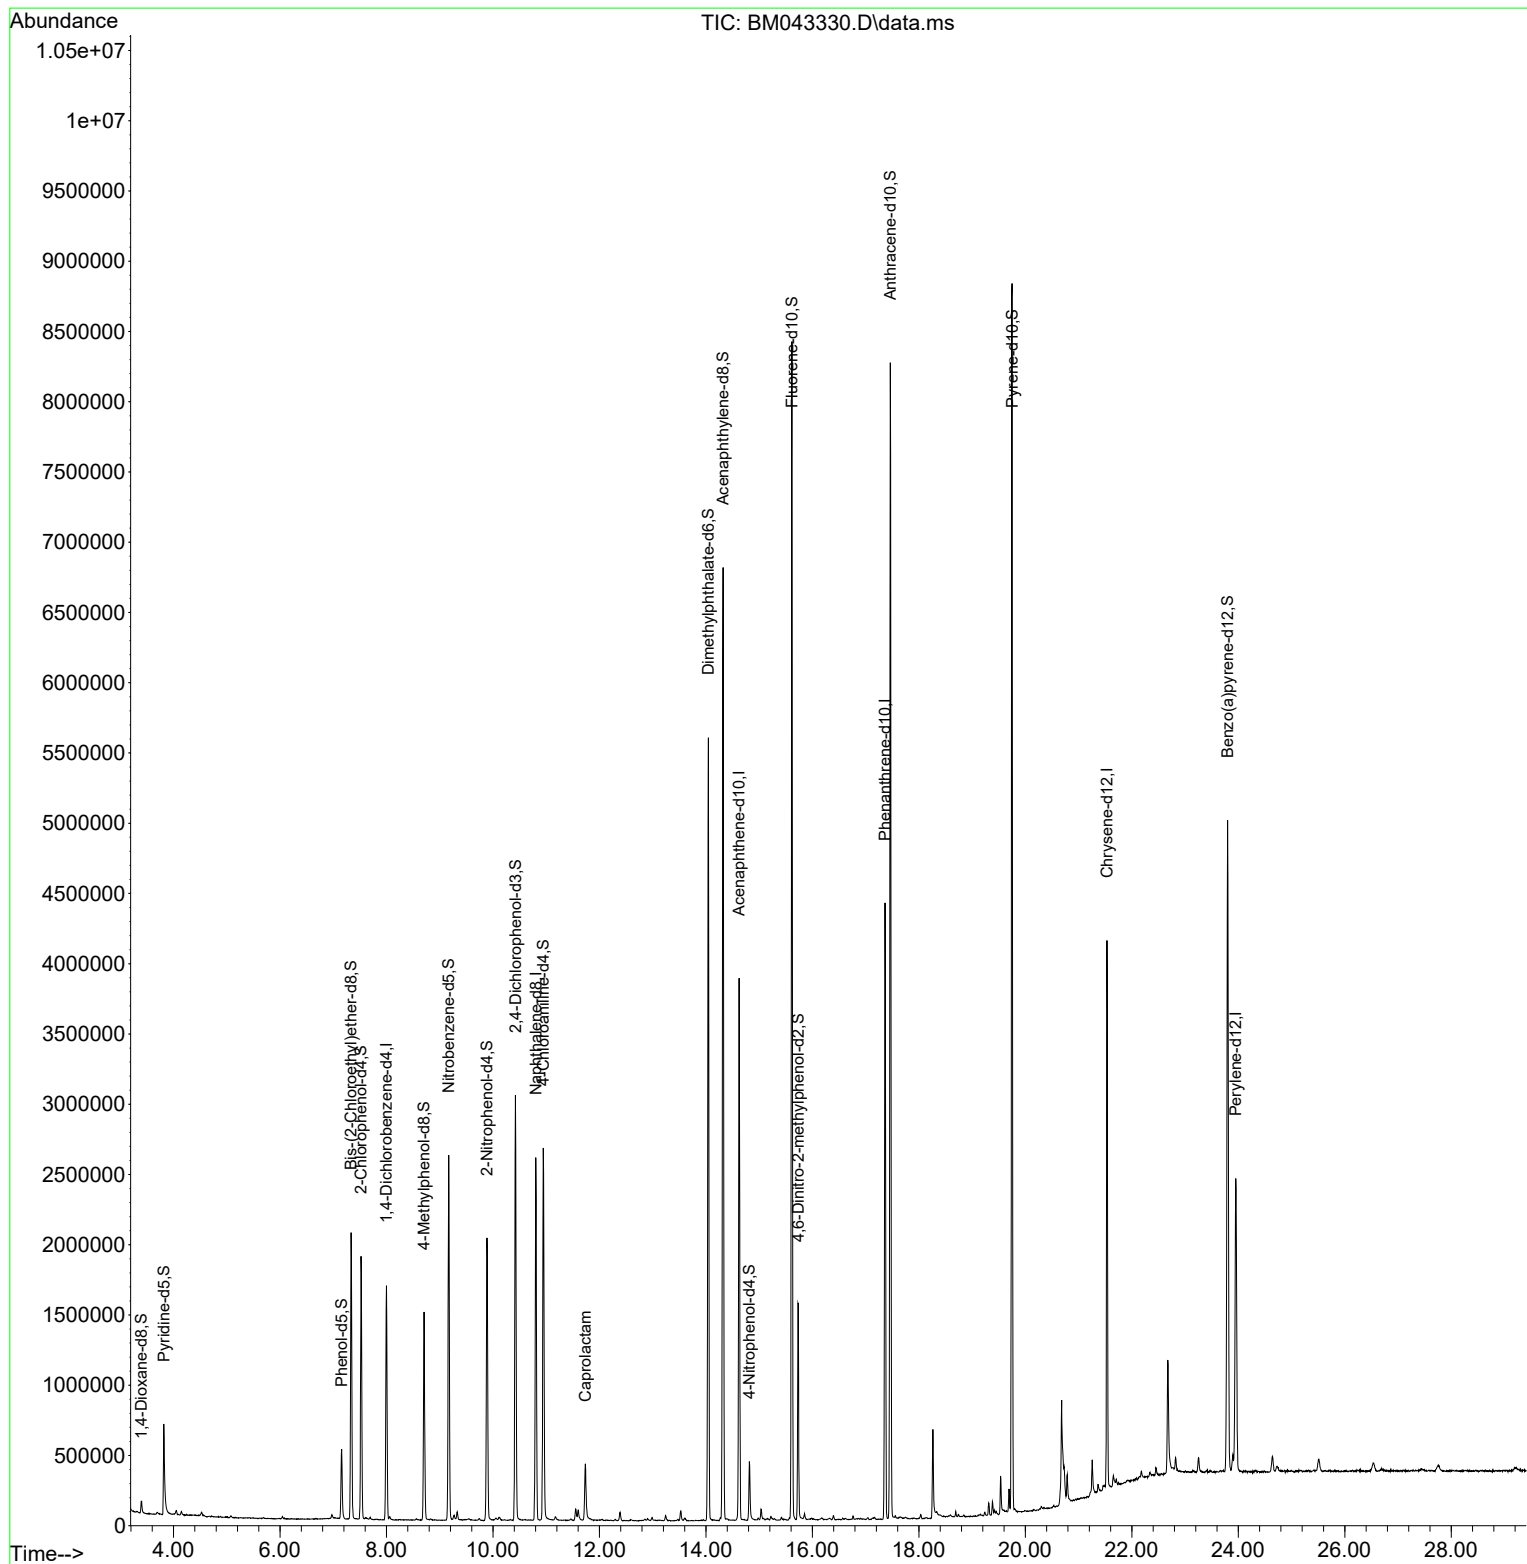

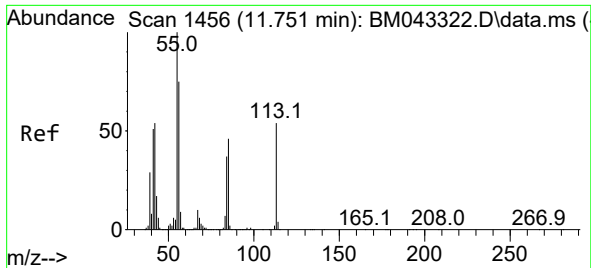

#34
 Caprolactam
 Concen: 6.929 ng/ul
 RT: 11.733 min Scan# 14
 Delta R.T. -0.018 min
 Lab File: BM043330.D
 Acq: 14 Dec 2023 08:59

Instrument :
 BNA_P
 ClientSampleId :
 YCH81

Tgt Ion:113 Resp: 76456
 Ion Ratio Lower Upper
 113 100
 55 193.8 139.5 209.3
 56 142.2 103.5 155.3

