

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121323\
 Data File : BM043331.D
 Acq On : 14 Dec 2023 09:38
 Operator : MA/JU
 Sample : 05686-08
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCH82

Quant Time: Dec 14 22:56:15 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 13 22:33:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.999	152	395740	20.000	ng/ul	0.00
20) Naphthalene-d8	10.804	136	1905325	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.622	164	1139826	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.363	188	2181227	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.533	240	1454002	20.000	ng/ul	# 0.00
88) Perylene-d12	23.950	264	1373560	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	43058	4.270	ng/uL	0.00
4) Pyridine-d5	3.817	84	314633	10.516	ng/ul	0.00
7) Phenol-d5	7.152	99	234510	5.969	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	890818	36.627	ng/ul	0.00
11) 2-Chlorophenol-d4	7.522	132	755061	25.210	ng/ul	0.00
15) 4-Methylphenol-d8	8.704	113	468669	15.078	ng/ul	0.00
21) Nitrobenzene-d5	9.169	128	571084	35.166	ng/ul	0.00
24) 2-Nitrophenol-d4	9.887	143	553092	35.319	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.422	165	916657	26.262	ng/ul	0.00
31) 4-Chloroaniline-d4	10.945	131	1347149	26.823	ng/ul	0.00
46) Dimethylphthalate-d6	14.045	166	3268530	32.713	ng/ul	0.00
49) Acenaphthylene-d8	14.322	160	3991084	34.526	ng/ul	0.00
54) 4-Nitrophenol-d4	14.816	143	77351	4.320	ng/ul	0.00
60) Fluorene-d10	15.616	176	2870798	32.961	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.733	200	232725	19.386	ng/ul	0.00
73) Anthracene-d10	17.463	188	4185264	35.467	ng/ul	0.00
81) Pyrene-d10	19.745	212	4162572	44.742	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.798	264	2909454	36.300	ng/ul	0.00
Target Compounds						
					Qvalue	
34) Caprolactam	11.734	113	57114	5.670	ng/ul	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121323\
Data File : BM043331.D
Acq On : 14 Dec 2023 09:38
Operator : MA/JU
Sample : 05686-08
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCH82

Quant Time: Dec 14 22:56:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 13 22:33:14 2023
Response via : Initial Calibration

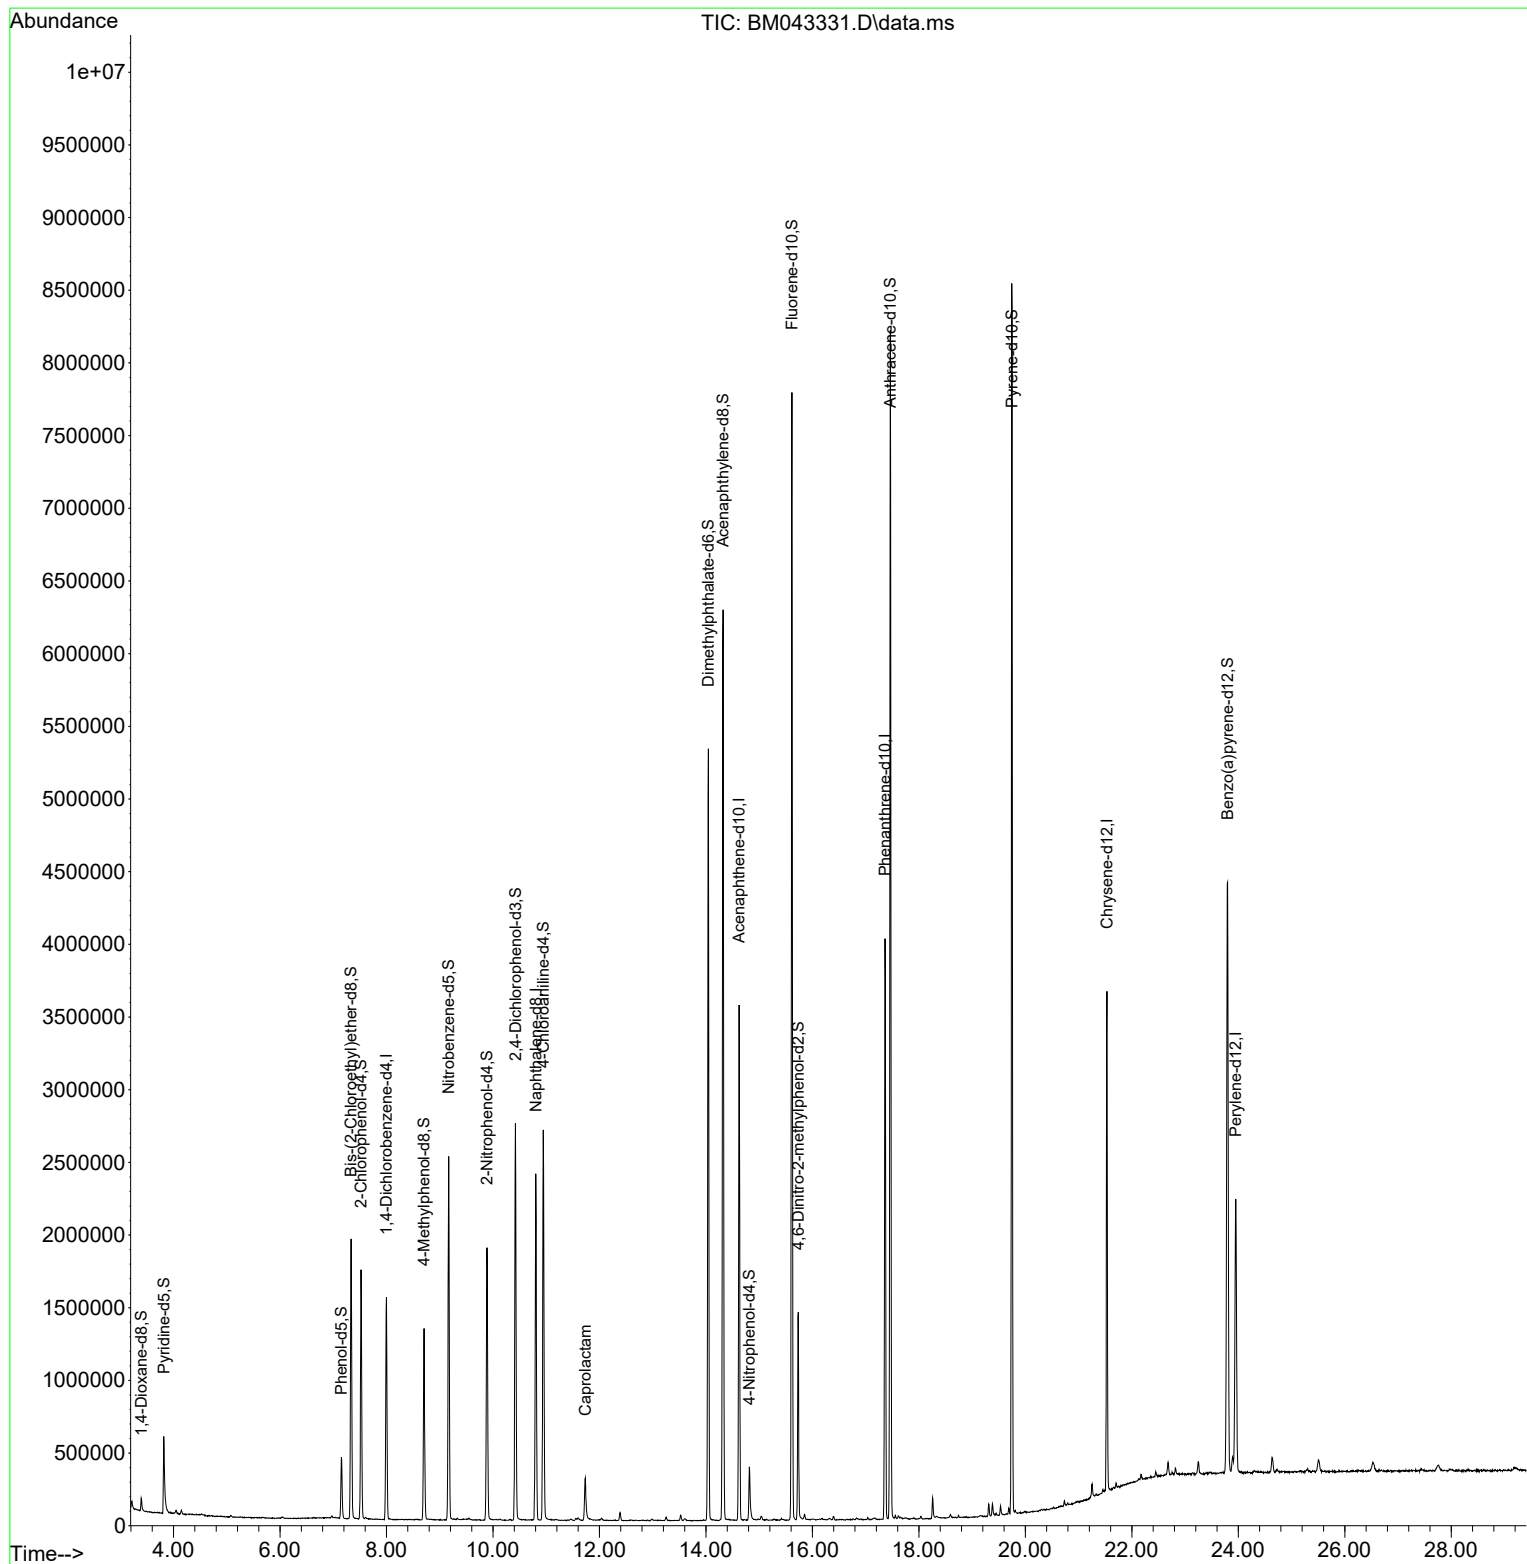

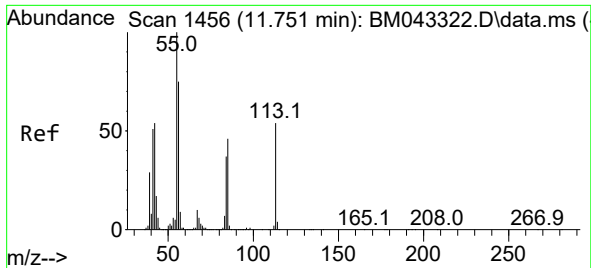

#34
Caprolactam
Concen: 5.670 ng/ul
RT: 11.734 min Scan# 14
Delta R.T. -0.017 min
Lab File: BM043331.D
Acq: 14 Dec 2023 09:38

Instrument :
BNA_P
ClientSampleId :
YCH82

Tgt Ion:113 Resp: 57114
Ion Ratio Lower Upper
113 100
55 185.3 139.5 209.3
56 136.5 103.5 155.3

