

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121323\
 Data File : BM043332.D
 Acq On : 14 Dec 2023 10:14
 Operator : MA/JU
 Sample : 05686-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCH80

Quant Time: Dec 14 22:56:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 13 22:33:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.998	152	453206	20.000	ng/ul	0.00
20) Naphthalene-d8	10.804	136	2165390	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.621	164	1296511	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.362	188	2483973	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.533	240	1680353	20.000	ng/ul	# 0.00
88) Perylene-d12	23.950	264	1601036	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	46779	4.051	ng/uL	0.00
4) Pyridine-d5	3.816	84	296110	8.642	ng/ul	0.00
7) Phenol-d5	7.157	99	233492	5.189	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	842588	30.251	ng/ul	0.00
11) 2-Chlorophenol-d4	7.522	132	733240	21.377	ng/ul	0.00
15) 4-Methylphenol-d8	8.704	113	463145	13.011	ng/ul	0.00
21) Nitrobenzene-d5	9.169	128	537337	29.114	ng/ul	0.00
24) 2-Nitrophenol-d4	9.886	143	522946	29.383	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.422	165	887521	22.373	ng/ul	0.00
31) 4-Chloroaniline-d4	10.945	131	1307983	22.916	ng/ul	0.00
46) Dimethylphthalate-d6	14.045	166	3227269	28.396	ng/ul	0.00
49) Acenaphthylene-d8	14.321	160	3759440	28.592	ng/ul	0.00
54) 4-Nitrophenol-d4	14.816	143	81528	4.003	ng/ul	0.00
60) Fluorene-d10	15.616	176	2803842	28.301	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.733	200	240390	17.584	ng/ul	0.00
73) Anthracene-d10	17.462	188	4277885	31.833	ng/ul	0.00
81) Pyrene-d10	19.745	212	4338988	40.356	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.797	264	3041615	32.557	ng/ul	0.00
Target Compounds						
					Qvalue	
34) Caprolactam	11.739	113	205304	17.933	ng/ul	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121323\
Data File : BM043332.D
Acq On : 14 Dec 2023 10:14
Operator : MA/JU
Sample : 05686-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCH80

Quant Time: Dec 14 22:56:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 13 22:33:14 2023
Response via : Initial Calibration

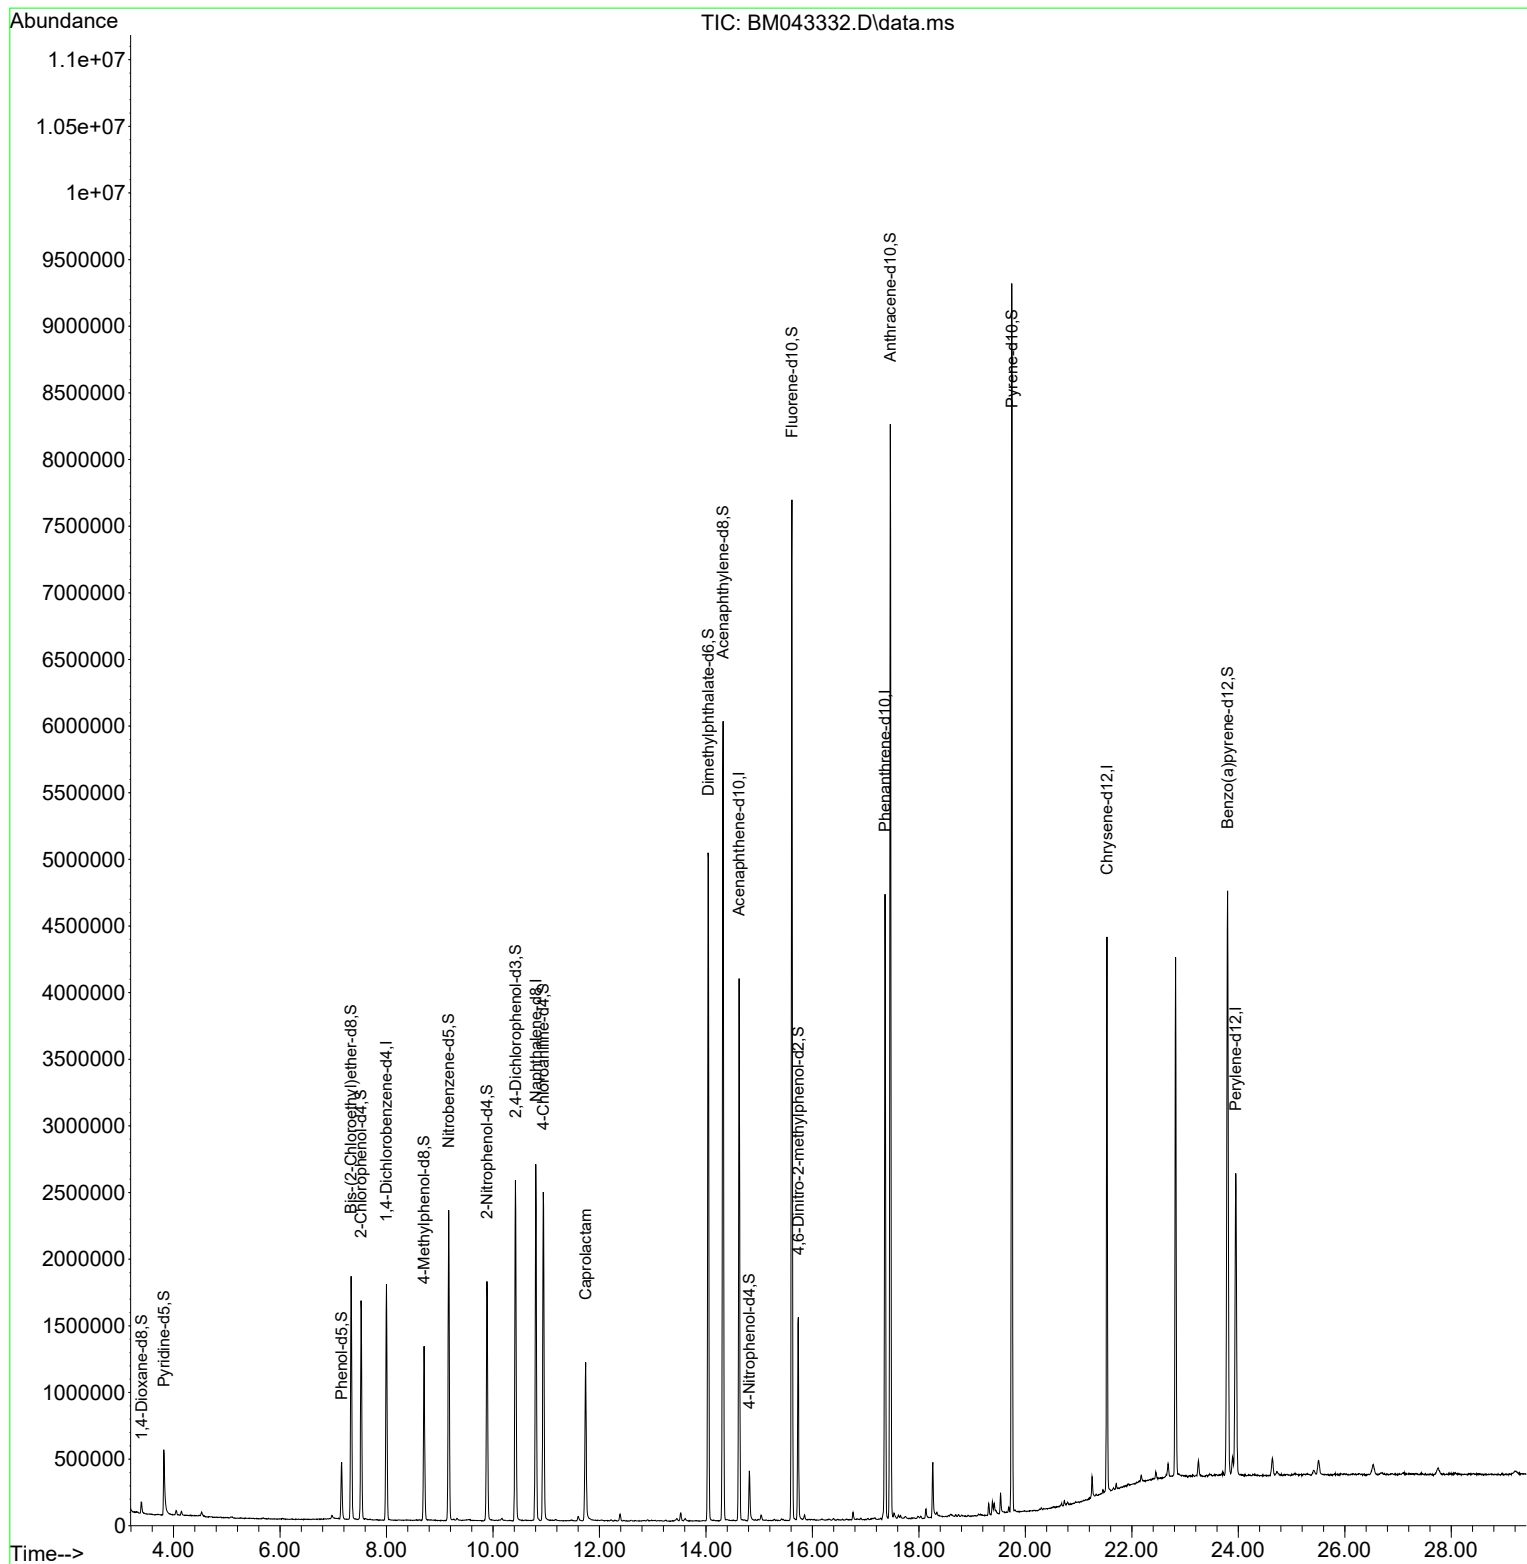

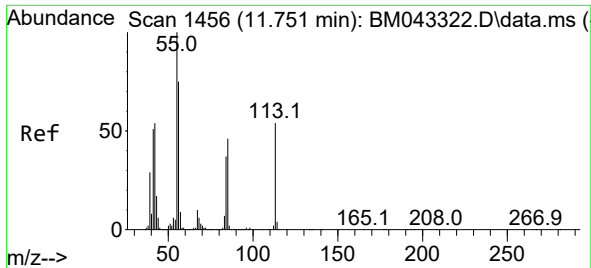

#34
Caprolactam
Concen: 17.933 ng/ul
RT: 11.739 min Scan# 14
Delta R.T. -0.012 min
Lab File: BM043332.D
Acq: 14 Dec 2023 10:14

Instrument :
BNA_P
ClientSampleId :
YCH80

Tgt Ion:113 Resp: 205304
Ion Ratio Lower Upper
113 100
55 186.6 139.5 209.3
56 142.5 103.5 155.3

