

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018811.D
 Acq On : 13 Dec 2023 18:40
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020724

Quant Time: Dec 13 23:34:31 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 13 23:34:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.834	152	258863	20.000	ng/u1	0.00
20) Naphthalene-d8	10.628	136	957452	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.463	164	564758	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.216	188	1180075	20.000	ng/u1	0.00
79) Chrysene-d12	21.304	240	1227522	20.000	ng/u1	0.00
88) Perylene-d12	23.663	264	1474368	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	59744	7.865	ng/uL	0.00
4) Pyridine-d5	3.675	84	387423	19.040	ng/u1	0.00
7) Phenol-d5	6.999	99	445678	17.156	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.169	67	266918	17.336	ng/u1	0.00
11) 2-Chlorophenol-d4	7.363	132	356524	17.588	ng/u1	0.00
15) 4-Methylphenol-d8	8.546	113	339583	16.153	ng/u1	0.00
21) Nitrobenzene-d5	8.993	128	160179	18.797	ng/u1	0.00
24) 2-Nitrophenol-d4	9.716	143	166336	18.827	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.251	165	343121	18.993	ng/u1	0.00
31) 4-Chloroaniline-d4	10.769	131	420594	17.815	ng/u1	0.00
46) Dimethylphthalate-d6	13.881	166	916331	18.179	ng/u1	0.00
49) Acenaphthylene-d8	14.157	160	1052353	18.960	ng/u1	0.00
54) 4-Nitrophenol-d4	14.669	143	151290	18.285	ng/u1	0.00
60) Fluorene-d10	15.457	176	791586	18.709	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.581	200	132203	18.684	ng/u1	0.00
73) Anthracene-d10	17.310	188	1188731	19.161	ng/u1	0.00
81) Pyrene-d10	19.551	212	1425810	14.922	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.515	264	1600252	18.615	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.293	88	63700	7.647	ng/uL	97
5) Pyridine	3.693	79	391561	19.056	ng/u1	95
6) Benzaldehyde	6.975	77	197631	14.735	ng/u1	92
8) Phenol	7.028	94	443419	17.406	ng/u1	99
10) Bis(2-Chloroethyl)ether	7.263	93	370458	17.706	ng/u1	98
12) 2-Chlorophenol	7.393	128	358696	17.484	ng/u1	99
13) 2-Methylphenol	8.281	108	323567	16.590	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.357	45	430454	16.215	ng/u1	97
16) Acetophenone	8.657	105	517110	16.504	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.646	70	248240	14.402	ng/u1	98
18) 4-Methylphenol	8.610	108	345025	16.201	ng/u1	98
19) Hexachloroethane	8.910	117	152625	18.147	ng/u1	86
22) Nitrobenzene	9.034	77	383319	18.501	ng/u1	98
23) Isophorone	9.563	82	690264	16.340	ng/u1	98
25) 2-Nitrophenol	9.746	139	181369	19.173	ng/u1	99
26) 2,4-Dimethylphenol	9.810	107	339305	18.340	ng/u1	99
27) Bis(2-Chloroethoxy)met...	10.046	93	462769	17.352	ng/u1	100
29) 2,4-Dichlorophenol	10.275	162	332449	19.105	ng/u1	98
30) Naphthalene	10.675	128	1088456	18.740	ng/u1	99
32) 4-Chloroaniline	10.793	127	410439	18.240	ng/u1	99
33) Hexachlorobutadiene	10.963	225	251501	21.581	ng/u1	98
34) Caprolactam	11.569	113	78687	14.747	ng/u1	89
35) 4-Chloro-3-methylphenol	11.916	107	318088	16.318	ng/u1	99
36) 2-Methylnaphthalene	12.287	142	723741	17.589	ng/u1	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018811.D
 Acq On : 13 Dec 2023 18:40
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020724


Quant Time: Dec 13 23:34:31 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 13 23:34:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.510	142	727107	17.498	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.657	216	443369	21.638	ng/ul	97
40) Hexachlorocyclopentadiene	12.634	237	243733	20.068	ng/ul	99
41) 2,4,6-Trichlorophenol	12.898	196	257371	19.526	ng/ul	100
42) 2,4,5-Trichlorophenol	12.969	196	275333	19.267	ng/ul	99
43) 1,1'-Biphenyl	13.298	154	958226	19.618	ng/ul	98
44) 2-Chloronaphthalene	13.340	162	764953	19.829	ng/ul	98
45) 2-Nitroaniline	13.551	65	176319	16.860	ng/ul	94
47) Dimethylphthalate	13.928	163	906360	18.267	ng/ul	100
48) 2,6-Dinitrotoluene	14.051	165	166355	17.746	ng/ul	93
50) Acenaphthylene	14.187	152	1184144	18.976	ng/ul	100
51) 3-Nitroaniline	14.375	138	162436	17.359	ng/ul	97
52) Acenaphthene	14.528	153	785252	19.032	ng/ul	99
53) 2,4-Dinitrophenol	14.581	184	84693	17.047	ng/ul	95
55) 4-Nitrophenol	14.687	109	114024	18.241	ng/ul	95
56) Dibenzofuran	14.863	168	1096385	19.119	ng/ul	98
57) 2,4-Dinitrotoluene	14.834	165	235731	17.877	ng/ul	94
58) 2,3,4,6-Tetrachlorophenol	15.092	232	229538	19.149	ng/ul	93
59) Diethylphthalate	15.292	149	854910	17.608	ng/ul	99
61) Fluorene	15.516	166	874127	19.264	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.510	204	471175	19.799	ng/ul	94
63) 4-Nitroaniline	15.539	138	156945	17.605	ng/ul	97
66) 4,6-Dinitro-2-methylph...	15.592	198	143285	18.941	ng/ul	95
67) N-Nitrosodiphenylamine	15.728	169	726163	18.570	ng/ul	99
68) 4-Bromophenyl-phenylether	16.404	248	288260	19.349	ng/ul	95
69) Hexachlorobenzene	16.516	284	332475	19.988	ng/ul	97
70) Atrazine	16.681	200	167200	14.382	ng/ul	98
71) Pentachlorophenol	16.863	266	189039	19.109	ng/ul	99
72) Phenanthrene	17.257	178	1359620	19.077	ng/ul	99
74) Anthracene	17.345	178	1381276	19.335	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.263	216	432024	21.173	ng/ul	99
76) Pentachlorobenzene	14.781	250	411597	20.535	ng/ul	99
77) Carbazole	17.622	167	1194330	20.976	ng/ul	99
78) Di-n-butylphthalate	18.180	149	1412394	18.629	ng/ul	99
80) Fluoranthene	19.227	202	1642645	14.543	ng/ul	96
82) Pyrene	19.580	202	1705488	14.968	ng/ul	96
83) Butylbenzylphthalate	20.457	149	634095	15.201	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.227	252	571481	19.158	ng/ul	98
85) Benzo(a)anthracene	21.286	228	1850116	18.569	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.216	149	977691	17.053	ng/ul	100
87) Chrysene	21.339	228	1712935	18.669	ng/ul	100
89) Di-n-octyl phthalate	22.127	149	1690815	15.707	ng/ul	100
90) Benzo(b)fluoranthene	22.945	252	1960415	18.034	ng/ul	99
91) Benzo(k)fluoranthene	22.992	252	1911056	18.169	ng/ul	99
93) Benzo(a)pyrene	23.563	252	1858177	18.707	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	26.121	276	2370276	19.973	ng/ul	97
95) Dibenzo(a,h)anthracene	26.139	278	1986339	20.120	ng/ul	97
96) Benzo(g,h,i)perylene	26.874	276	1897520	19.868	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Dec 13 23:34:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 13 23:34:47 2023
Response via : Initial Calibration









#2
1,4-Dioxane
Concen: 7.647 ng/uL
RT: 3.293 min Scan# 35
Delta R.T. 0.000 min
Lab File: BP018811.D
Acq: 13 Dec 2023 18:40




Instrument :
BNA_P
ClientSampleId :
SSTD020724


Tgt Ion: 88 Resp: 63700
Ion Ratio Lower Upper
88 100
43 24.1 21.8 32.6
58 68.8 56.5 84.7

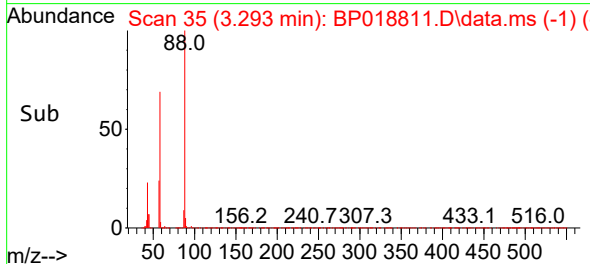

#5
Pyridine
Concen: 19.056 ng/uL
RT: 3.693 min Scan# 103
Delta R.T. 0.000 min
Lab File: BP018811.D
Acq: 13 Dec 2023 18:40

Tgt Ion: 79 Resp: 391561
Ion Ratio Lower Upper
79 100
52 65.8 57.4 86.0
51 32.7 26.2 39.4



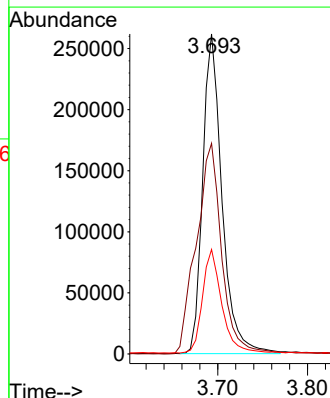
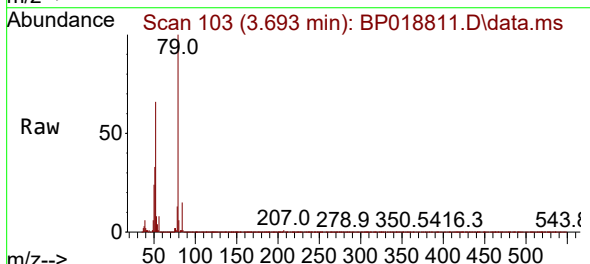




#6
Benzaldehyde
Concen: 14.735 ng/ul
RT: 6.975 min Scan# 60
Delta R.T. 0.000 min
Lab File: BP018811.D
Acq: 13 Dec 2023 18:40




Instrument :
BNA_P
ClientSampleId :
SSTD020724


Tgt Ion: 77 Resp: 197631
Ion Ratio Lower Upper
77 100
105 105.2 77.9 116.9
106 101.8 74.6 111.8

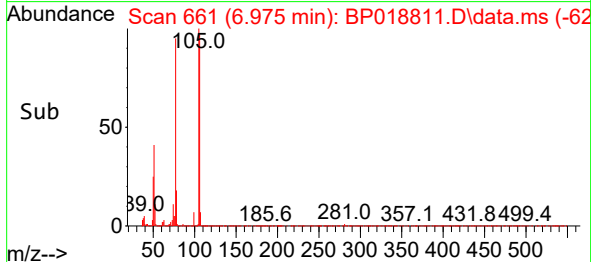

#8
Phenol
Concen: 17.406 ng/ul
RT: 7.028 min Scan# 670
Delta R.T. 0.000 min
Lab File: BP018811.D
Acq: 13 Dec 2023 18:40

Tgt Ion: 94 Resp: 443419
Ion Ratio Lower Upper
94 100
65 25.7 21.0 31.6
66 35.3 28.6 43.0

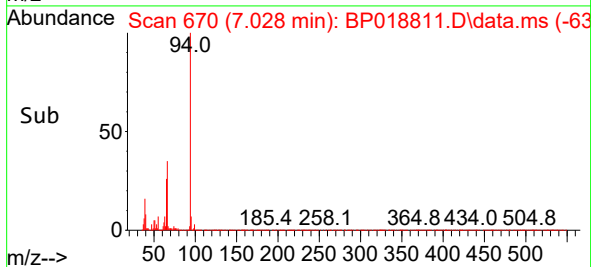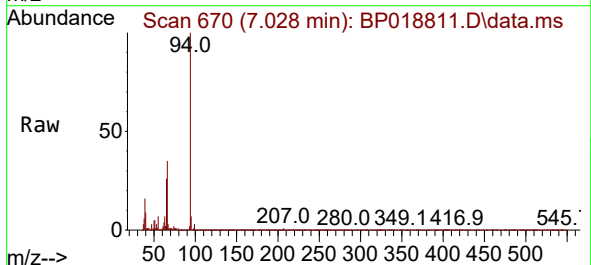



#10

Bis(2-Chloroethyl)ether

Concen: 17.706 ng/ul

RT: 7.263 min Scan# 710

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40

Instrument :

BNA_P

ClientSampleId :

SSTD020724





Tgt Ion: 93 Resp: 370458

Ion Ratio Lower Upper

93 100

63 70.9 58.3 87.5

95 32.6 25.9 38.9

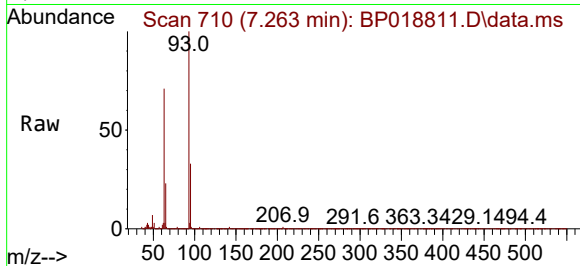

#12

2-Chlorophenol

Concen: 17.484 ng/ul

RT: 7.393 min Scan# 732

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40




Tgt Ion:128 Resp: 358696


Ion Ratio Lower Upper

128 100

64 45.3 37.0 55.4

130 33.4 26.8 40.2

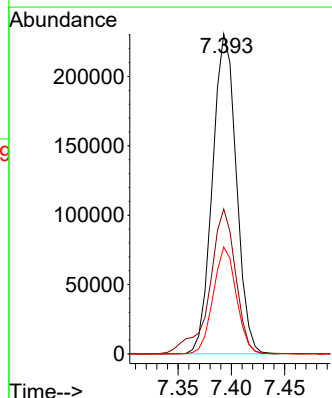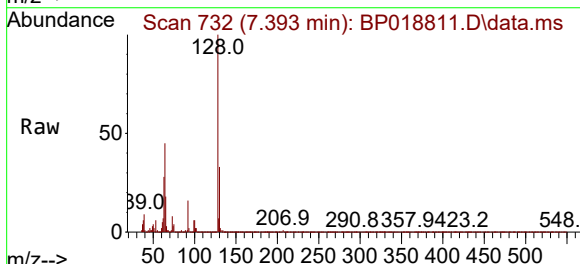



#13

2-Methylphenol

Concen: 16.590 ng/ul

RT: 8.281 min Scan# 883

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40

Instrument :

BNA_P

ClientSampleId :





SSTD020724

Tgt Ion:108 Resp: 323567

Ion Ratio Lower Upper

108 100

107 89.0 70.6 105.8

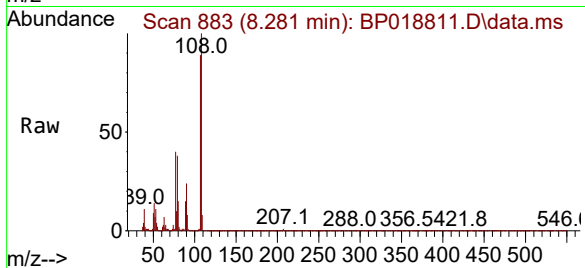

#14

2,2'-oxybis(1-Chloropropane)

Concen: 16.215 ng/ul

RT: 8.357 min Scan# 896

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40




Tgt Ion: 45 Resp: 430454


Ion Ratio Lower Upper

45 100

77 17.3 12.7 19.1

79 12.5 10.5 15.7



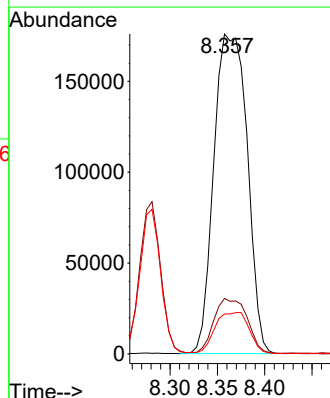
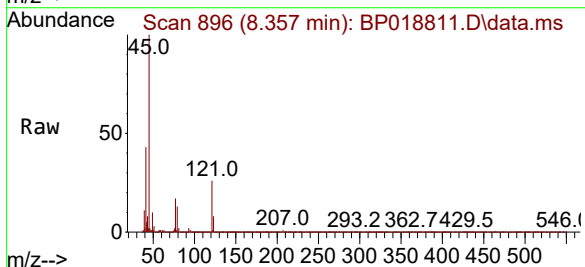




#16
Acetophenone
Concen: 16.504 ng/ul
RT: 8.657 min Scan# 947
Delta R.T. 0.000 min
Lab File: BP018811.D
Acq: 13 Dec 2023 18:40




Instrument :
BNA_P
ClientSampleId :
SSTD020724


Tgt Ion:105 Resp: 517110
Ion Ratio Lower Upper
105 100
77 74.8 59.4 89.0
51 23.4 19.4 29.0



#17
N-Nitroso-di-n-propylamine
Concen: 14.402 ng/ul
RT: 8.646 min Scan# 945
Delta R.T. 0.000 min
Lab File: BP018811.D
Acq: 13 Dec 2023 18:40

Tgt Ion: 70 Resp: 248240
Ion Ratio Lower Upper
70 100
42 49.0 41.0 61.4
101 10.4 7.8 11.8
130 21.5 16.9 25.3









#18
4-Methylphenol
Concen: 16.201 ng/ul
RT: 8.610 min Scan# 910
Delta R.T. 0.000 min
Lab File: BP018811.D
Acq: 13 Dec 2023 18:40




Instrument :
BNA_P
ClientSampleId :
SSTD020724


Tgt Ion:108 Resp: 345025
Ion Ratio Lower Upper
108 100
107 111.3 90.6 136.0



#19
Hexachloroethane
Concen: 18.147 ng/ul
RT: 8.910 min Scan# 990
Delta R.T. 0.000 min
Lab File: BP018811.D
Acq: 13 Dec 2023 18:40

Tgt Ion:117 Resp: 152625
Ion Ratio Lower Upper
117 100
201 121.8 83.7 125.5
199 73.2 52.3 78.5









#22
Nitrobenzene
Concen: 18.501 ng/ul
RT: 9.034 min Scan# 1011
Delta R.T. 0.000 min
Lab File: BP018811.D
Acq: 13 Dec 2023 18:40




Instrument :
BNA_P
ClientSampleId :
SSTD020724


Tgt Ion: 77 Resp: 383319
Ion Ratio Lower Upper
77 100
123 46.1 35.8 53.8
65 13.0 10.5 15.7



#23
Isophorone
Concen: 16.340 ng/ul
RT: 9.563 min Scan# 1101
Delta R.T. 0.000 min
Lab File: BP018811.D
Acq: 13 Dec 2023 18:40

Tgt Ion: 82 Resp: 690264
Ion Ratio Lower Upper
82 100
95 7.0 5.5 8.3
138 18.2 13.5 20.3



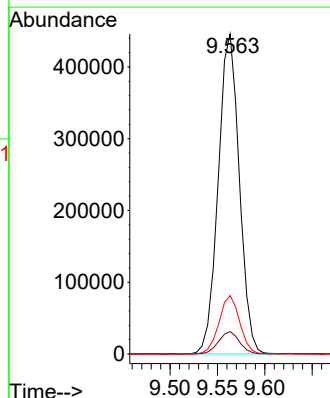





#25
2-Nitrophenol
Concen: 19.173 ng/ul
RT: 9.746 min Scan# 1132
Delta R.T. 0.000 min
Lab File: BP018811.D
Acq: 13 Dec 2023 18:40




Instrument :
BNA_P
ClientSampleId :
SSTD020724


Tgt Ion:139 Resp: 181369
Ion Ratio Lower Upper
139 100
65 47.9 39.1 58.7
109 30.4 23.8 35.6

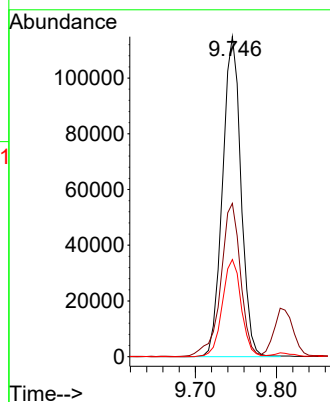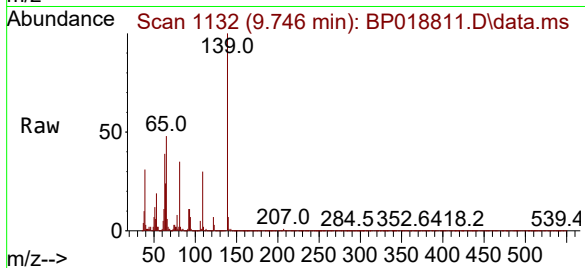

#26
2,4-Dimethylphenol
Concen: 18.340 ng/ul
RT: 9.810 min Scan# 1143
Delta R.T. 0.000 min
Lab File: BP018811.D
Acq: 13 Dec 2023 18:40

Tgt Ion:107 Resp: 339305
Ion Ratio Lower Upper
107 100
121 49.6 40.0 60.0
122 84.7 69.1 103.7




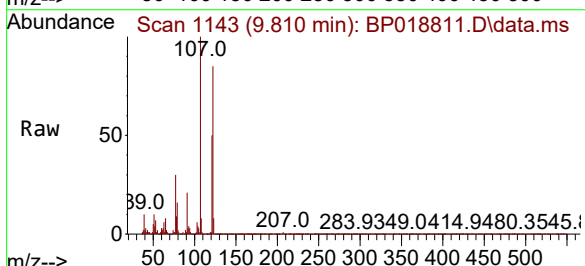




#27
 Bis(2-Chloroethoxy)methane
 Concen: 17.352 ng/ul
 RT: 10.046 min Scan# 1183
 Delta R.T. 0.000 min
 Lab File: BP018811.D
 Acq: 13 Dec 2023 18:40




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020724


Tgt Ion: 93 Resp: 462769
 Ion Ratio Lower Upper
 93 100
 95 32.3 26.1 39.1
 123 11.1 8.9 13.3

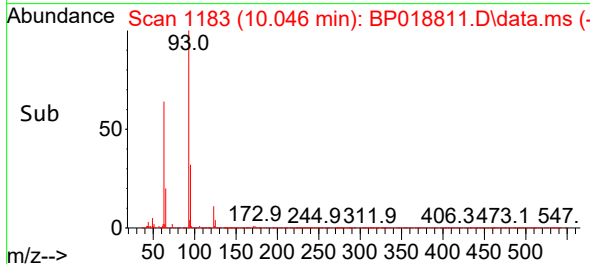

#29
 2,4-Dichlorophenol
 Concen: 19.105 ng/ul
 RT: 10.275 min Scan# 1222
 Delta R.T. 0.000 min
 Lab File: BP018811.D
 Acq: 13 Dec 2023 18:40

Tgt Ion: 162 Resp: 332449
 Ion Ratio Lower Upper
 162 100
 164 65.1 51.7 77.5
 98 34.2 29.2 43.8

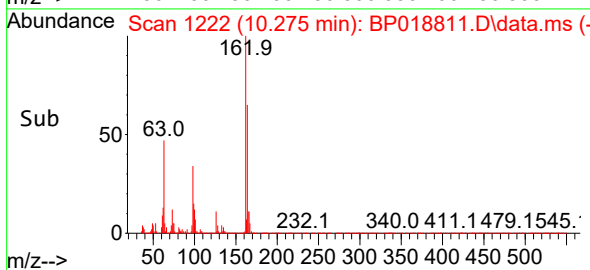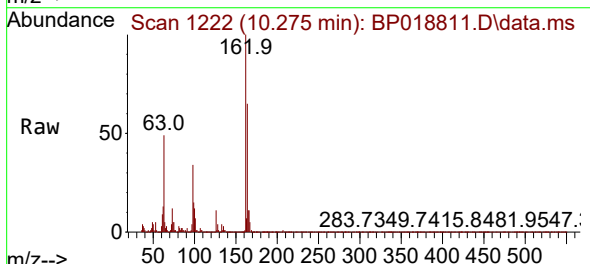



#30

Naphthalene

Concen: 18.740 ng/ul

RT: 10.675 min Scan# 1290

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40

Instrument :

BNA_P

ClientSampleId :

SSTD020724





Tgt Ion:128 Resp: 1088456

Ion Ratio Lower Upper

128 100

129 10.7 8.9 13.3

127 13.5 10.5 15.7

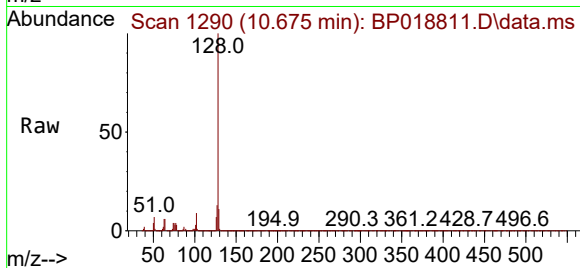

#32

4-Chloroaniline

Concen: 18.240 ng/ul

RT: 10.793 min Scan# 1310

Delta R.T. 0.000 min

Lab File: BP018811.D




Acq: 13 Dec 2023 18:40


Tgt Ion:127 Resp: 410439

Ion Ratio Lower Upper

127 100

129 32.3 25.6 38.4

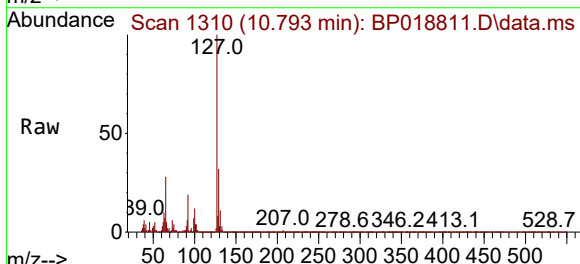



#33

Hexachlorobutadiene

Concen: 21.581 ng/ul

RT: 10.963 min Scan# 1339

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40

Instrument :

BNA_P

ClientSampleId :

SSTD020724





Tgt Ion:225 Resp: 251501

Ion Ratio Lower Upper

225 100

223 63.6 49.5 74.3

227 64.4 50.9 76.3

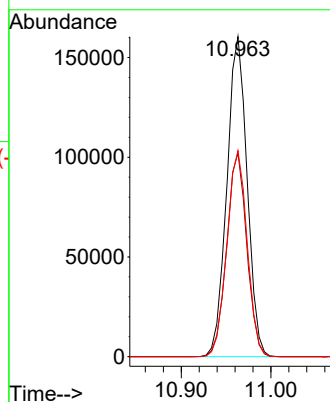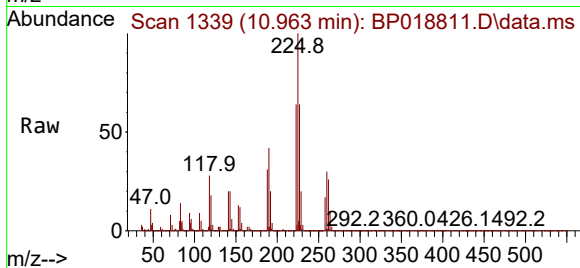

#34

Caprolactam

Concen: 14.747 ng/ul

RT: 11.569 min Scan# 1442

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40




Tgt Ion:113 Resp: 78687


Ion Ratio Lower Upper

113 100

55 151.0 133.7 200.5

56 111.2 97.4 146.2




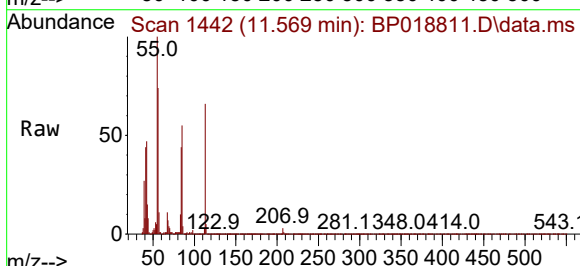




#35
4-Chloro-3-methylphenol
Concen: 16.318 ng/ul
RT: 11.916 min Scan# 1501
Delta R.T. 0.000 min
Lab File: BP018811.D
Acq: 13 Dec 2023 18:40




Instrument :
BNA_P
ClientSampleId :
SSTD020724


Tgt Ion:107 Resp: 318088
Ion Ratio Lower Upper
107 100
144 26.3 21.0 31.6
142 80.7 63.6 95.4

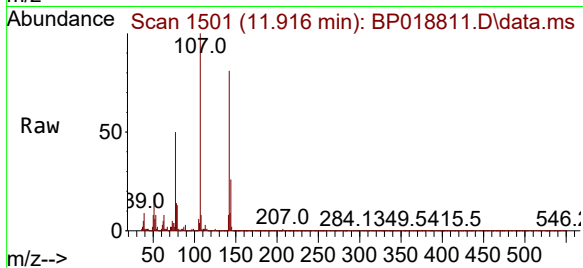

#36
2-Methylnaphthalene
Concen: 17.589 ng/ul
RT: 12.287 min Scan# 1564
Delta R.T. 0.000 min
Lab File: BP018811.D
Acq: 13 Dec 2023 18:40

Tgt Ion:142 Resp: 723741
Ion Ratio Lower Upper
142 100
141 88.5 71.4 107.0




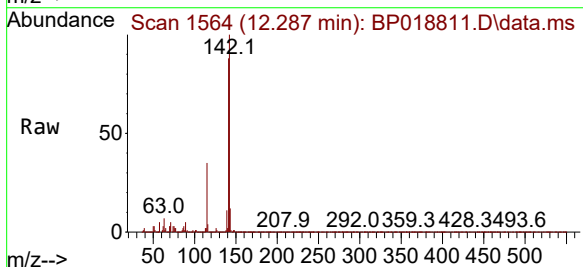




#37
1-Methylnaphthalene
Concen: 17.498 ng/ul
RT: 12.510 min Scan# 1602
Delta R.T. 0.000 min
Lab File: BP018811.D
Acq: 13 Dec 2023 18:40




Instrument :
BNA_P
ClientSampleId :
SSTD020724


Tgt Ion:142 Resp: 727107
Ion Ratio Lower Upper
142 100
141 91.1 73.5 110.3
116 3.5 2.8 4.2

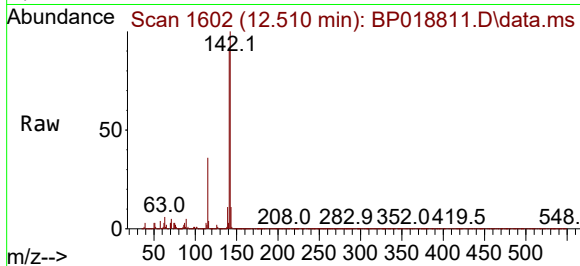

#39
1,2,4,5-Tetrachlorobenzene
Concen: 21.638 ng/ul
RT: 12.657 min Scan# 1627
Delta R.T. 0.000 min
Lab File: BP018811.D
Acq: 13 Dec 2023 18:40

Tgt Ion:216 Resp: 443369
Ion Ratio Lower Upper
216 100
214 76.7 63.9 95.9
179 19.4 16.3 24.5
108 14.4 12.6 19.0

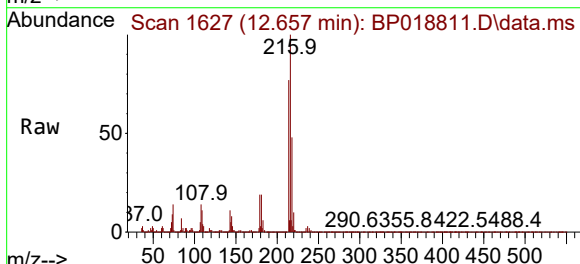



#40

Hexachlorocyclopentadiene

Concen: 20.068 ng/ul

RT: 12.634 min Scan# 1623

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40

Instrument :

BNA_P

ClientSampleId :

SSTD020724





Tgt Ion:237 Resp: 243733

Ion Ratio Lower Upper

237 100

235 62.6 49.4 74.0

272 13.4 9.8 14.8

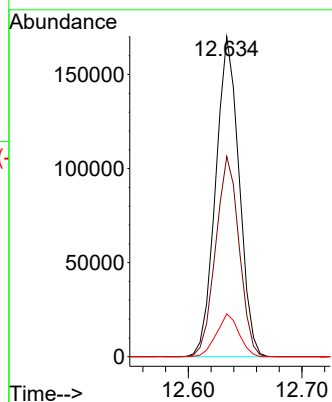

#41

2,4,6-Trichlorophenol

Concen: 19.526 ng/ul

RT: 12.898 min Scan# 1668

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40




Tgt Ion:196 Resp: 257371


Ion Ratio Lower Upper

196 100

198 96.4 76.9 115.3

200 31.2 25.0 37.6





#42

2,4,5-Trichlorophenol

Concen: 19.267 ng/ul

RT: 12.969 min Scan# 1

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40

Instrument :

BNA_P

ClientSampleId :

SSTD020724





Tgt Ion:196 Resp: 275333

Ion Ratio Lower Upper

196 100

198 98.5 77.9 116.9

200 32.0 25.2 37.8



#43

1,1'-Biphenyl

Concen: 19.618 ng/ul

RT: 13.298 min Scan# 1736

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40




Tgt Ion:154 Resp: 958226


Ion Ratio Lower Upper

154 100

153 39.9 32.8 49.2

76 12.8 10.7 16.1

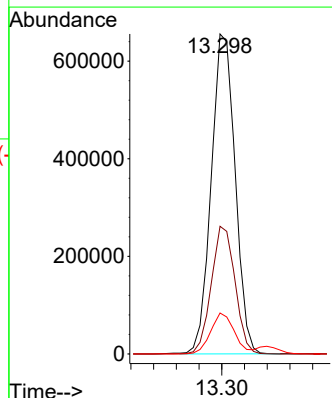



#44

2-Chloronaphthalene

Concen: 19.829 ng/ul

RT: 13.340 min Scan# 1743

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40

Instrument :

BNA_P

ClientSampleId :

SSTD020724





Tgt Ion:162 Resp: 764953

Ion Ratio Lower Upper

162 100

164 32.4 25.7 38.5

127 36.2 30.3 45.5

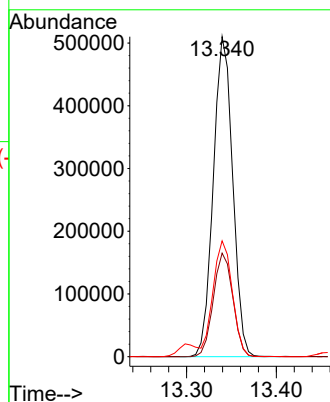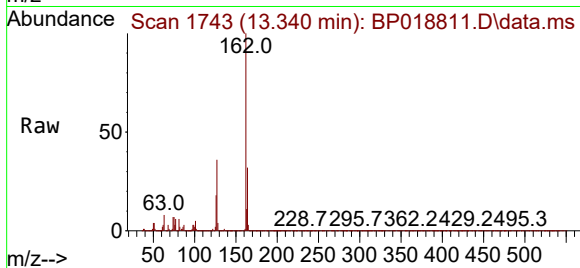

#45

2-Nitroaniline

Concen: 16.860 ng/ul

RT: 13.551 min Scan# 1779

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40




Tgt Ion: 65 Resp: 176319


Ion Ratio Lower Upper

65 100

92 75.9 56.9 85.3

138 116.8 88.2 132.2




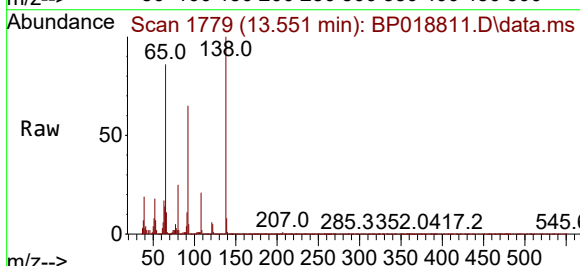




#47
Dimethylphthalate
Concen: 18.267 ng/ul
RT: 13.928 min Scan# 1843
Delta R.T. 0.000 min
Lab File: BP018811.D
Acq: 13 Dec 2023 18:40




Instrument :
BNA_P
ClientSampleId :
SSTD020724


Tgt Ion:163 Resp: 906360
Ion Ratio Lower Upper
163 100
194 4.1 3.2 4.8
164 10.0 8.0 12.0



#48
2,6-Dinitrotoluene
Concen: 17.746 ng/ul
RT: 14.051 min Scan# 1864
Delta R.T. 0.000 min
Lab File: BP018811.D
Acq: 13 Dec 2023 18:40

Tgt Ion:165 Resp: 166355
Ion Ratio Lower Upper
165 100
89 52.1 46.6 70.0
121 20.2 17.3 25.9









#50
Acenaphthylene
Concen: 18.976 ng/ul
RT: 14.187 min Scan# 1184144
Delta R.T. 0.000 min
Lab File: BP018811.D
Acq: 13 Dec 2023 18:40




Instrument :
BNA_P
ClientSampleId :
SSTD020724


Tgt Ion:152 Resp: 1184144
Ion Ratio Lower Upper
152 100
151 19.8 15.9 23.9
153 13.1 10.6 16.0

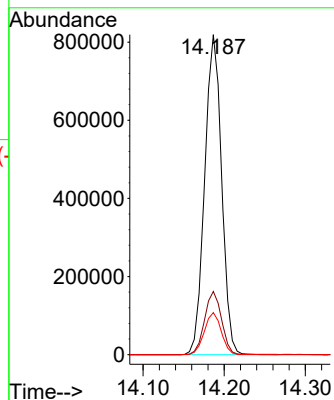

#51
3-Nitroaniline
Concen: 17.359 ng/ul
RT: 14.375 min Scan# 1919
Delta R.T. 0.000 min
Lab File: BP018811.D
Acq: 13 Dec 2023 18:40

Tgt Ion:138 Resp: 162436
Ion Ratio Lower Upper
138 100
108 12.5 9.5 14.3
92 119.4 93.1 139.7



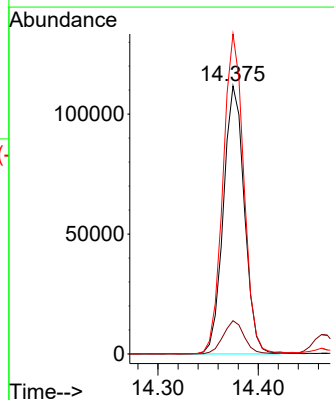





#52
Acenaphthene
Concen: 19.032 ng/ul
RT: 14.528 min Scan# 1945
Delta R.T. 0.000 min
Lab File: BP018811.D
Acq: 13 Dec 2023 18:40




Instrument :
BNA_P
ClientSampleId :
SSTD020724


Tgt Ion:153 Resp: 785252
Ion Ratio Lower Upper
153 100
152 47.9 38.1 57.1
154 87.7 71.7 107.5

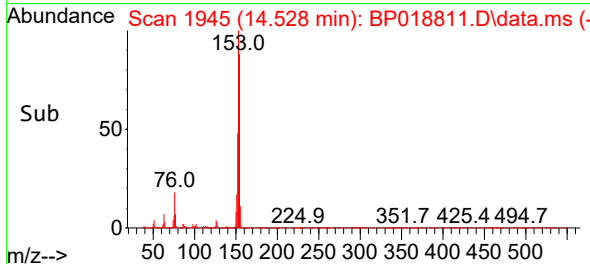

#53
2,4-Dinitrophenol
Concen: 17.047 ng/ul
RT: 14.581 min Scan# 1954
Delta R.T. 0.000 min
Lab File: BP018811.D
Acq: 13 Dec 2023 18:40

Tgt Ion:184 Resp: 84693
Ion Ratio Lower Upper
184 100
63 54.6 48.2 72.4
154 58.9 49.1 73.7


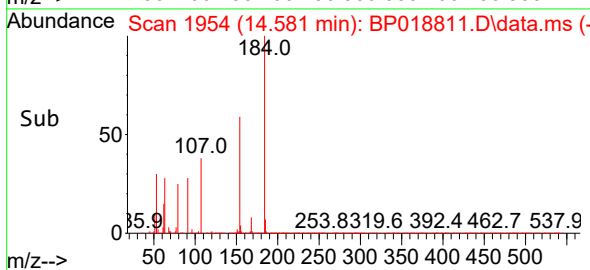

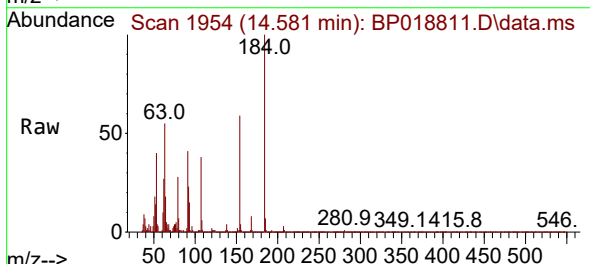




#55
4-Nitrophenol
Concen: 18.241 ng/ul
RT: 14.687 min Scan# 1972
Delta R.T. 0.000 min
Lab File: BP018811.D
Acq: 13 Dec 2023 18:40




Instrument :
BNA_P
ClientSampleId :
SSTD020724


Tgt Ion:109 Resp: 114024
Ion Ratio Lower Upper
109 100
139 135.7 109.0 163.4
65 122.6 106.2 159.4

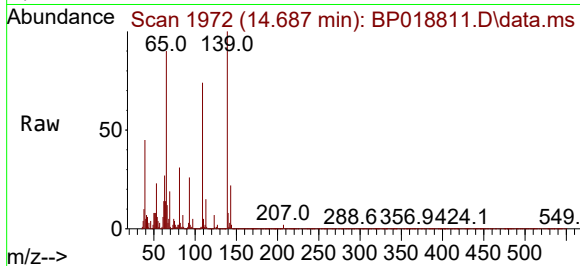

#56
Dibenzofuran
Concen: 19.119 ng/ul
RT: 14.863 min Scan# 2002
Delta R.T. 0.000 min
Lab File: BP018811.D
Acq: 13 Dec 2023 18:40

Tgt Ion:168 Resp: 1096385
Ion Ratio Lower Upper
168 100
139 35.4 29.1 43.7

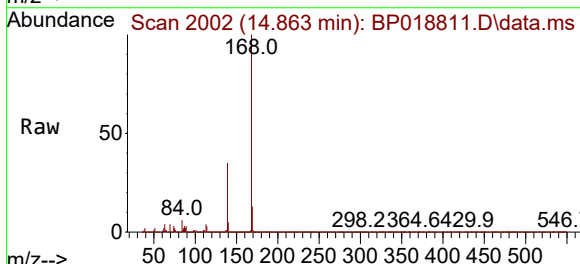



#57

2,4-Dinitrotoluene

Concen: 17.877 ng/ul

RT: 14.834 min Scan# 1997

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40

Instrument :

BNA_P

ClientSampleId :

SSTD020724





Tgt Ion:165 Resp: 235731

Ion Ratio Lower Upper

165 100

63 36.9 32.7 49.1

182 2.8 2.1 3.1



#58

2,3,4,6-Tetrachlorophenol

Concen: 19.149 ng/ul

RT: 15.092 min Scan# 2041

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40

Tgt Ion:232 Resp: 229538




Ion Ratio Lower Upper


232 100

131 36.4 33.8 50.8

130 2.0 1.8 2.8

166 27.9 24.7 37.1

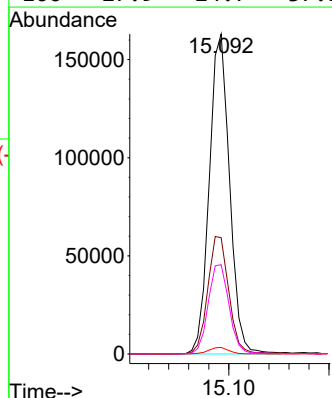



#59

Diethylphthalate

Concen: 17.608 ng/ul

RT: 15.292 min Scan# 2075

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40

Instrument :

BNA_P

ClientSampleId :

SSTD020724





Tgt Ion:149 Resp: 854910

Ion Ratio Lower Upper

149 100

177 23.6 18.2 27.4

150 12.1 9.9 14.9



#61

Fluorene

Concen: 19.264 ng/ul

RT: 15.516 min Scan# 2113

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40




Tgt Ion:166 Resp: 874127


Ion Ratio Lower Upper

166 100

165 97.8 78.0 117.0

167 13.4 10.8 16.2









#62
4-Chlorophenyl-phenylether
Concen: 19.799 ng/ul
RT: 15.510 min Scan# 2112
Delta R.T. 0.000 min
Lab File: BP018811.D
Acq: 13 Dec 2023 18:40




Instrument :
BNA_P
ClientSampleId :
SSTD020724


Tgt Ion:204 Resp: 471175
Ion Ratio Lower Upper
204 100
206 32.6 27.1 40.7
141 50.9 45.8 68.8

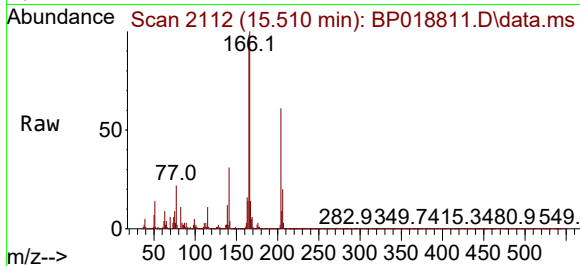

#63
4-Nitroaniline
Concen: 17.605 ng/ul
RT: 15.539 min Scan# 2117
Delta R.T. 0.000 min
Lab File: BP018811.D
Acq: 13 Dec 2023 18:40

Tgt Ion:138 Resp: 156945
Ion Ratio Lower Upper
138 100
92 49.9 42.3 63.5
108 75.0 62.0 93.0




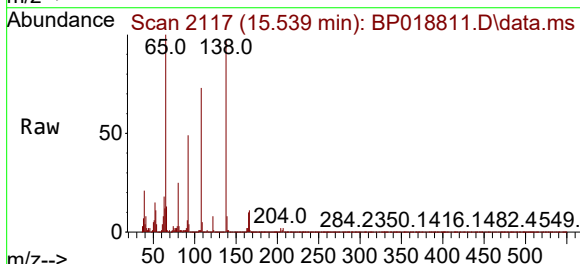




#66
4,6-Dinitro-2-methylphenol
Concen: 18.941 ng/ul
RT: 15.592 min Scan# 2126
Delta R.T. 0.000 min
Lab File: BP018811.D
Acq: 13 Dec 2023 18:40




Instrument :
BNA_P
ClientSampleId :
SSTD020724


Tgt Ion:198 Resp: 143285
Ion Ratio Lower Upper
198 100
182 4.7 3.4 5.2
77 22.8 20.6 30.8

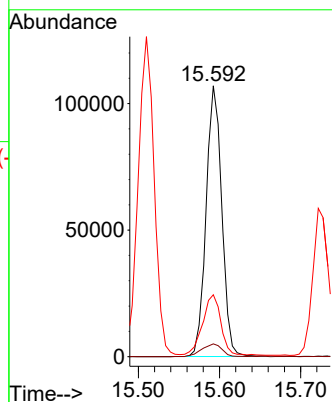

#67
N-Nitrosodiphenylamine
Concen: 18.570 ng/ul
RT: 15.728 min Scan# 2149
Delta R.T. 0.000 min
Lab File: BP018811.D
Acq: 13 Dec 2023 18:40

Tgt Ion:169 Resp: 726163
Ion Ratio Lower Upper
169 100
168 67.0 53.1 79.7
167 36.2 29.1 43.7


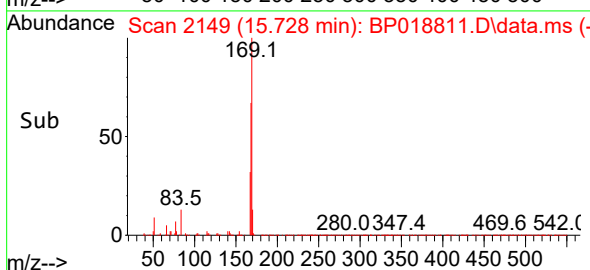






#68
4-Bromophenyl-phenylether
Concen: 19.349 ng/ul
RT: 16.404 min Scan# 2264
Delta R.T. 0.000 min
Lab File: BP018811.D
Acq: 13 Dec 2023 18:40




Instrument :
BNA_P
ClientSampleId :
SSTD020724


Tgt Ion:	248	Resp:	288260
Ion Ratio	Lower	Upper	
248	100		
250	96.6	79.3	118.9
141	64.7	57.2	85.8



#69
Hexachlorobenzene
Concen: 19.988 ng/ul
RT: 16.516 min Scan# 2283
Delta R.T. 0.000 min
Lab File: BP018811.D
Acq: 13 Dec 2023 18:40

Tgt Ion:	284	Resp:	332475
Ion Ratio	Lower	Upper	
284	100		
142	29.0	25.8	38.6
249	31.5	24.9	37.3

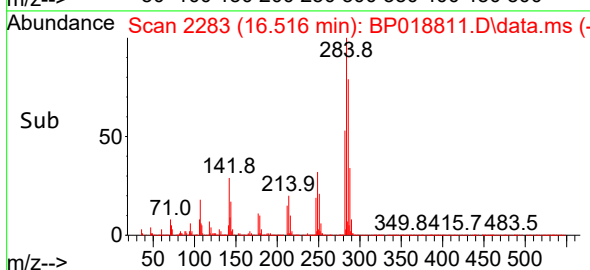



#70

Atrazine

Concen: 14.382 ng/ul

RT: 16.681 min Scan# 21

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40

Instrument :

BNA_P

ClientSampleId :

SSTD020724





Tgt Ion:200 Resp: 167200

Ion Ratio Lower Upper

200 100

173 24.8 21.0 31.4

215 48.4 38.2 57.2

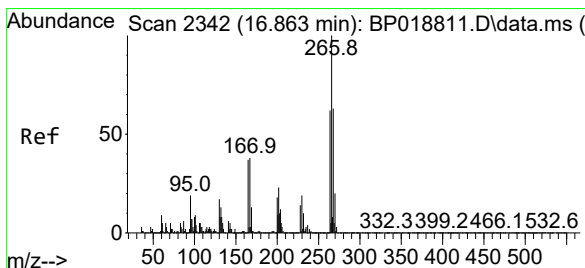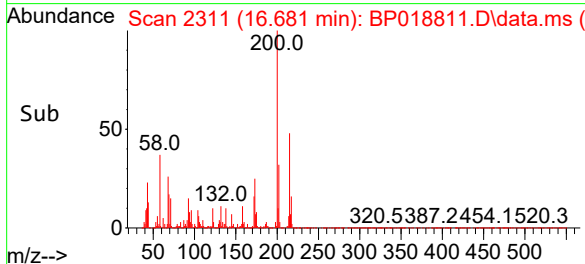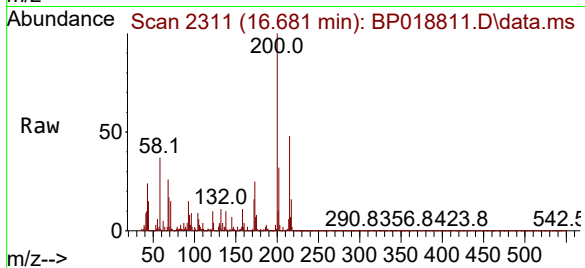

#71

Pentachlorophenol

Concen: 19.109 ng/ul

RT: 16.863 min Scan# 2342

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40




Tgt Ion:266 Resp: 189039


Ion Ratio Lower Upper

266 100

264 61.9 50.2 75.2

268 63.5 50.5 75.7

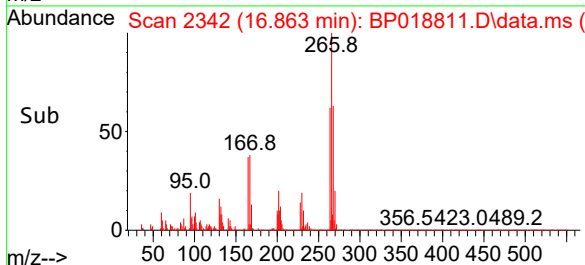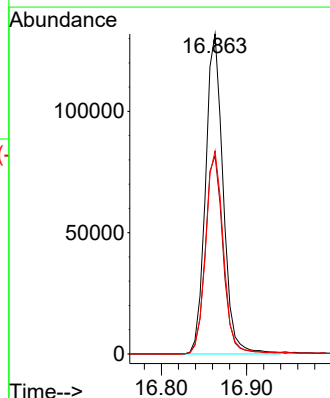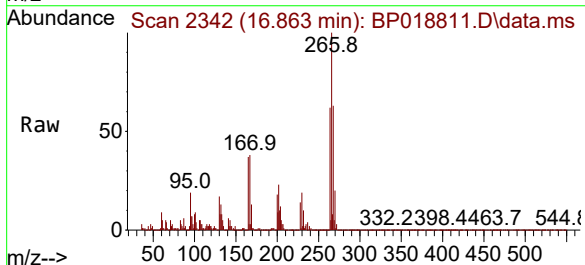



#72

Phenanthrene

Concen: 19.077 ng/ul

RT: 17.257 min Scan# 2409

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40

Instrument :

BNA_P

ClientSampleId :

SSTD020724





Tgt Ion:178 Resp: 1359620

Ion Ratio Lower Upper

178 100

179 15.2 12.3 18.5

176 18.9 15.4 23.2

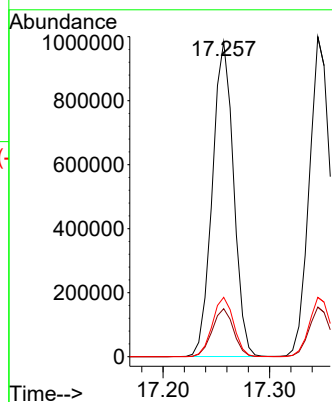

#74

Anthracene

Concen: 19.335 ng/ul

RT: 17.345 min Scan# 2424

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40




Tgt Ion:178 Resp: 1381276


Ion Ratio Lower Upper

178 100

179 15.5 12.5 18.7

176 18.6 15.0 22.6





#75

1,2,3,4-Tetrachlorobenzene

Concen: 21.173 ng/uL

RT: 13.263 min Scan# 1730

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40

Instrument :

BNA_P

ClientSampleId :

SSTD020724





Tgt Ion:216 Resp: 432024

Ion Ratio Lower Upper

216 100

214 77.8 61.4 92.2

218 49.2 39.2 58.8

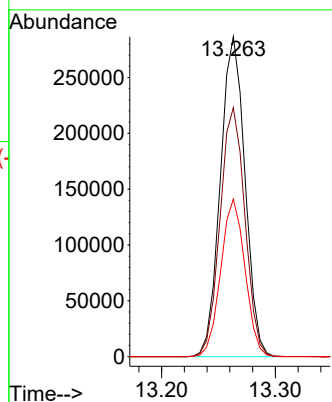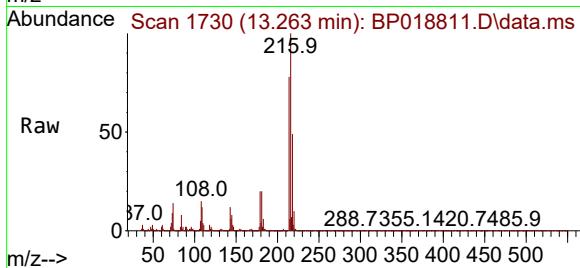

#76

Pentachlorobenzene

Concen: 20.535 ng/uL

RT: 14.781 min Scan# 1988

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40




Tgt Ion:250 Resp: 411597


Ion Ratio Lower Upper

250 100

248 62.9 50.6 75.8

252 62.6 51.3 76.9

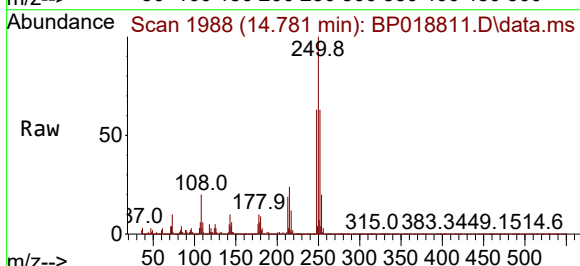



#77

Carbazole

Concen: 20.976 ng/ul

RT: 17.622 min Scan# 2471

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40

Instrument :

BNA_P

ClientSampleId :

SSTD020724





Tgt Ion:167 Resp: 1194330

Ion Ratio Lower Upper

167 100

166 21.9 17.1 25.7

139 12.2 10.2 15.4

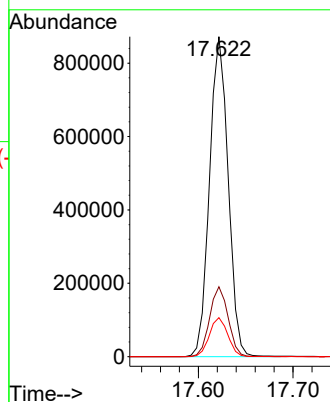

#78

Di-n-butylphthalate

Concen: 18.629 ng/ul

RT: 18.180 min Scan# 2566

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40




Tgt Ion:149 Resp: 1412394


Ion Ratio Lower Upper

149 100

150 8.8 7.4 11.2

104 4.9 3.9 5.9





#80

Fluoranthene

Concen: 14.543 ng/ul

RT: 19.227 min Scan# 2744

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40

Instrument :

BNA_P

ClientSampleId :

SSTD020724





Tgt Ion:202 Resp: 1642645

Ion Ratio Lower Upper

202 100

101 10.0 9.1 13.7

100 7.6 7.1 10.7



#82

Pyrene

Concen: 14.968 ng/ul

RT: 19.580 min Scan# 2804

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40




Tgt Ion:202 Resp: 1705488


Ion Ratio Lower Upper

202 100

101 11.8 11.0 16.4

100 9.8 9.1 13.7





#83

Butylbenzylphthalate

Concen: 15.201 ng/ul

RT: 20.457 min Scan# 2953

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40

Instrument :

BNA_P

ClientSampleId :

SSTD020724





Tgt Ion:149 Resp: 634095

Ion Ratio Lower Upper

149 100

91 70.3 56.6 85.0

206 22.3 17.4 26.0

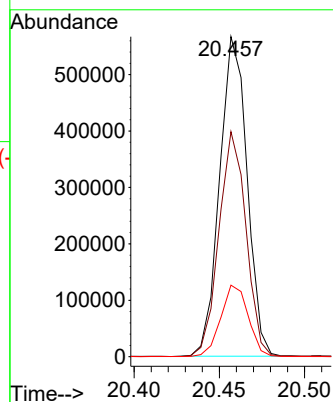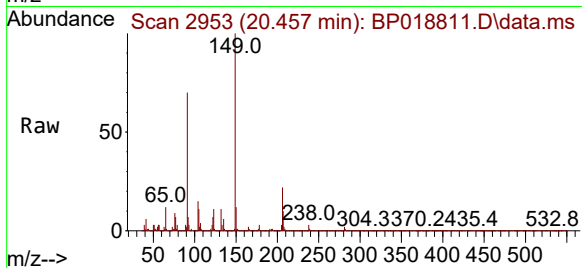

#84

3,3'-Dichlorobenzidine

Concen: 19.158 ng/ul

RT: 21.227 min Scan# 3084

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40




Tgt Ion:252 Resp: 571481


Ion Ratio Lower Upper

252 100

254 65.3 51.0 76.4

126 8.9 7.8 11.6

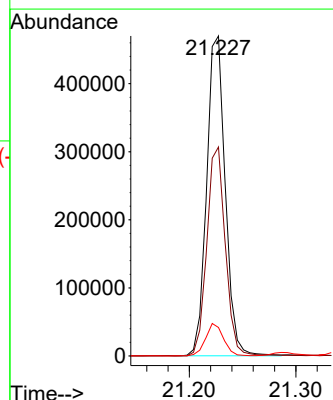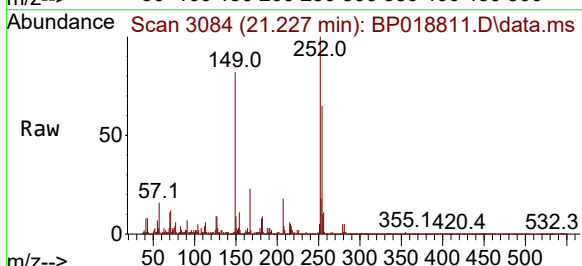



#85

Benzo(a)anthracene

Concen: 18.569 ng/ul

RT: 21.286 min Scan# 3094

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40

Instrument :

BNA_P

ClientSampleId :

SSTD020724





Tgt Ion:228 Resp: 1850116

Ion Ratio Lower Upper

228 100

229 19.6 15.7 23.5

226 27.2 21.9 32.9

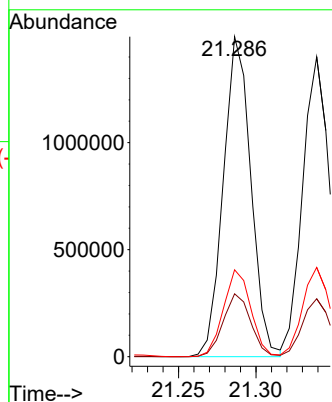

#86

Bis(2-ethylhexyl)phthalate

Concen: 17.053 ng/ul

RT: 21.216 min Scan# 3082

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40




Tgt Ion:149 Resp: 977691


Ion Ratio Lower Upper

149 100

167 28.0 22.2 33.2

279 4.2 3.3 4.9





#87

Chrysene

Concen: 18.669 ng/ul

RT: 21.339 min Scan# 3103

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40

Instrument :

BNA_P

ClientSampleId :

SSTD020724





Tgt Ion:228 Resp: 1712935

Ion Ratio Lower Upper

228 100

226 29.8 23.9 35.9

229 19.3 15.6 23.4

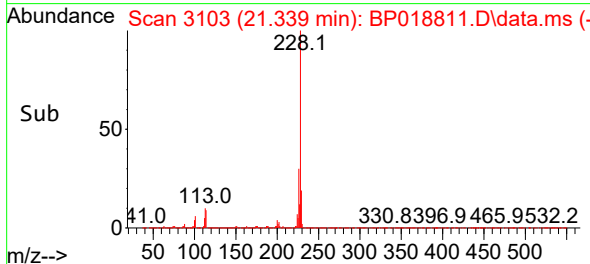

#89

Di-n-octyl phthalate

Concen: 15.707 ng/ul




RT: 22.127 min Scan# 3237


Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40

Tgt Ion:149 Resp: 1690815

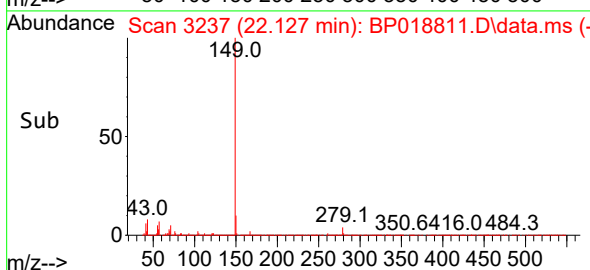



#90

Benzo(b)fluoranthene

Concen: 18.034 ng/ul

RT: 22.945 min Scan# 3376

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40

Instrument :

BNA_P

ClientSampleId :

SSTD020724





Tgt Ion:252 Resp: 1960415

Ion Ratio Lower Upper

252 100

253 22.0 17.3 25.9

125 8.9 7.8 11.6

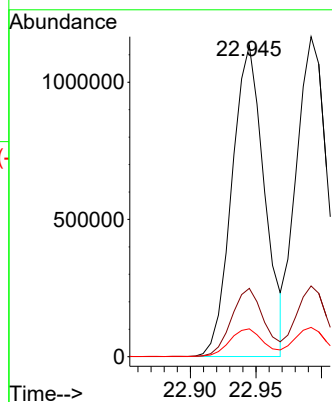

#91

Benzo(k)fluoranthene

Concen: 18.169 ng/ul

RT: 22.992 min Scan# 3384

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40




Tgt Ion:252 Resp: 1911056


Ion Ratio Lower Upper

252 100

253 22.1 17.7 26.5

125 9.1 8.0 12.0





#93

Benzo(a)pyrene

Concen: 18.707 ng/ul

RT: 23.563 min Scan# 3481

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40

Instrument :

BNA_P

ClientSampleId :

SSTD020724





Tgt Ion:252 Resp: 1858177

Ion Ratio Lower Upper

252 100

253 21.8 17.8 26.8

125 10.1 9.2 13.8

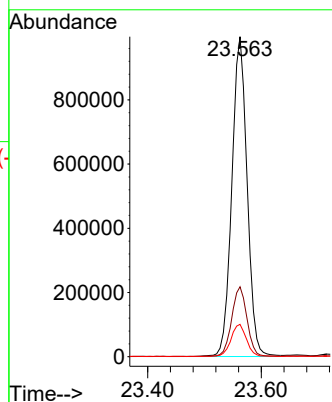

#94

Indeno(1,2,3-cd)pyrene

Concen: 19.973 ng/ul

RT: 26.121 min Scan# 3916

Delta R.T. 0.000 min

Lab File: BP018811.D

Acq: 13 Dec 2023 18:40




Tgt Ion:276 Resp: 2370276


Ion Ratio Lower Upper

276 100

138 21.9 19.4 29.2

277 25.4 19.8 29.6









#95
 Dibenzo(a,h)anthracene
 Concen: 20.120 ng/ul
 RT: 26.139 min Scan# 3919
 Delta R.T. 0.000 min
 Lab File: BP018811.D
 Acq: 13 Dec 2023 18:40

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020724

Tgt Ion:278 Resp: 1986339
 Ion Ratio Lower Upper
 278 100
 139 14.4 13.0 19.6
 279 24.3 18.7 28.1



#96
 Benzo(g,h,i)perylene
 Concen: 19.868 ng/ul
 RT: 26.874 min Scan# 4044
 Delta R.T. 0.000 min
 Lab File: BP018811.D
 Acq: 13 Dec 2023 18:40

Tgt Ion:276 Resp: 1897520
 Ion Ratio Lower Upper
 276 100
 138 18.8 18.1 27.1
 277 23.9 19.4 29.0

