

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018816.D
 Acq On : 13 Dec 2023 21:30
 Operator : MA/JU
 Sample : 05627-19
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLD1

Quant Time: Dec 13 23:35:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 13 23:34:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.834	152	238086	20.000	ng/ul	0.00
20) Naphthalene-d8	10.628	136	877182	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.463	164	525589	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.210	188	1192876	20.000	ng/ul	0.00
79) Chrysene-d12	21.298	240	1283611	20.000	ng/ul	0.00
88) Perylene-d12	23.662	264	1523700	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	31208	4.467	ng/uL	0.00
4) Pyridine-d5	3.681	84	213985	11.434	ng/ul	0.00
7) Phenol-d5	7.005	99	83707	3.503	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.169	67	370815	26.186	ng/ul	0.00
11) 2-Chlorophenol-d4	7.363	132	228604	12.262	ng/ul	0.00
15) 4-Methylphenol-d8	8.546	113	171201	8.854	ng/ul	0.00
21) Nitrobenzene-d5	8.993	128	212683	27.242	ng/ul	0.00
24) 2-Nitrophenol-d4	9.716	143	126583	15.639	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.251	165	247619	14.961	ng/ul	0.00
31) 4-Chloroaniline-d4	10.769	131	499952	23.114	ng/ul	0.00
46) Dimethylphthalate-d6	13.881	166	1390892	29.651	ng/ul	0.00
49) Acenaphthylene-d8	14.157	160	1490345	28.853	ng/ul	0.00
54) 4-Nitrophenol-d4	14.681	143	22499	2.922	ng/ul	0.01
60) Fluorene-d10	15.457	176	1214054	30.833	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.575	200	84198	11.772	ng/ul	0.00
73) Anthracene-d10	17.310	188	2148857	34.266	ng/ul	0.00
81) Pyrene-d10	19.551	212	2728936	27.312	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.510	264	3042689	34.248	ng/ul	0.00


Target Compounds					Qvalue
78) Di-n-butylphthalate	18.180	149	15000027	195.727	ng/ul# 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018816.D
Acq On : 13 Dec 2023 21:30
Operator : MA/JU
Sample : 05627-19
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLD1


Quant Time: Dec 13 23:35:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 13 23:34:47 2023
Response via : Initial Calibration

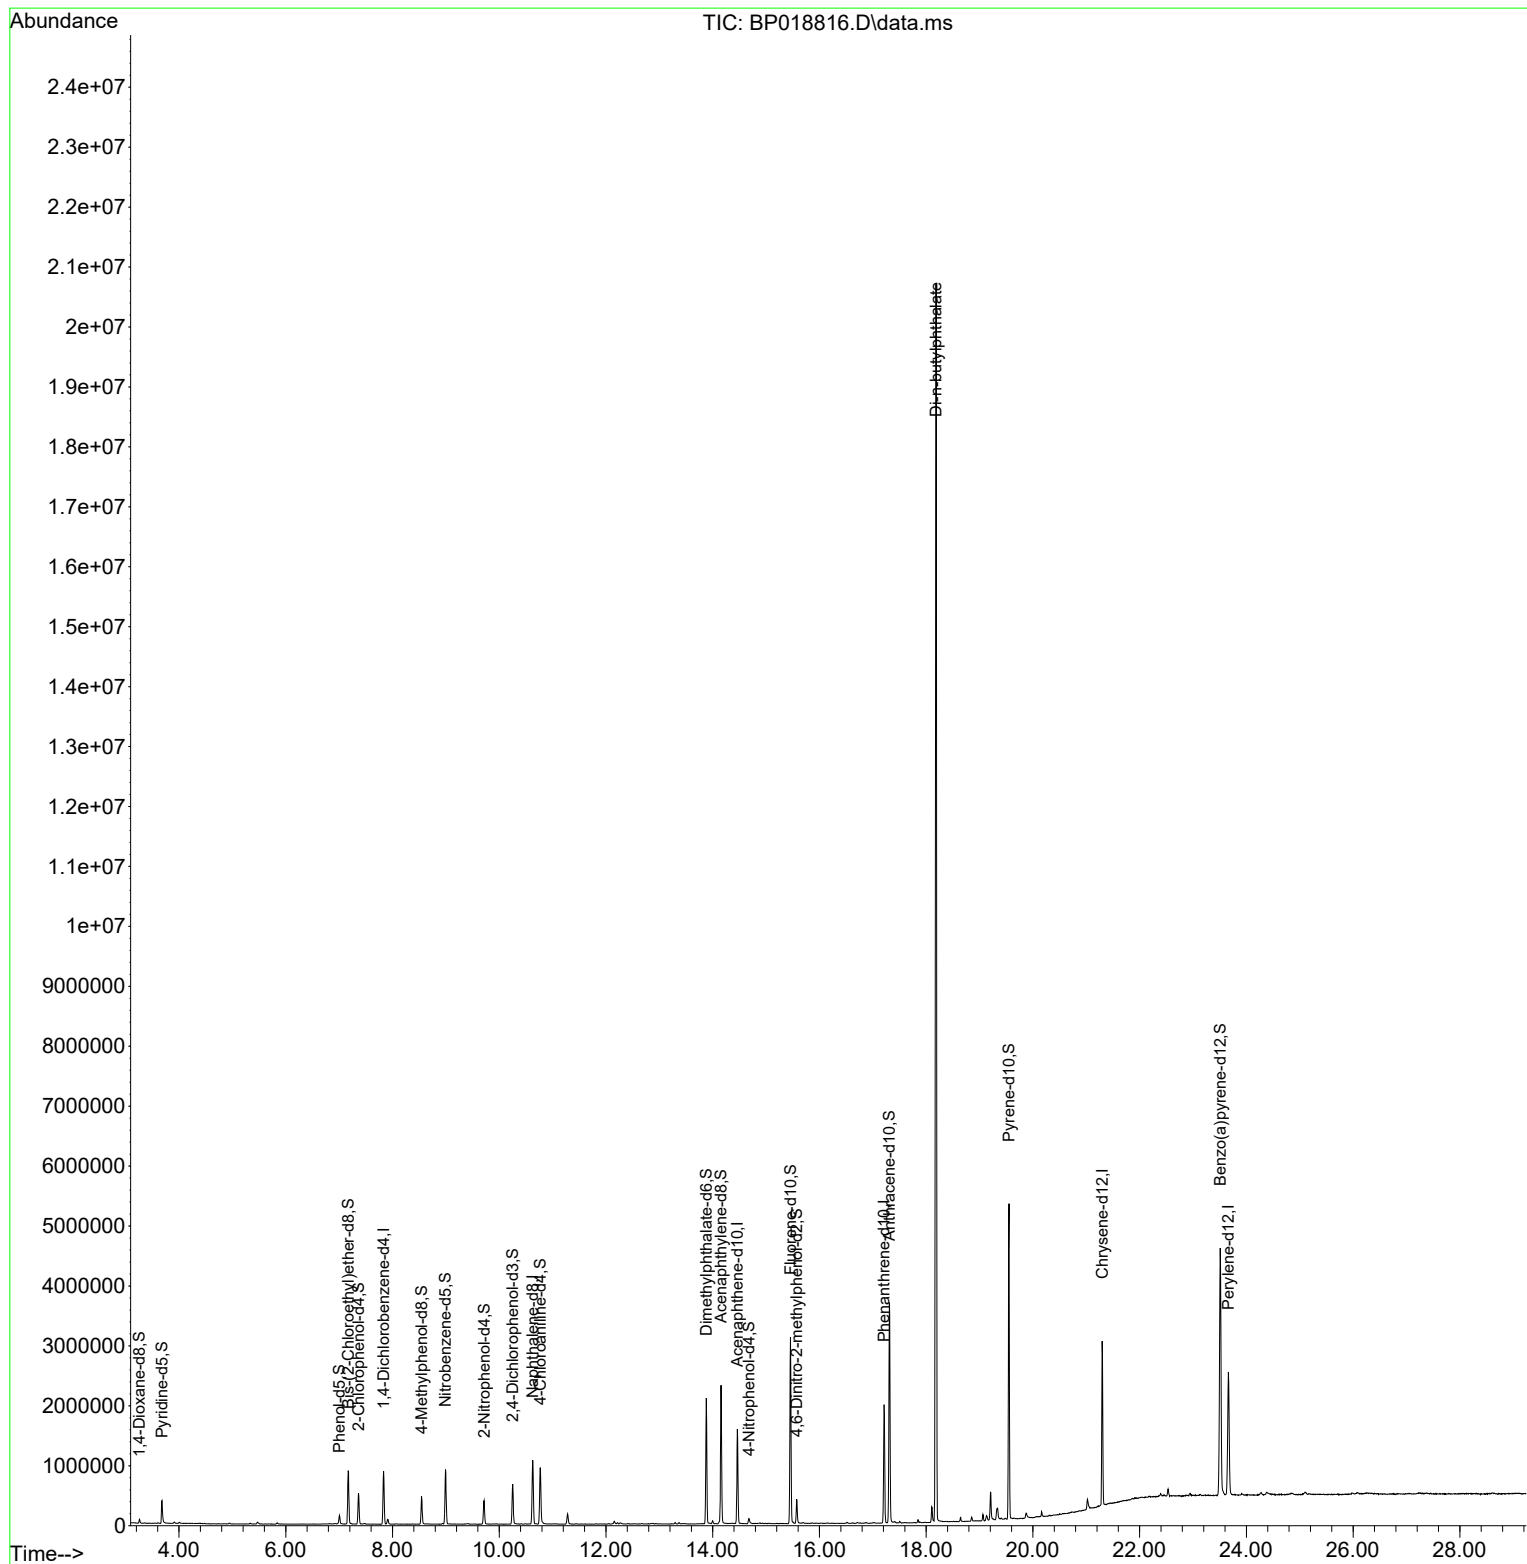

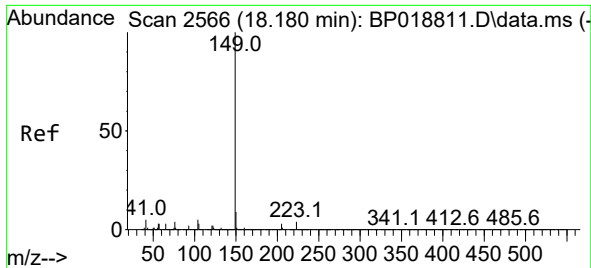

#78
 Di-n-butylphthalate
 Concen: 195.727 ng/ul
 RT: 18.180 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BP018816.D
 Acq: 13 Dec 2023 21:30

Instrument :
 BNA_P
 ClientSampleId :
 DCLD1

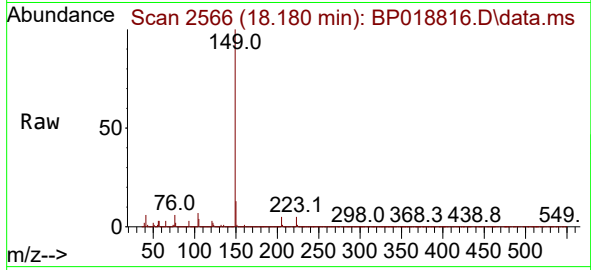

Tgt Ion:149 Resp:15000027
 Ion Ratio Lower Upper
 149 100
 150 12.6 7.4 11.2#
 104 6.7 3.9 5.9#

