

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018817.D
 Acq On : 13 Dec 2023 22:04
 Operator : MA/JU
 Sample : 05627-20
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLD2

Quant Time: Dec 13 23:36:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 13 23:34:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.834	152	244868	20.000	ng/ul	0.00
20) Naphthalene-d8	10.628	136	910542	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.463	164	554541	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.210	188	1325435	20.000	ng/ul	0.00
79) Chrysene-d12	21.298	240	1410784	20.000	ng/ul	0.00
88) Perylene-d12	23.663	264	1653891	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	32719	4.553	ng/uL	0.00
4) Pyridine-d5	3.681	84	198687	10.323	ng/ul	0.00
7) Phenol-d5	7.005	99	175419	7.139	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.169	67	397417	27.287	ng/ul	0.00
11) 2-Chlorophenol-d4	7.364	132	430625	22.458	ng/ul	0.00
15) 4-Methylphenol-d8	8.546	113	298472	15.009	ng/ul	0.00
21) Nitrobenzene-d5	8.993	128	240842	29.718	ng/ul	0.00
24) 2-Nitrophenol-d4	9.716	143	248610	29.589	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.252	165	485093	28.235	ng/ul	0.00
31) 4-Chloroaniline-d4	10.769	131	464317	20.680	ng/ul	0.00
46) Dimethylphthalate-d6	13.881	166	1710696	34.564	ng/ul	0.00
49) Acenaphthylene-d8	14.157	160	1833055	33.635	ng/ul	0.00
54) 4-Nitrophenol-d4	14.675	143	67354	8.291	ng/ul	0.00
60) Fluorene-d10	15.457	176	1490338	35.873	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.575	200	228166	28.710	ng/ul	0.00
73) Anthracene-d10	17.310	188	2532314	36.342	ng/ul	0.00
81) Pyrene-d10	19.545	212	3223120	29.350	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.510	264	3490981	36.201	ng/ul	0.00


Target Compounds					Qvalue	
78) Di-n-butylphthalate	18.181	149	12959135	152.185	ng/ul#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018817.D
Acq On : 13 Dec 2023 22:04
Operator : MA/JU
Sample : 05627-20
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLD2


Quant Time: Dec 13 23:36:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 13 23:34:47 2023
Response via : Initial Calibration

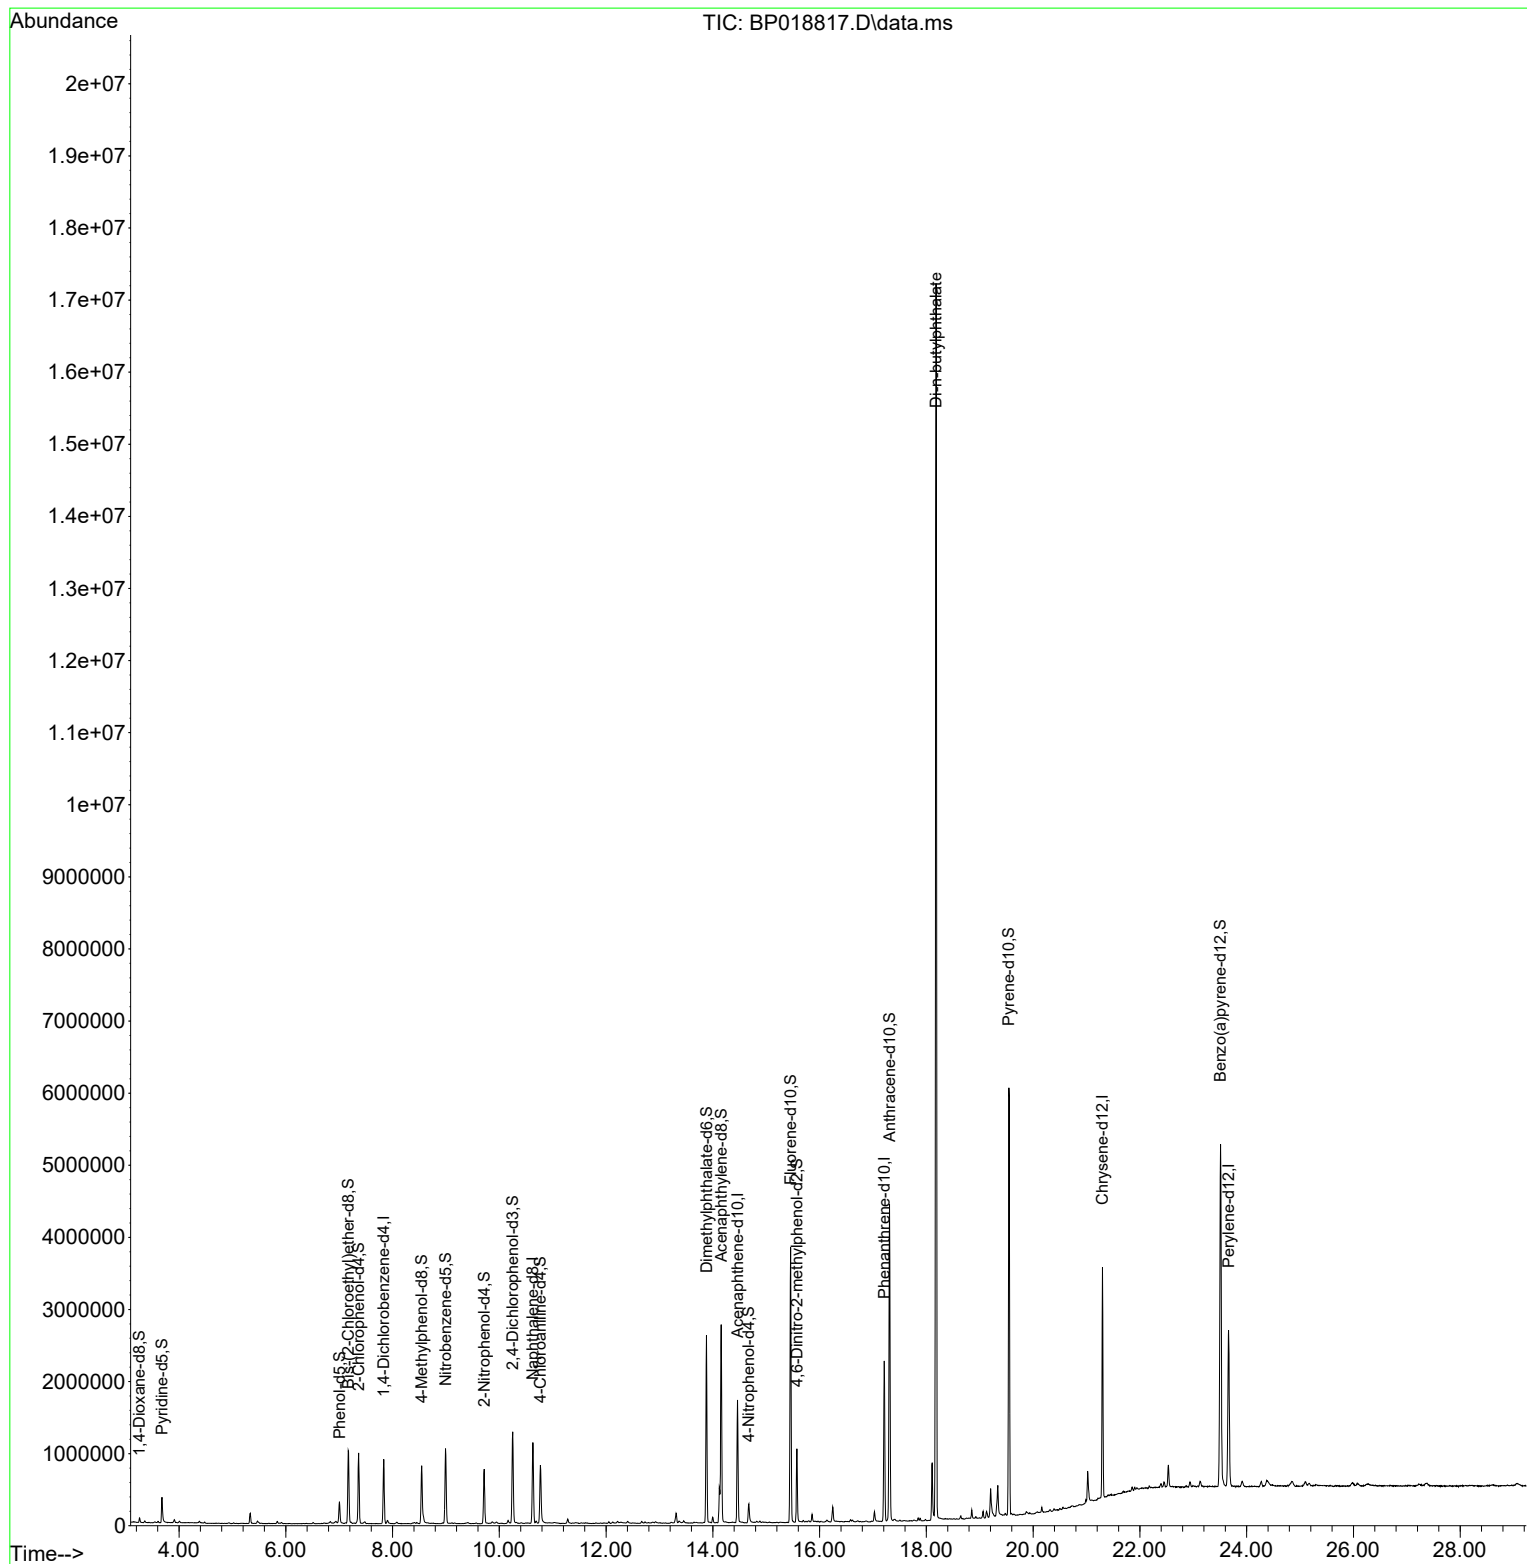

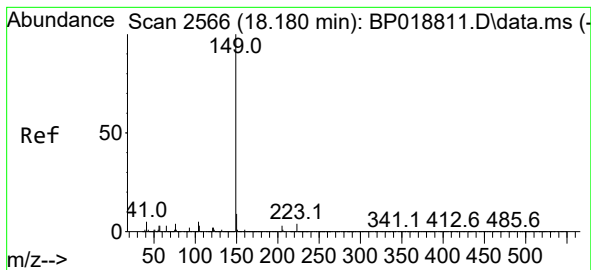

#78
 Di-n-butylphthalate
 Concen: 152.185 ng/ul
 RT: 18.181 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BP018817.D
 Acq: 13 Dec 2023 22:04

Instrument :
 BNA_P
 ClientSampleId :
 DCLD2

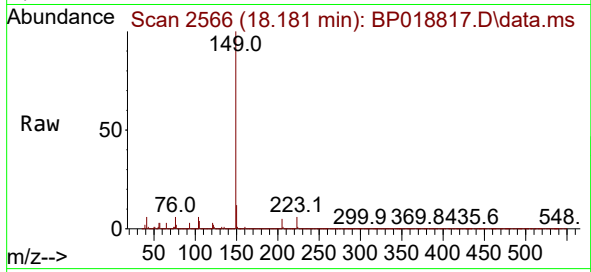

Tgt Ion:149 Resp:12959135
 Ion Ratio Lower Upper
 149 100
 150 12.2 7.4 11.2#
 104 6.4 3.9 5.9#

