

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018818.D
 Acq On : 13 Dec 2023 22:38
 Operator : MA/JU
 Sample : 05627-21
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLD3

Quant Time: Dec 13 23:36:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 13 23:34:47 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.834	152	252167	20.000	ng/ul	0.00
20) Naphthalene-d8	10.628	136	924787	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.463	164	552406	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.210	188	1255532	20.000	ng/ul	0.00
79) Chrysene-d12	21.298	240	1364977	20.000	ng/ul	0.00
88) Perylene-d12	23.663	264	1613614	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	30219	4.084	ng/uL	0.00
4) Pyridine-d5	3.681	84	133411	6.731	ng/ul	0.00
7) Phenol-d5	7.005	99	156909	6.200	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.169	67	373642	24.912	ng/ul	0.00
11) 2-Chlorophenol-d4	7.364	132	399377	20.226	ng/ul	0.00
15) 4-Methylphenol-d8	8.546	113	260844	12.737	ng/ul	0.00
21) Nitrobenzene-d5	8.993	128	227314	27.617	ng/ul	0.00
24) 2-Nitrophenol-d4	9.716	143	226259	26.514	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.252	165	426888	24.465	ng/ul	0.00
31) 4-Chloroaniline-d4	10.769	131	520292	22.816	ng/ul	0.00
46) Dimethylphthalate-d6	13.881	166	1497602	30.376	ng/ul	0.00
49) Acenaphthylene-d8	14.157	160	1555556	28.653	ng/ul	0.00
54) 4-Nitrophenol-d4	14.669	143	55243	6.826	ng/ul	0.00
60) Fluorene-d10	15.457	176	1295097	31.294	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.575	200	195328	25.946	ng/ul	0.00
73) Anthracene-d10	17.310	188	2240387	33.942	ng/ul	0.00
81) Pyrene-d10	19.551	212	2966173	27.916	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.510	264	3261997	34.671	ng/ul	0.00
Target Compounds						
78) Di-n-butylphthalate	18.181	149	7452831	92.395	ng/ul	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018818.D
Acq On : 13 Dec 2023 22:38
Operator : MA/JU
Sample : 05627-21
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLD3

Quant Time: Dec 13 23:36:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 13 23:34:47 2023
Response via : Initial Calibration

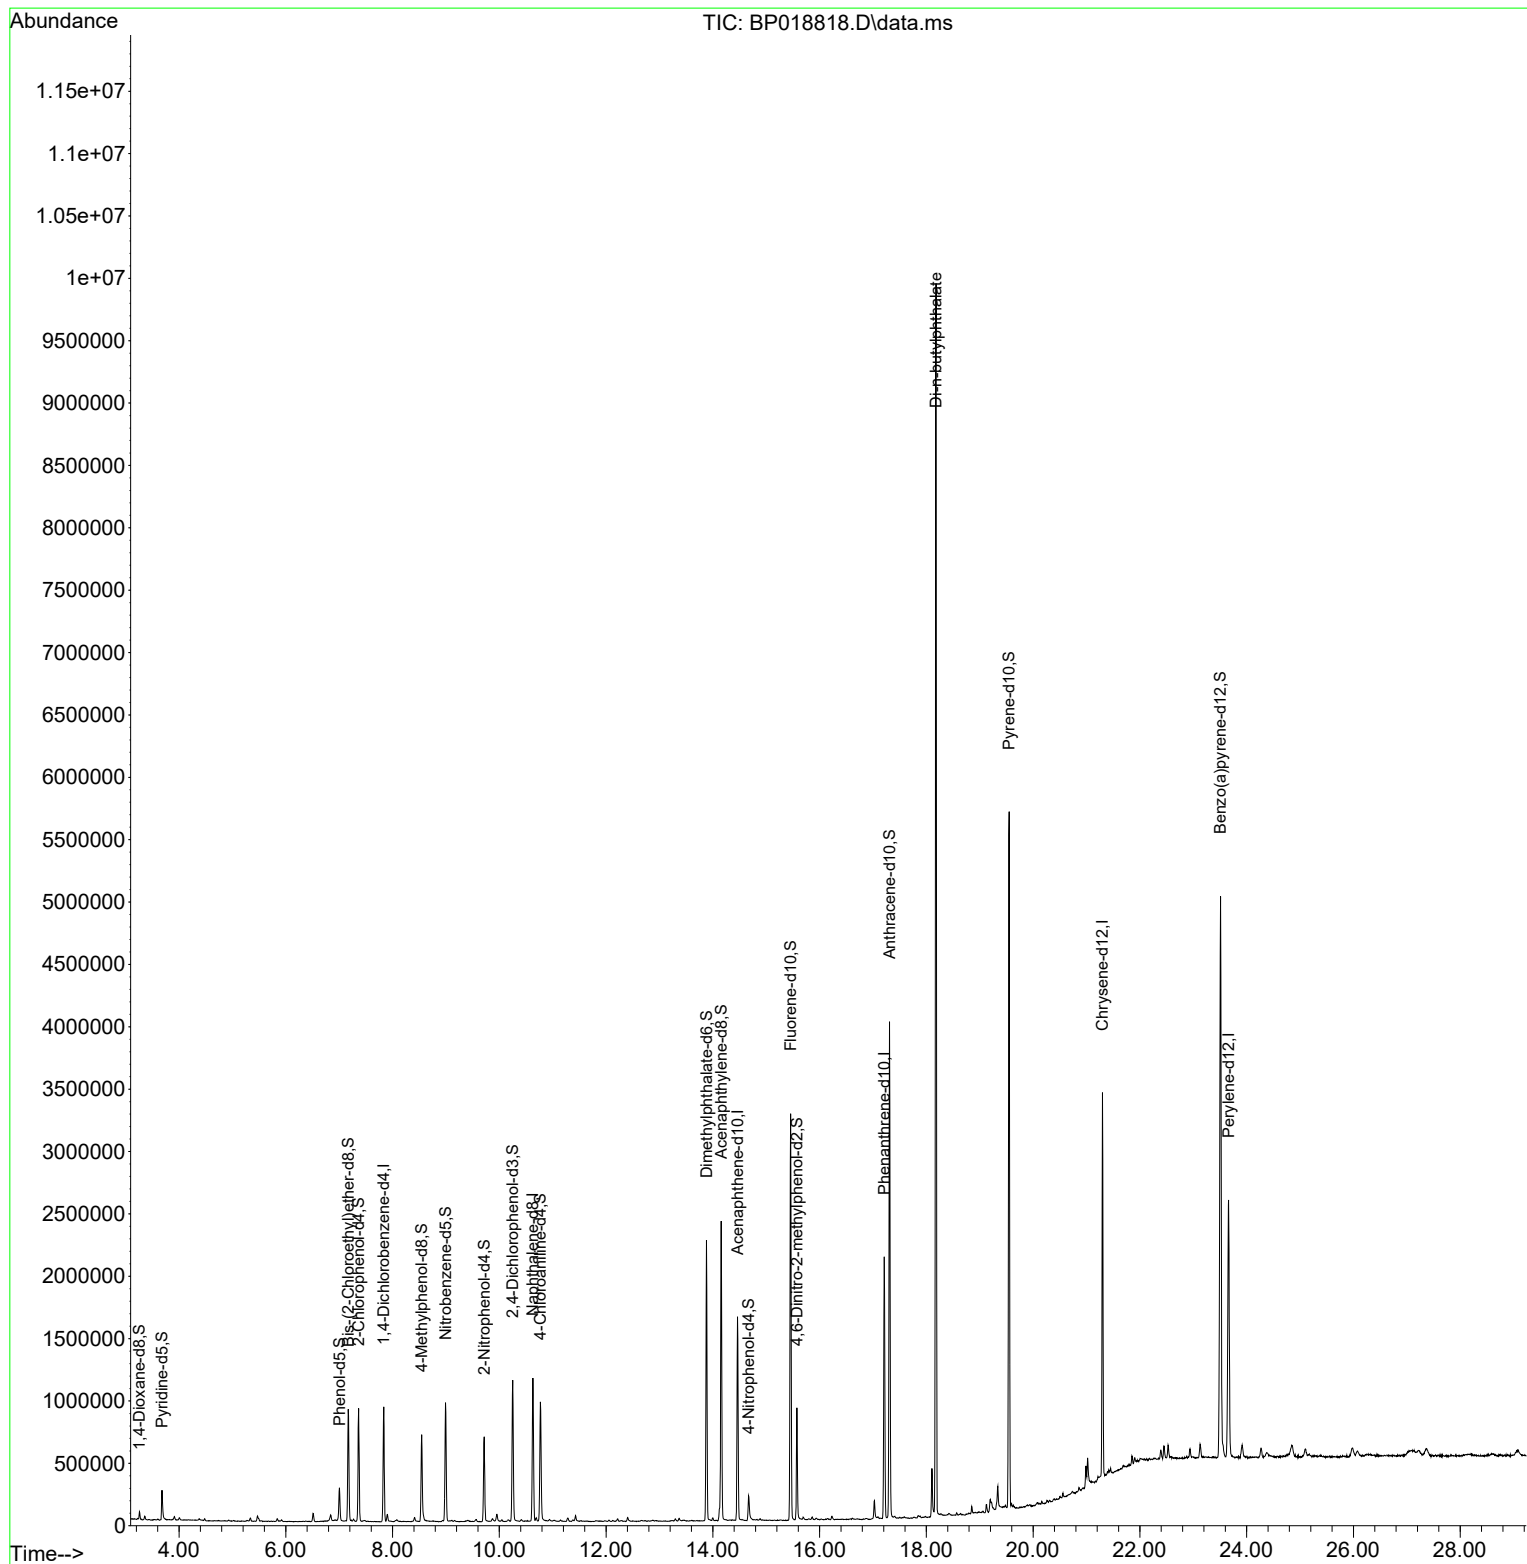

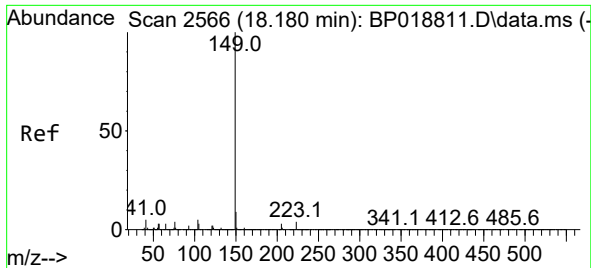

#78
 Di-n-butylphthalate
 Concen: 92.395 ng/ul
 RT: 18.181 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BP018818.D
 Acq: 13 Dec 2023 22:38

Instrument :
 BNA_P
 ClientSampleId :
 DCLD3

Tgt Ion:149 Resp: 7452831
 Ion Ratio Lower Upper
 149 100
 150 9.5 7.4 11.2
 104 5.0 3.9 5.9

