

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018837.D
 Acq On : 14 Dec 2023 11:02
 Operator : MA/JU
 Sample : 05646-17
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AS4

Quant Time: Dec 14 21:53:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 13 23:34:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.834	152	226010	20.000	ng/ul	0.00
20) Naphthalene-d8	10.628	136	795265	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.463	164	465505	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.210	188	1072890	20.000	ng/ul	0.00
79) Chrysene-d12	21.298	240	1243680	20.000	ng/ul	0.00
88) Perylene-d12	23.656	264	1483857	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	21662	3.266	ng/uL	0.00
4) Pyridine-d5	3.681	84	207515	11.681	ng/ul	0.00
7) Phenol-d5	7.004	99	327151	14.424	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.169	67	226531	16.852	ng/ul	0.00
11) 2-Chlorophenol-d4	7.363	132	300181	16.961	ng/ul	0.00
15) 4-Methylphenol-d8	8.545	113	271651	14.800	ng/ul	0.00
21) Nitrobenzene-d5	8.993	128	136260	19.251	ng/ul	0.00
24) 2-Nitrophenol-d4	9.716	143	144560	19.699	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.251	165	281114	18.734	ng/ul	0.00
31) 4-Chloroaniline-d4	10.769	131	370616	18.899	ng/ul	0.00
46) Dimethylphthalate-d6	13.881	166	812856	19.565	ng/ul	0.00
49) Acenaphthylene-d8	14.157	160	1003907	21.944	ng/ul	0.00
54) 4-Nitrophenol-d4	14.669	143	76742	11.253	ng/ul	0.00
60) Fluorene-d10	15.457	176	801474	22.982	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.575	200	76558	11.901	ng/ul	0.00
73) Anthracene-d10	17.310	188	1293797	22.938	ng/ul	0.00
81) Pyrene-d10	19.545	212	1729599	17.866	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.504	264	1985654	22.950	ng/ul	-0.01
Target Compounds						Qvalue
39) 1,2,4,5-Tetrachloroben...	12.651	216	158993	9.414	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.263	216	596943	32.178	ng/uL	99
76) Pentachlorobenzene	14.775	250	62485	3.429	ng/uL	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018837.D
Acq On : 14 Dec 2023 11:02
Operator : MA/JU
Sample : 05646-17
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AS4

Quant Time: Dec 14 21:53:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 13 23:34:47 2023
Response via : Initial Calibration




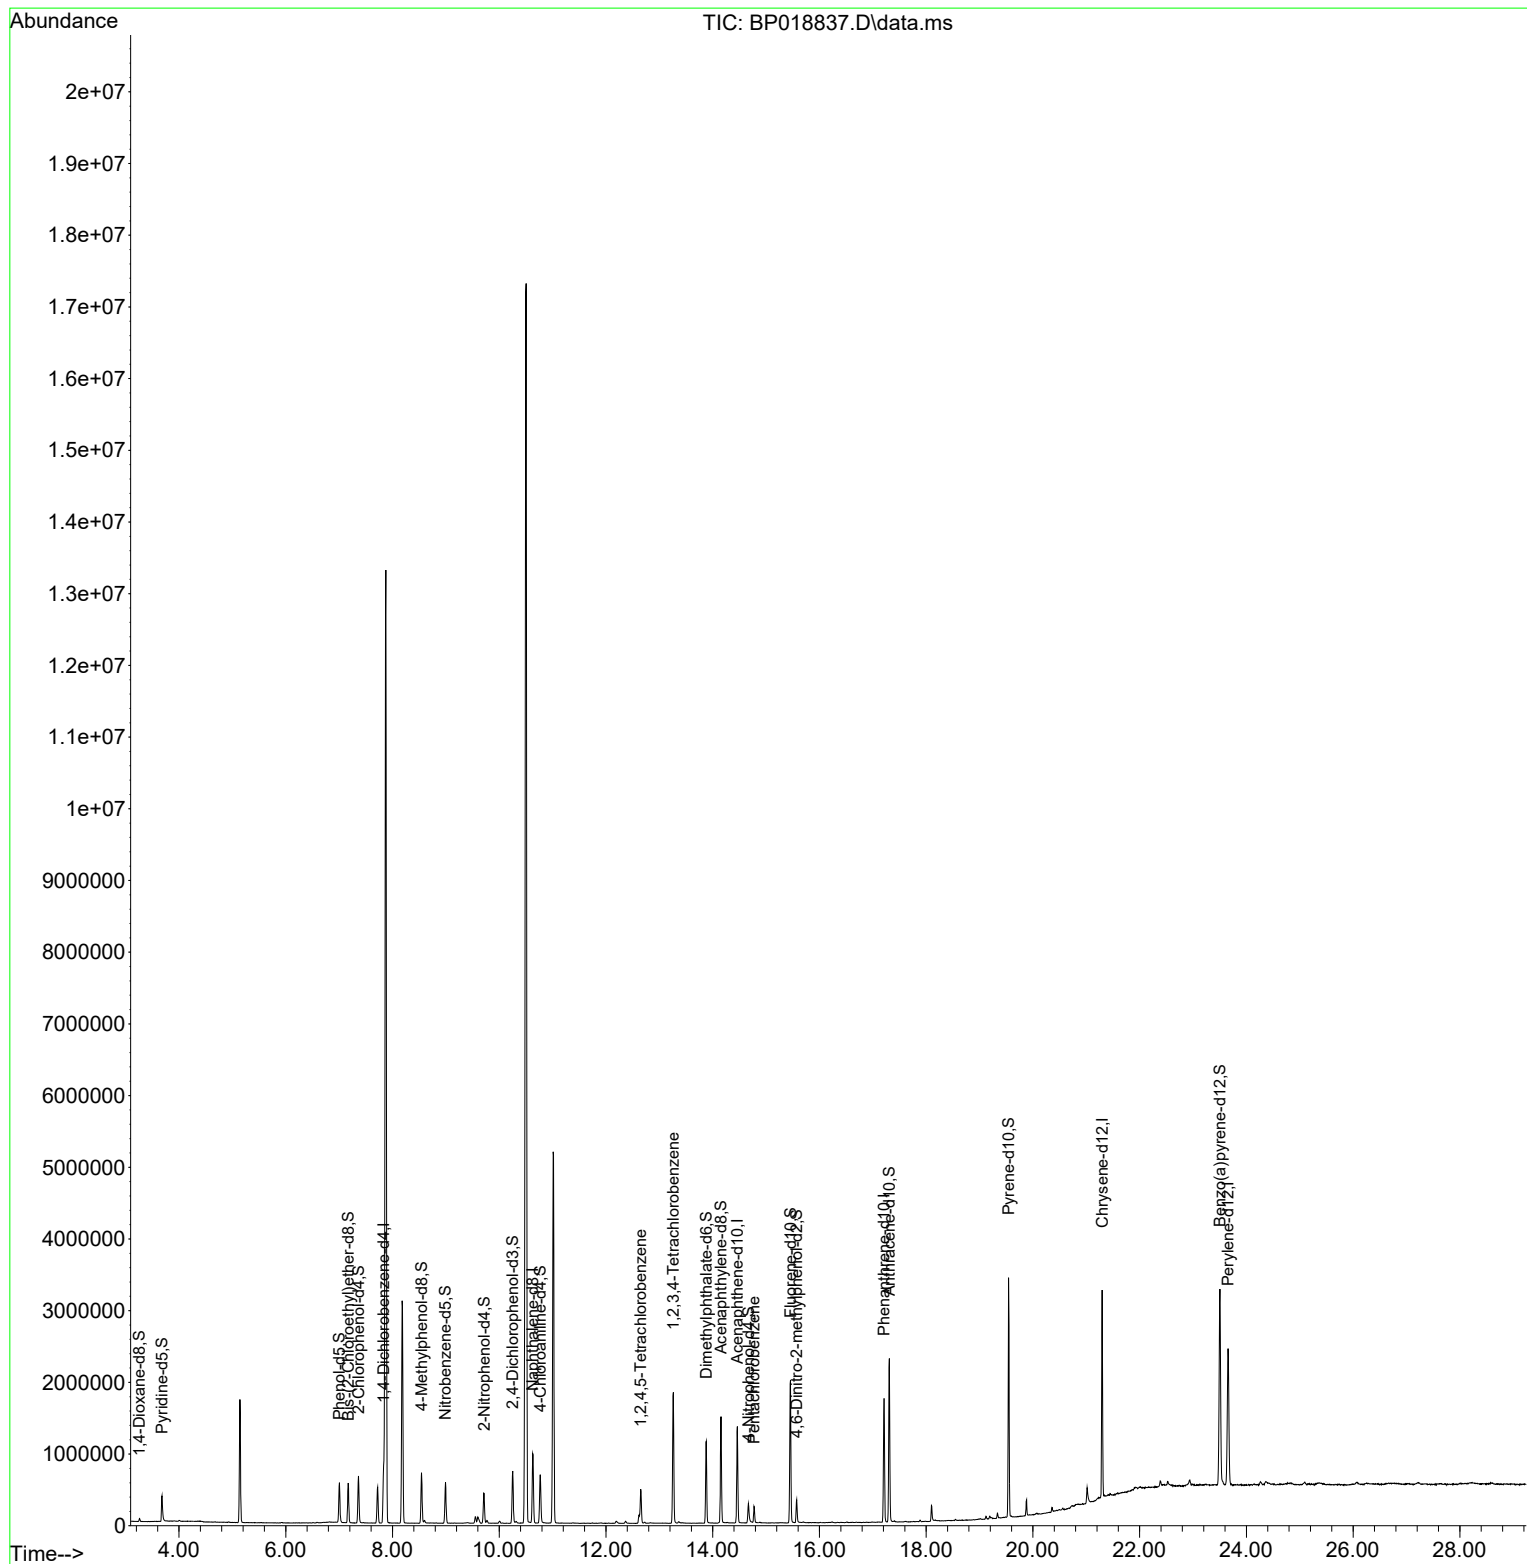


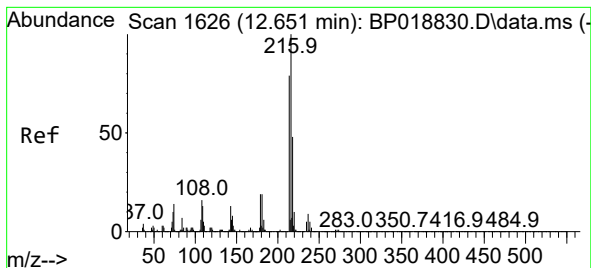

#39
1,2,4,5-Tetrachlorobenzene
Concen: 9.414 ng/ul
RT: 12.651 min Scan# 1626
Delta R.T. -0.006 min
Lab File: BP018837.D
Acq: 14 Dec 2023 11:02




Instrument :
BNA_P
ClientSampleId :
C0AS4


Tgt Ion:	216	Resp:	158993
Ion Ratio	Lower	Upper	
216	100		
214	80.6	63.9	95.9
179	20.3	16.3	24.5
108	14.9	12.6	19.0

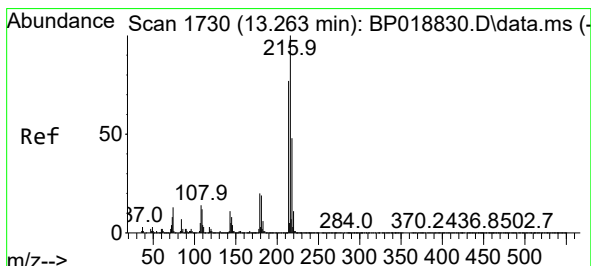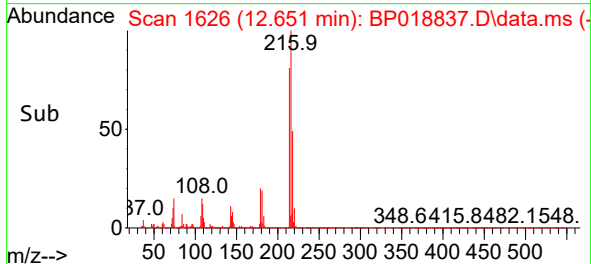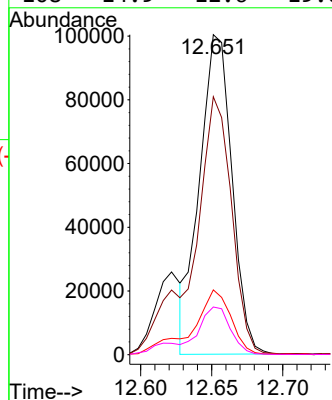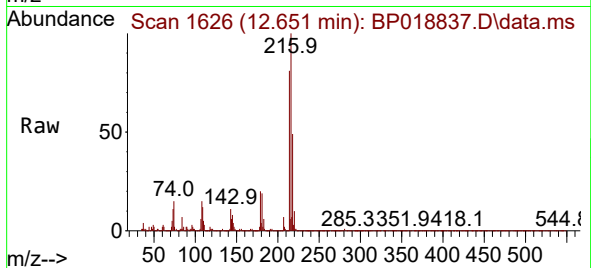

#75
1,2,3,4-Tetrachlorobenzene
Concen: 32.178 ng/ul
RT: 13.263 min Scan# 1730
Delta R.T. -0.000 min
Lab File: BP018837.D
Acq: 14 Dec 2023 11:02

Tgt Ion:	216	Resp:	596943
Ion Ratio	Lower	Upper	
216	100		
214	77.8	61.4	92.2
218	48.7	39.2	58.8

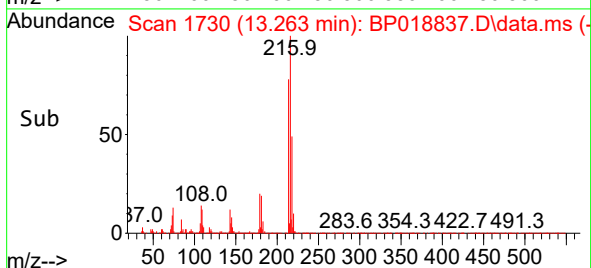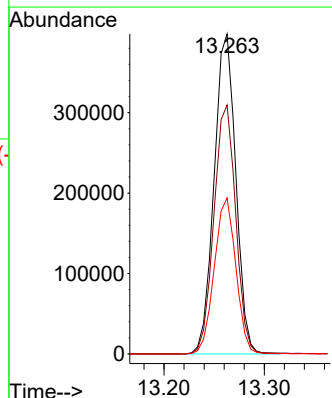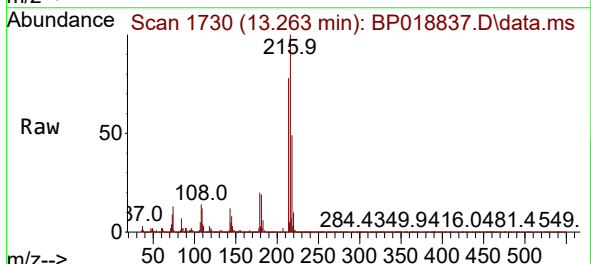

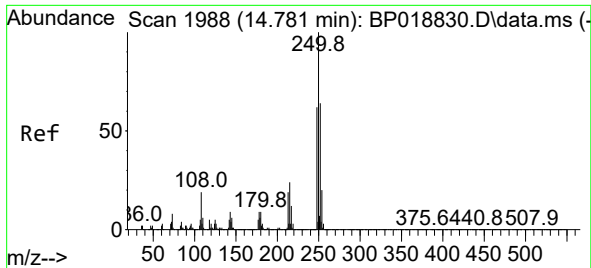

#76
 Pentachlorobenzene
 Concen: 3.429 ng/uL
 RT: 14.775 min Scan# 1987
 Delta R.T. -0.006 min
 Lab File: BP018837.D
 Acq: 14 Dec 2023 11:02

Instrument :
 BNA_P
 ClientSampleId :
 C0AS4

Tgt Ion:250 Resp: 62485
 Ion Ratio Lower Upper
 250 100
 248 59.6 50.6 75.8
 252 61.8 51.3 76.9

