

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018851.D
 Acq On : 14 Dec 2023 19:50
 Operator : MA/JU
 Sample : 05627-20DL 10X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLD2DL

Quant Time: Dec 14 21:56:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 13 23:34:47 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.834	152	191226	20.000	ng/ul	0.00
20) Naphthalene-d8	10.628	136	677579	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.463	164	385258	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.210	188	905520	20.000	ng/ul	0.00
79) Chrysene-d12	21.298	240	910615	20.000	ng/ul	0.00
88) Perylene-d12	23.657	264	1171103	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	4024	0.717	ng/uL	0.00
4) Pyridine-d5	3.693	84	16992	1.130	ng/ul	0.02
7) Phenol-d5	7.005	99	15498	0.808	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.169	67	40902	3.596	ng/ul	0.00
11) 2-Chlorophenol-d4	7.363	132	39065	2.609	ng/ul	0.00
15) 4-Methylphenol-d8	8.546	113	25645	1.651	ng/ul	0.00
21) Nitrobenzene-d5	8.993	128	20856	3.458	ng/ul	0.00
24) 2-Nitrophenol-d4	9.716	143	17956	2.872	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.252	165	37635	2.944	ng/ul	0.00
31) 4-Chloroaniline-d4	10.775	131	41932	2.510	ng/ul	0.00
46) Dimethylphthalate-d6	13.875	166	144836	4.212	ng/ul	0.00
49) Acenaphthylene-d8	14.151	160	145428	3.841	ng/ul	0.00
54) 4-Nitrophenol-d4	14.687	143	1479	0.262	ng/ul	0.02
60) Fluorene-d10	15.451	176	134466	4.659	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.575	200	10356	1.907	ng/ul	0.00
73) Anthracene-d10	17.304	188	228458	4.799	ng/ul	0.00
81) Pyrene-d10	19.545	212	304292	4.293	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.498	264	311007	4.555	ng/ul	-0.02
Target Compounds						
78) Di-n-butylphthalate	18.169	149	1424606	24.488	ng/ul	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018851.D
Acq On : 14 Dec 2023 19:50
Operator : MA/JU
Sample : 05627-20DL 10X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLD2DL

Quant Time: Dec 14 21:56:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 13 23:34:47 2023
Response via : Initial Calibration

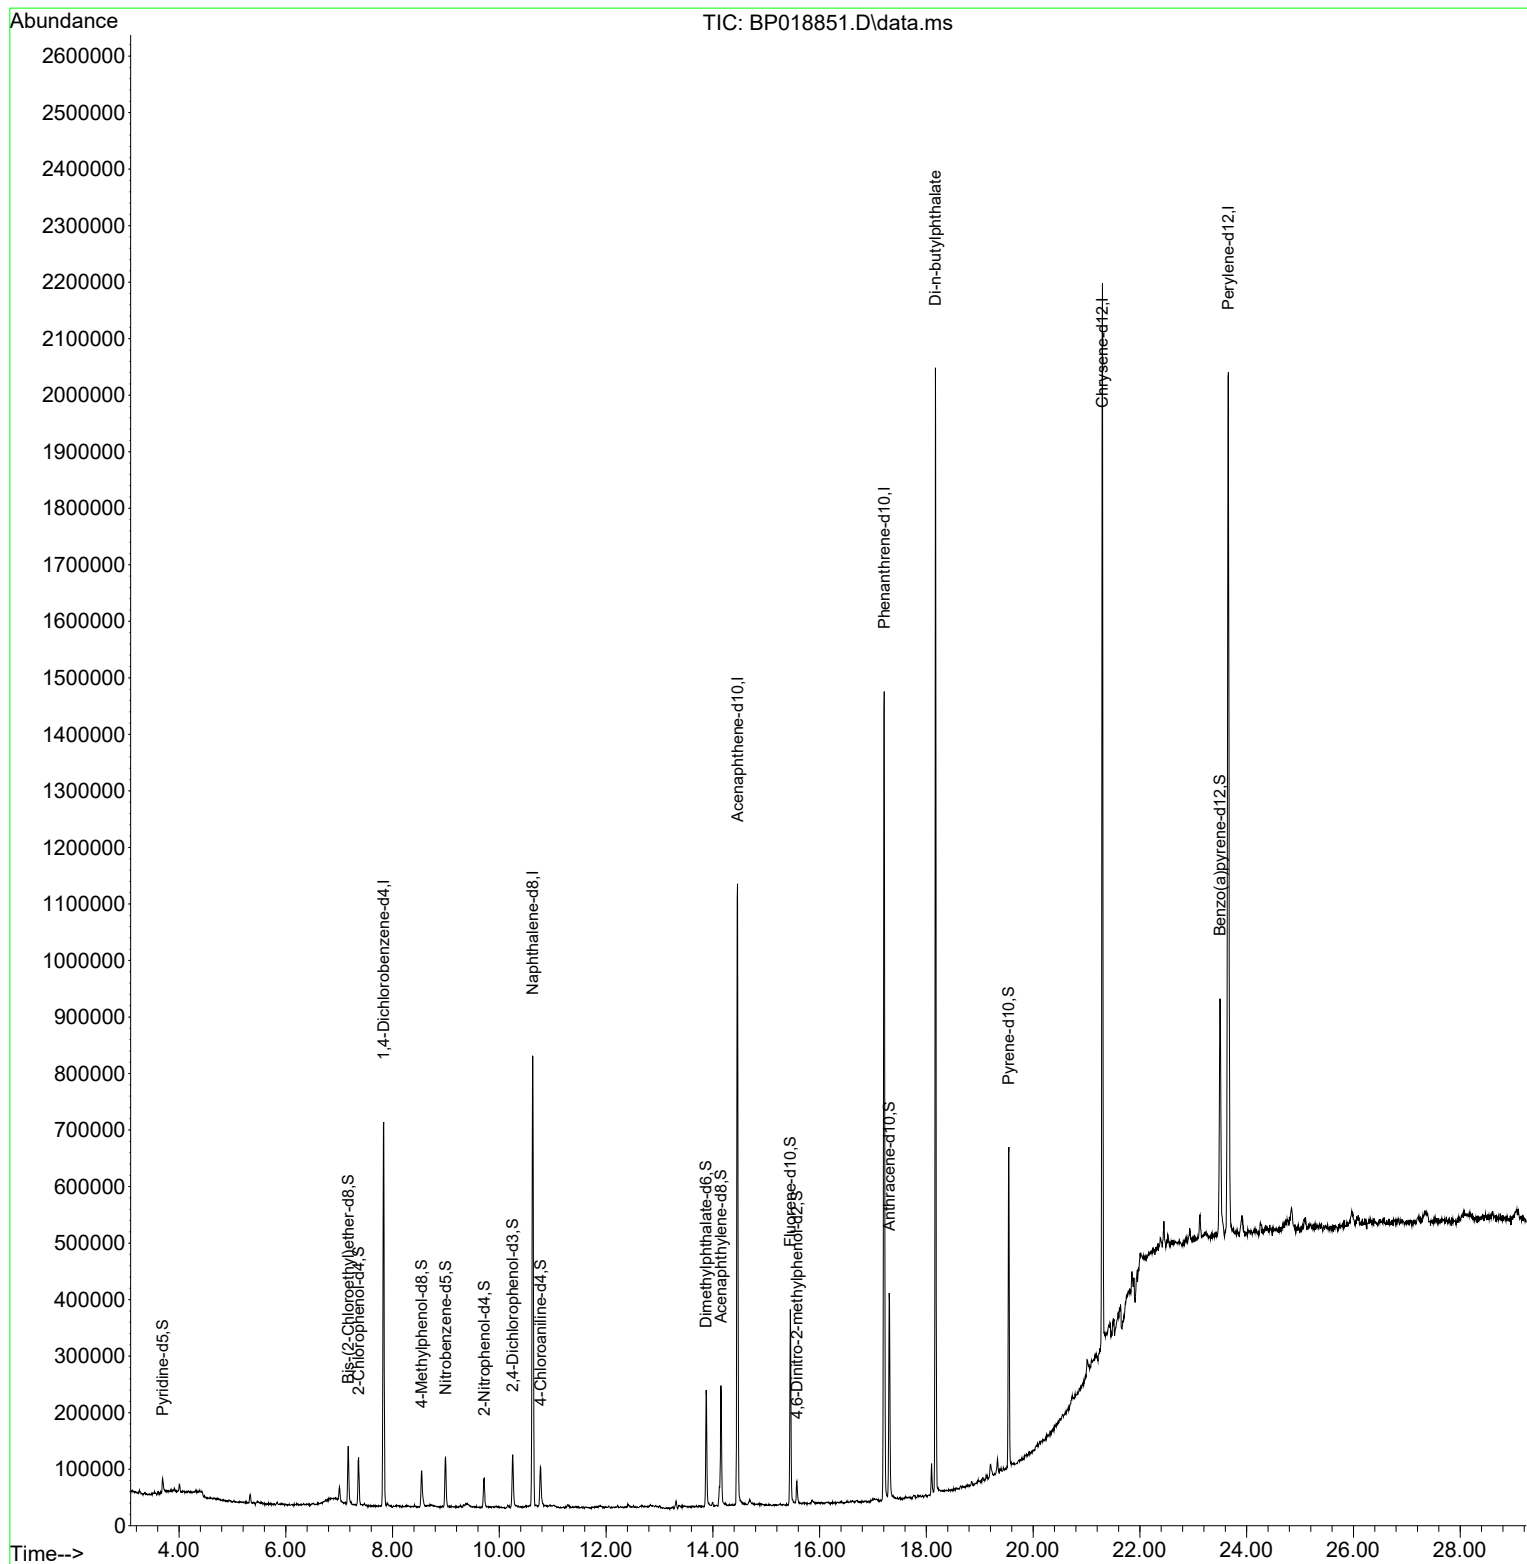

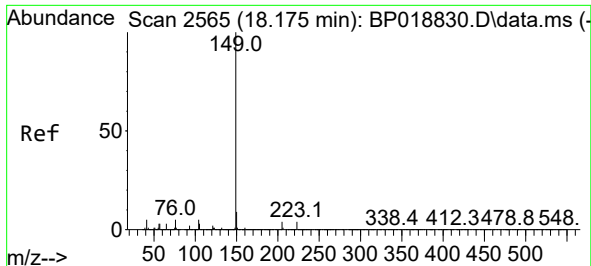

#78
 Di-n-butylphthalate
 Concen: 24.488 ng/ul
 RT: 18.169 min Scan# 21
 Delta R.T. -0.012 min
 Lab File: BP018851.D
 Acq: 14 Dec 2023 19:50

Instrument :
 BNA_P
 ClientSampleId :
 DCLD2DL

Tgt Ion:149 Resp: 1424606
 Ion Ratio Lower Upper
 149 100
 150 9.1 7.4 11.2
 104 5.0 3.9 5.9

