

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018852.D
 Acq On : 14 Dec 2023 20:24
 Operator : MA/JU
 Sample : 05627-18DL 10X
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLD0DL

Quant Time: Dec 14 21:56:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 13 23:34:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.834	152	250992	20.000	ng/ul	0.00
20) Naphthalene-d8	10.628	136	883352	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.457	164	441544	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.210	188	1085743	20.000	ng/ul	0.00
79) Chrysene-d12	21.298	240	1246256	20.000	ng/ul	0.00
88) Perylene-d12	23.657	264	1494832	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	5838	0.793	ng/uL	0.00
4) Pyridine-d5	3.693	84	18158	0.920	ng/ul	0.02
7) Phenol-d5	7.005	99	16854	0.669	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.169	67	54985	3.683	ng/ul	0.00
11) 2-Chlorophenol-d4	7.363	132	49096	2.498	ng/ul	0.00
15) 4-Methylphenol-d8	8.546	113	26836	1.317	ng/ul	0.00
21) Nitrobenzene-d5	8.993	128	26218	3.335	ng/ul	0.00
24) 2-Nitrophenol-d4	9.710	143	22472	2.757	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.251	165	49054	2.943	ng/ul	0.00
31) 4-Chloroaniline-d4	10.769	131	60064	2.757	ng/ul	0.00
46) Dimethylphthalate-d6	13.875	166	180256	4.574	ng/ul	0.00
49) Acenaphthylene-d8	14.151	160	183244	4.223	ng/ul	0.00
54) 4-Nitrophenol-d4	14.681	143	2648	0.409	ng/ul	0.01
60) Fluorene-d10	15.451	176	170577	5.157	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.569	200	12039	1.849	ng/ul	-0.01
73) Anthracene-d10	17.304	188	277091	4.854	ng/ul	0.00
81) Pyrene-d10	19.545	212	379551	3.912	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.504	264	405819	4.656	ng/ul	-0.01
Target Compounds						
78) Di-n-butylphthalate	18.175	149	3286721	47.118	ng/ul	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018852.D
Acq On : 14 Dec 2023 20:24
Operator : MA/JU
Sample : 05627-18DL 10X
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLD0DL

Quant Time: Dec 14 21:56:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 13 23:34:47 2023
Response via : Initial Calibration

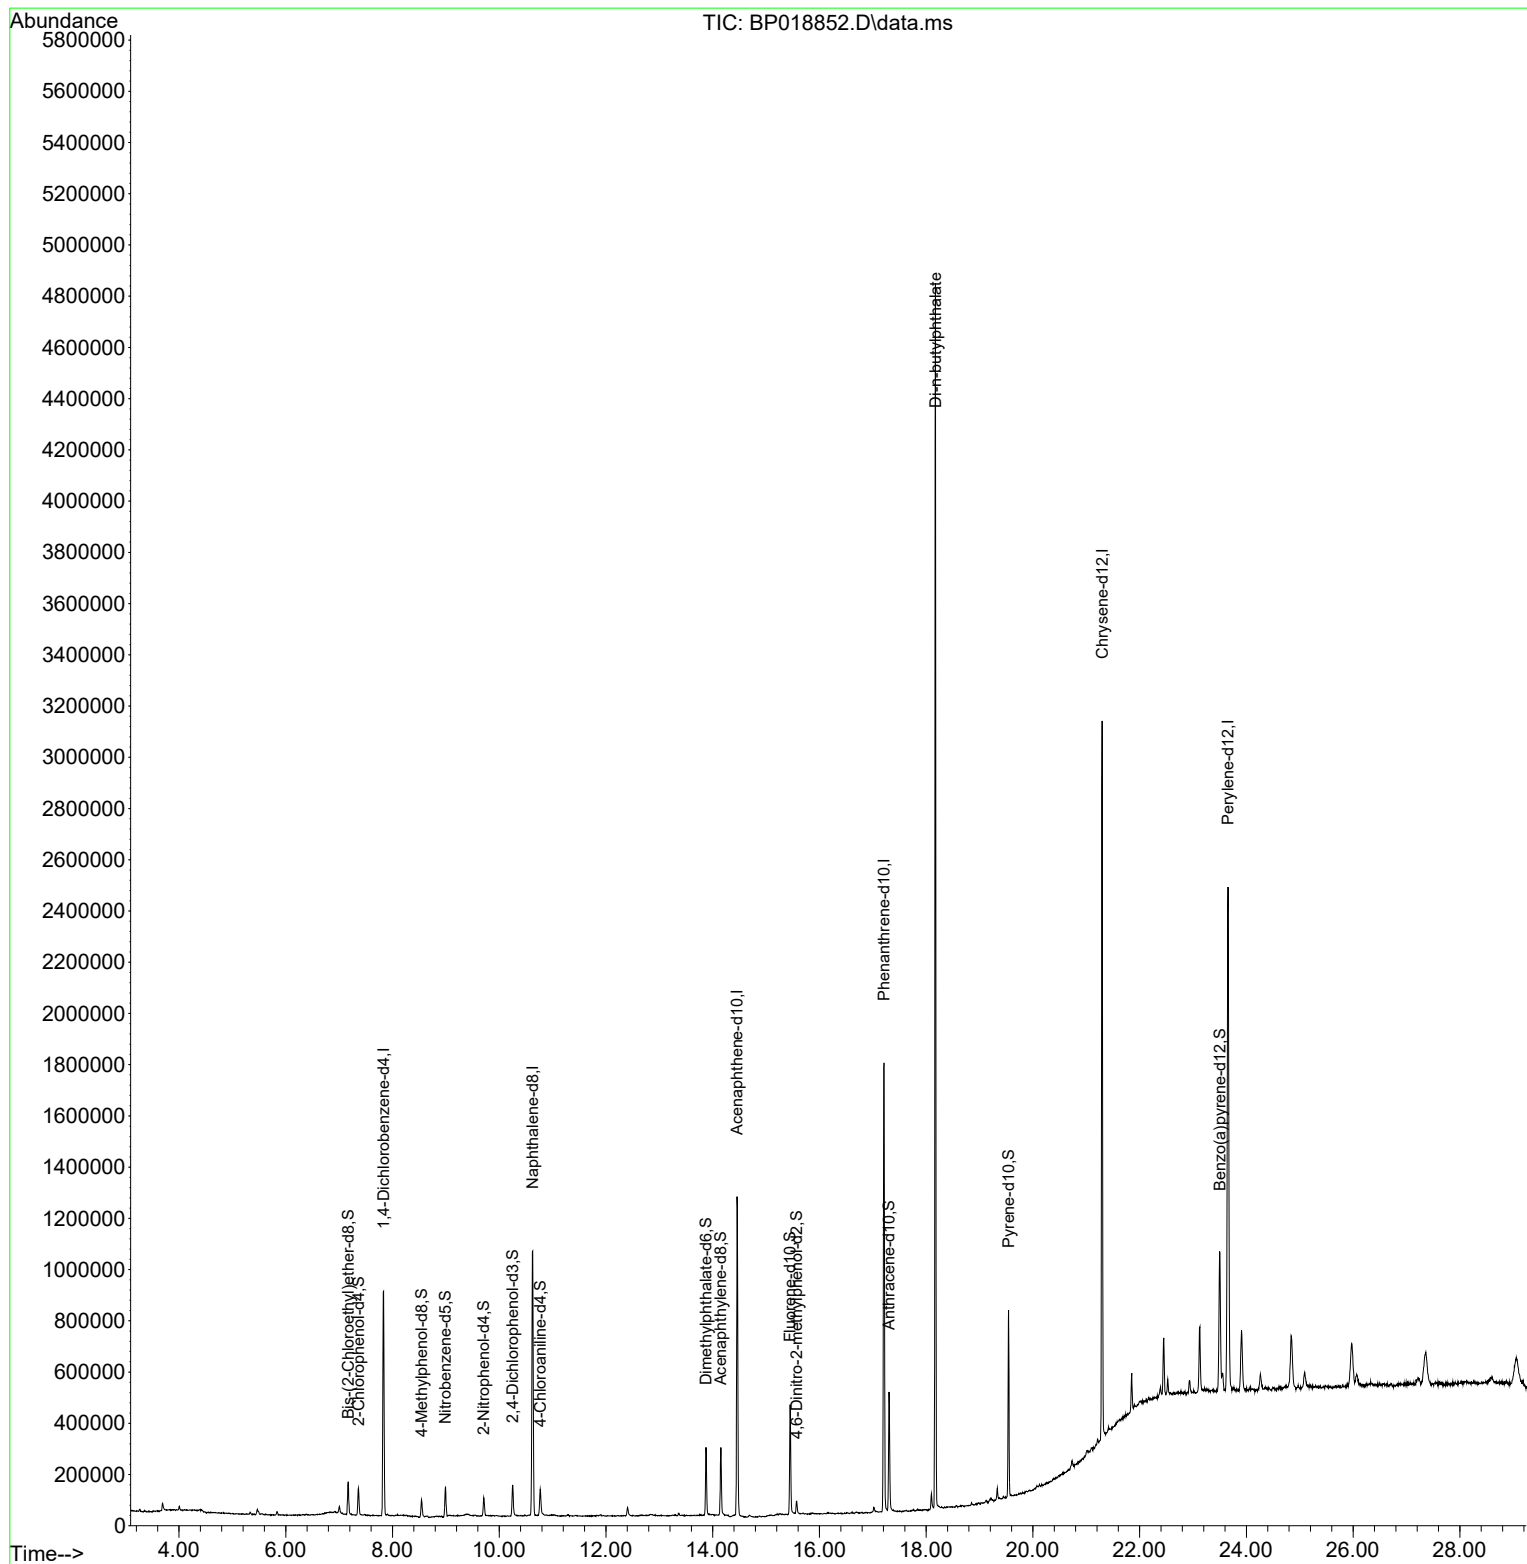

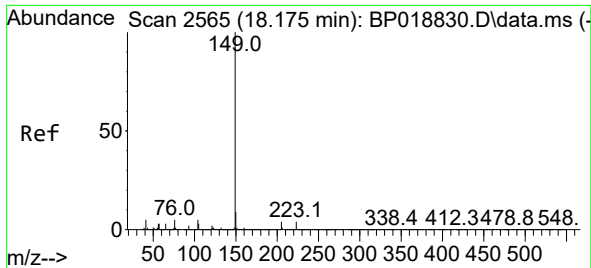

#78
 Di-n-butylphthalate
 Concen: 47.118 ng/ul
 RT: 18.175 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP018852.D
 Acq: 14 Dec 2023 20:24

Instrument :
 BNA_P
 ClientSampleId :
 DCLD0DL

Tgt Ion:149 Resp: 3286721
 Ion Ratio Lower Upper
 149 100
 150 9.2 7.4 11.2
 104 4.9 3.9 5.9

