




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018870.D
 Acq On : 15 Dec 2023 07:08
 Operator : MA/JU
 Sample : 05627-16
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLC8

Manual IntegrationsAPPROVED

Quant Time: Dec 15 07:35:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 13 23:34:47 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/16/2023
 Supervised By :mohammad ahmed 12/16/2023

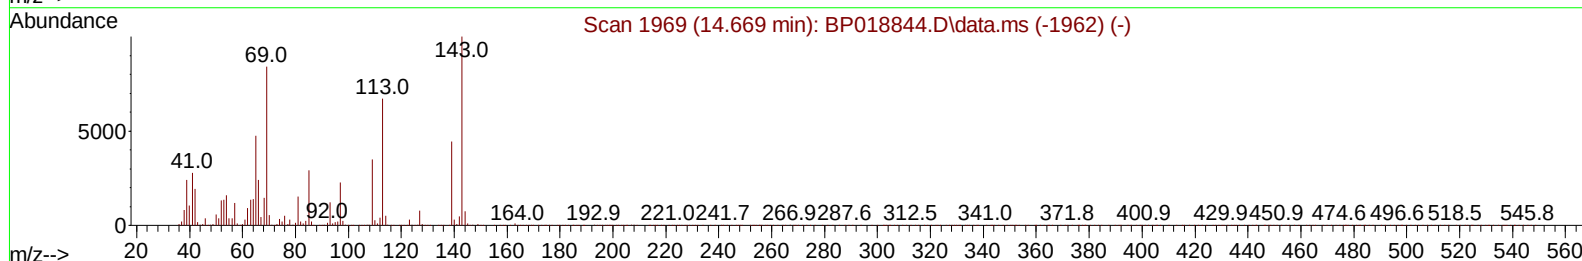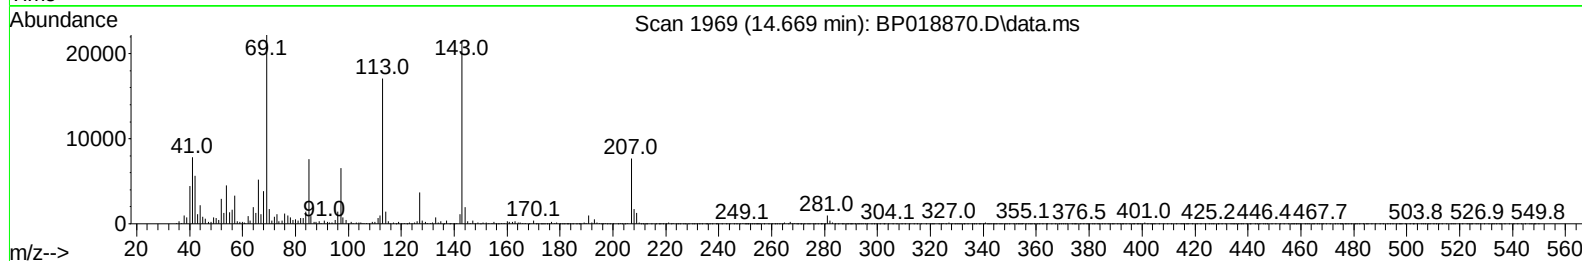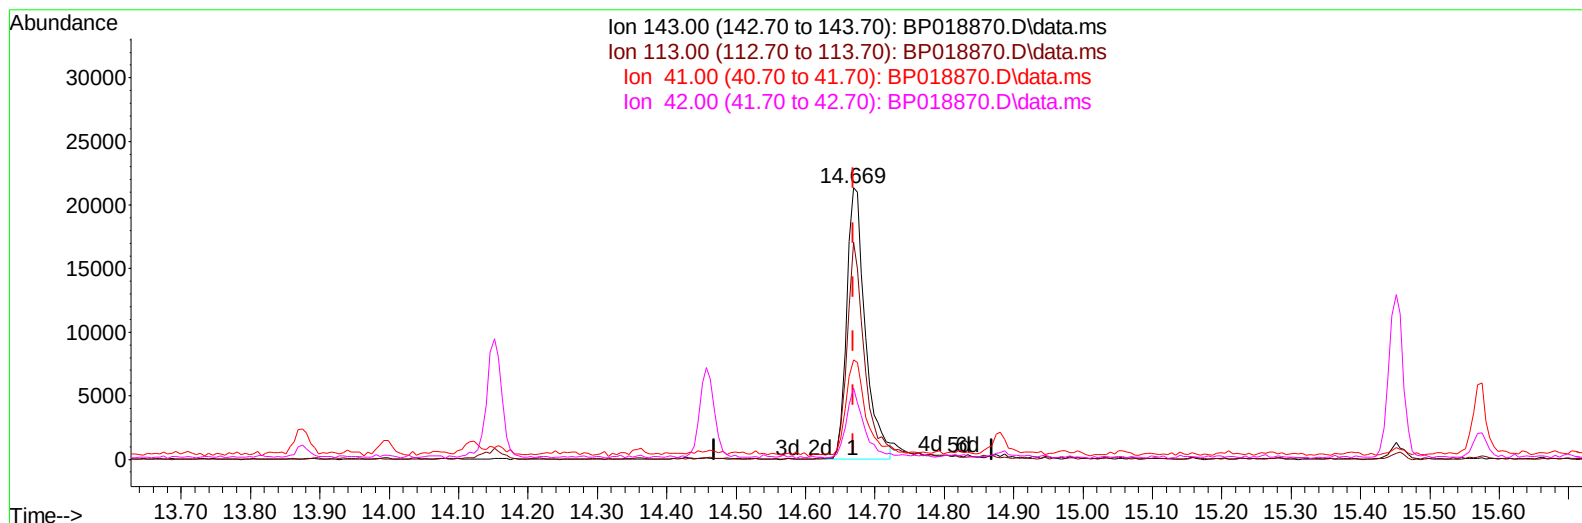

TIC: BP018870.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.669min (-0.000) 6.53 ng/u1

response 39823

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	70.80	80.02
41.00	34.60	36.56
42.00	23.00	26.36




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018870.D
 Acq On : 15 Dec 2023 07:08
 Operator : MA/JU
 Sample : 05627-16
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLC8

Manual IntegrationsAPPROVED

Quant Time: Dec 15 07:35:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 13 23:34:47 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/16/2023
 Supervised By :mohammad ahmed 12/16/2023

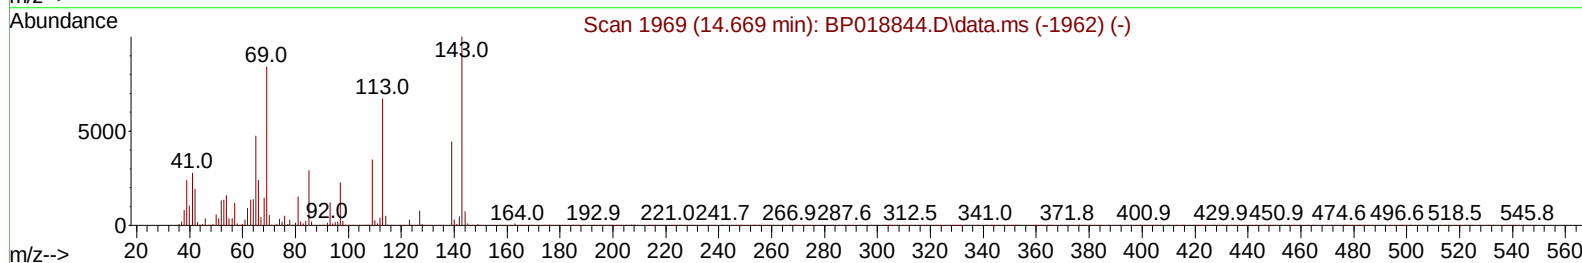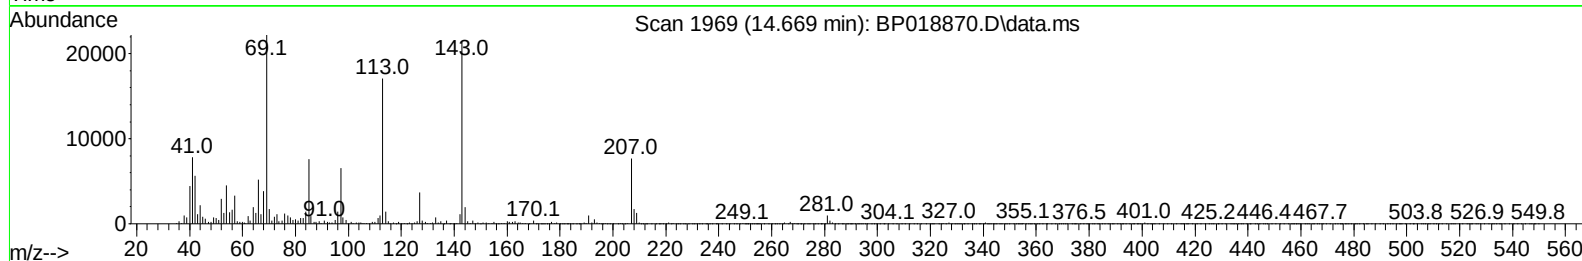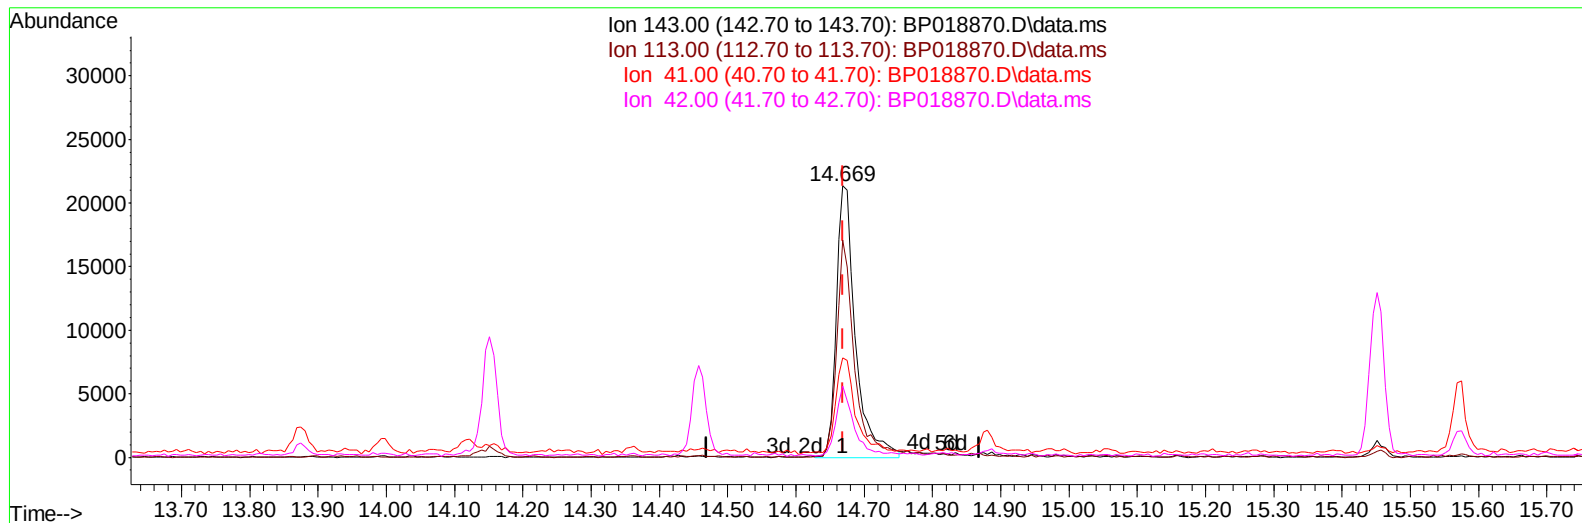

TIC: BP018870.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.669min (-0.000) 6.79 ng/ul m

response 41396

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	70.80	80.02
41.00	34.60	36.56
42.00	23.00	26.36

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018870.D
 Acq On : 15 Dec 2023 07:08
 Operator : MA/JU
 Sample : 05627-16
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLC8

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/16/2023
 Supervised By :mohammad ahmed 12/16/2023

Quant Time: Dec 15 07:36:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 13 23:34:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.828	152	215023	20.000	ng/ul	0.00
20) Naphthalene-d8	10.622	136	757381	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.457	164	416023	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.210	188	887131	20.000	ng/ul	0.00
79) Chrysene-d12	21.298	240	1004846	20.000	ng/ul	0.00
88) Perylene-d12	23.657	264	1210570	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	27509	4.360	ng/uL	0.00
4) Pyridine-d5	3.681	84	103532	6.126	ng/ul	0.00
7) Phenol-d5	6.999	99	143710	6.660	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.169	67	369759	28.912	ng/ul	0.00
11) 2-Chlorophenol-d4	7.363	132	364910	21.672	ng/ul	0.00
15) 4-Methylphenol-d8	8.540	113	218316	12.502	ng/ul	0.00
21) Nitrobenzene-d5	8.993	128	219635	32.582	ng/ul	0.00
24) 2-Nitrophenol-d4	9.710	143	201931	28.894	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.246	165	379018	26.522	ng/ul	0.00
31) 4-Chloroaniline-d4	10.763	131	389238	20.841	ng/ul	0.00
46) Dimethylphthalate-d6	13.875	166	1314433	35.400	ng/ul	0.00
49) Acenaphthylene-d8	14.151	160	1436545	35.136	ng/ul	0.00
54) 4-Nitrophenol-d4	14.669	143	41396m	6.792	ng/ul	0.00
60) Fluorene-d10	15.451	176	973571	31.237	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.575	200	127364	23.944	ng/ul	0.00
73) Anthracene-d10	17.310	188	1938180	41.558	ng/ul	0.00
81) Pyrene-d10	19.545	212	2497395	31.928	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.504	264	2910356	41.232	ng/ul	-0.01
Target Compounds						
78) Di-n-butylphthalate	18.175	149	9839027	172.631	ng/ul	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018870.D
Acq On : 15 Dec 2023 07:08
Operator : MA/JU
Sample : 05627-16
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLC8

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/16/2023
Supervised By :mohammad ahmed 12/16/2023

Quant Time: Dec 15 07:36:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 13 23:34:47 2023
Response via : Initial Calibration

