

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018822.D
 Acq On : 14 Dec 2023 00:53
 Operator : MA/JU
 Sample : 05675-22
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AD3

Quant Time: Dec 14 02:09:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 13 23:34:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.834	152	277373	20.000	ng/u1	0.00
20) Naphthalene-d8	10.628	136	1021517	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.463	164	593700	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.210	188	1269948	20.000	ng/u1	0.00
79) Chrysene-d12	21.298	240	1359259	20.000	ng/u1	0.00
88) Perylene-d12	23.657	264	1636019	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	30139	3.703	ng/uL	0.00
4) Pyridine-d5	3.681	84	202328	9.280	ng/u1	0.00
7) Phenol-d5	7.005	99	144267	5.183	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.169	67	453811	27.507	ng/u1	0.00
11) 2-Chlorophenol-d4	7.363	132	455145	20.955	ng/u1	0.00
15) 4-Methylphenol-d8	8.546	113	266075	11.812	ng/u1	0.00
21) Nitrobenzene-d5	8.993	128	273002	30.027	ng/u1	0.00
24) 2-Nitrophenol-d4	9.716	143	276252	29.307	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.252	165	497913	25.833	ng/u1	0.00
31) 4-Chloroaniline-d4	10.769	131	631576	25.073	ng/u1	0.00
46) Dimethylphthalate-d6	13.881	166	1573538	29.696	ng/u1	0.00
49) Acenaphthylene-d8	14.157	160	1773749	30.400	ng/u1	0.00
54) 4-Nitrophenol-d4	14.669	143	34170	3.929	ng/u1	0.00
60) Fluorene-d10	15.457	176	1375999	30.936	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.575	200	179314	23.549	ng/u1	0.00
73) Anthracene-d10	17.310	188	2178403	32.629	ng/u1	0.00
81) Pyrene-d10	19.545	212	2689993	25.423	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.504	264	3117509	32.681	ng/u1	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.293	88	22545	2.526	ng/uL	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018822.D
Acq On : 14 Dec 2023 00:53
Operator : MA/JU
Sample : 05675-22
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AD3

Quant Time: Dec 14 02:09:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 13 23:34:47 2023
Response via : Initial Calibration

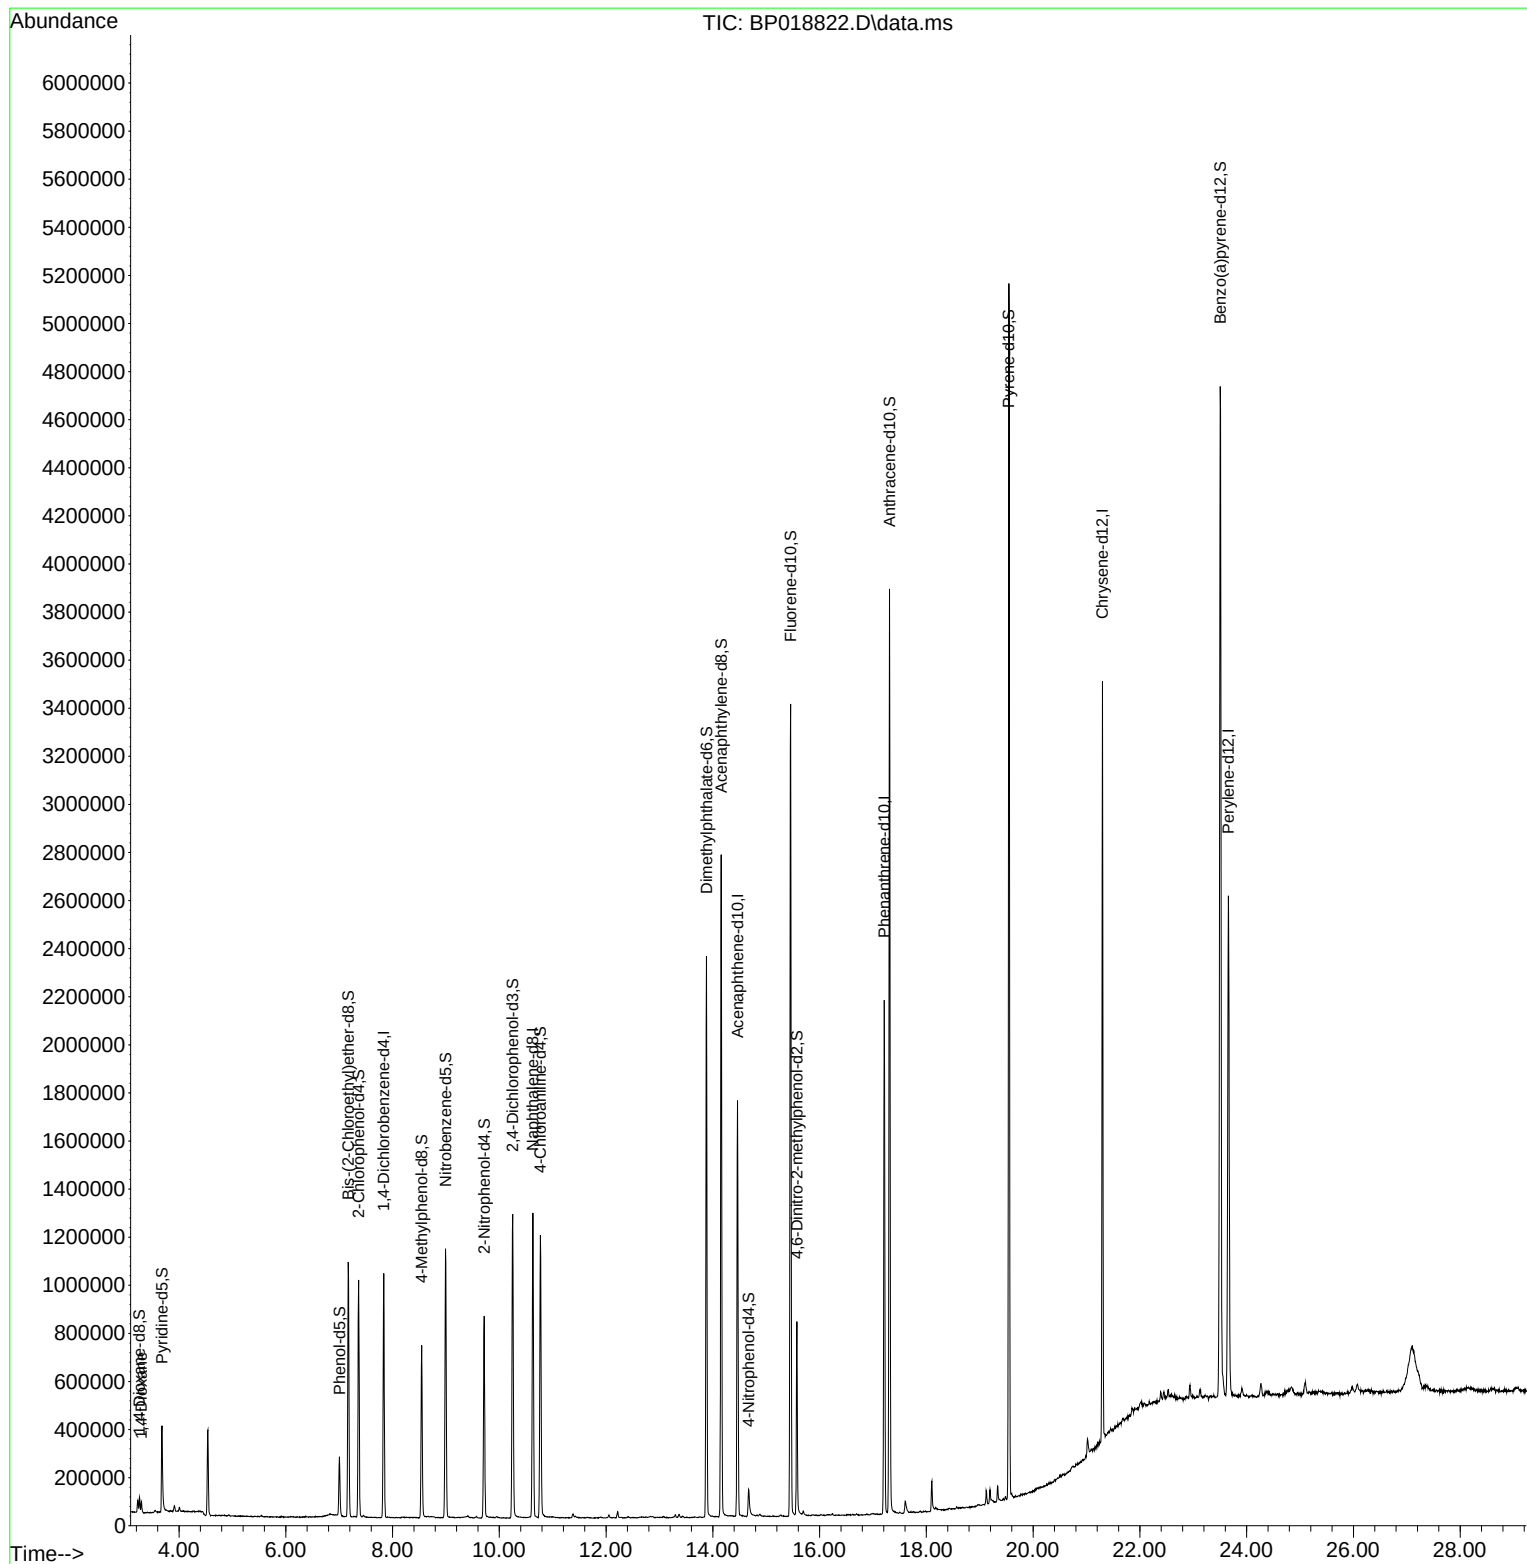

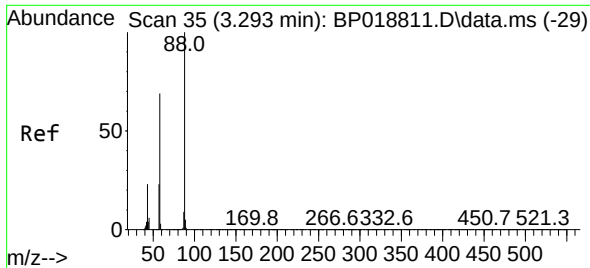

#2
 1,4-Dioxane
 Concen: 2.526 ng/uL
 RT: 3.293 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: BP018822.D
 Acq: 14 Dec 2023 00:53

Instrument :
 BNA_P
 ClientSampleId :
 H0AD3

Tgt Ion: 88 Resp: 22545
 Ion Ratio Lower Upper
 88 100
 43 23.6 21.8 32.6
 58 63.0 56.5 84.7

