

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018824.D
 Acq On : 14 Dec 2023 02:01
 Operator : MA/JU
 Sample : 05677-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AC7

Quant Time: Dec 14 02:29:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 13 23:34:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.834	152	289018	20.000	ng/ul	0.00
20) Naphthalene-d8	10.628	136	1039743	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.463	164	607228	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.210	188	1382777	20.000	ng/ul	0.00
79) Chrysene-d12	21.298	240	1569937	20.000	ng/ul	0.00
88) Perylene-d12	23.657	264	1862663	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	35231	4.154	ng/uL	0.00
4) Pyridine-d5	3.681	84	170526	7.506	ng/ul	0.00
7) Phenol-d5	7.005	99	161016	5.552	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.169	67	372022	21.641	ng/ul	0.00
11) 2-Chlorophenol-d4	7.364	132	400662	17.704	ng/ul	0.00
15) 4-Methylphenol-d8	8.546	113	248244	10.576	ng/ul	0.00
21) Nitrobenzene-d5	8.993	128	221808	23.969	ng/ul	0.00
24) 2-Nitrophenol-d4	9.716	143	221300	23.066	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.252	165	430108	21.924	ng/ul	0.00
31) 4-Chloroaniline-d4	10.769	131	398454	15.541	ng/ul	0.00
46) Dimethylphthalate-d6	13.881	166	1450434	26.763	ng/ul	0.00
49) Acenaphthylene-d8	14.157	160	1619415	27.136	ng/ul	0.00
54) 4-Nitrophenol-d4	14.669	143	55835	6.276	ng/ul	0.00
60) Fluorene-d10	15.457	176	1265391	27.816	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.575	200	180909	21.819	ng/ul	0.00
73) Anthracene-d10	17.310	188	2139715	29.434	ng/ul	0.00
81) Pyrene-d10	19.545	212	2770854	22.673	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.504	264	3145758	28.965	ng/ul	-0.01
Target Compounds						
					Qvalue	
72) Phenanthrene	17.251	178	148572	1.779	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018824.D
Acq On : 14 Dec 2023 02:01
Operator : MA/JU
Sample : 05677-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC7

Quant Time: Dec 14 02:29:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 13 23:34:47 2023
Response via : Initial Calibration

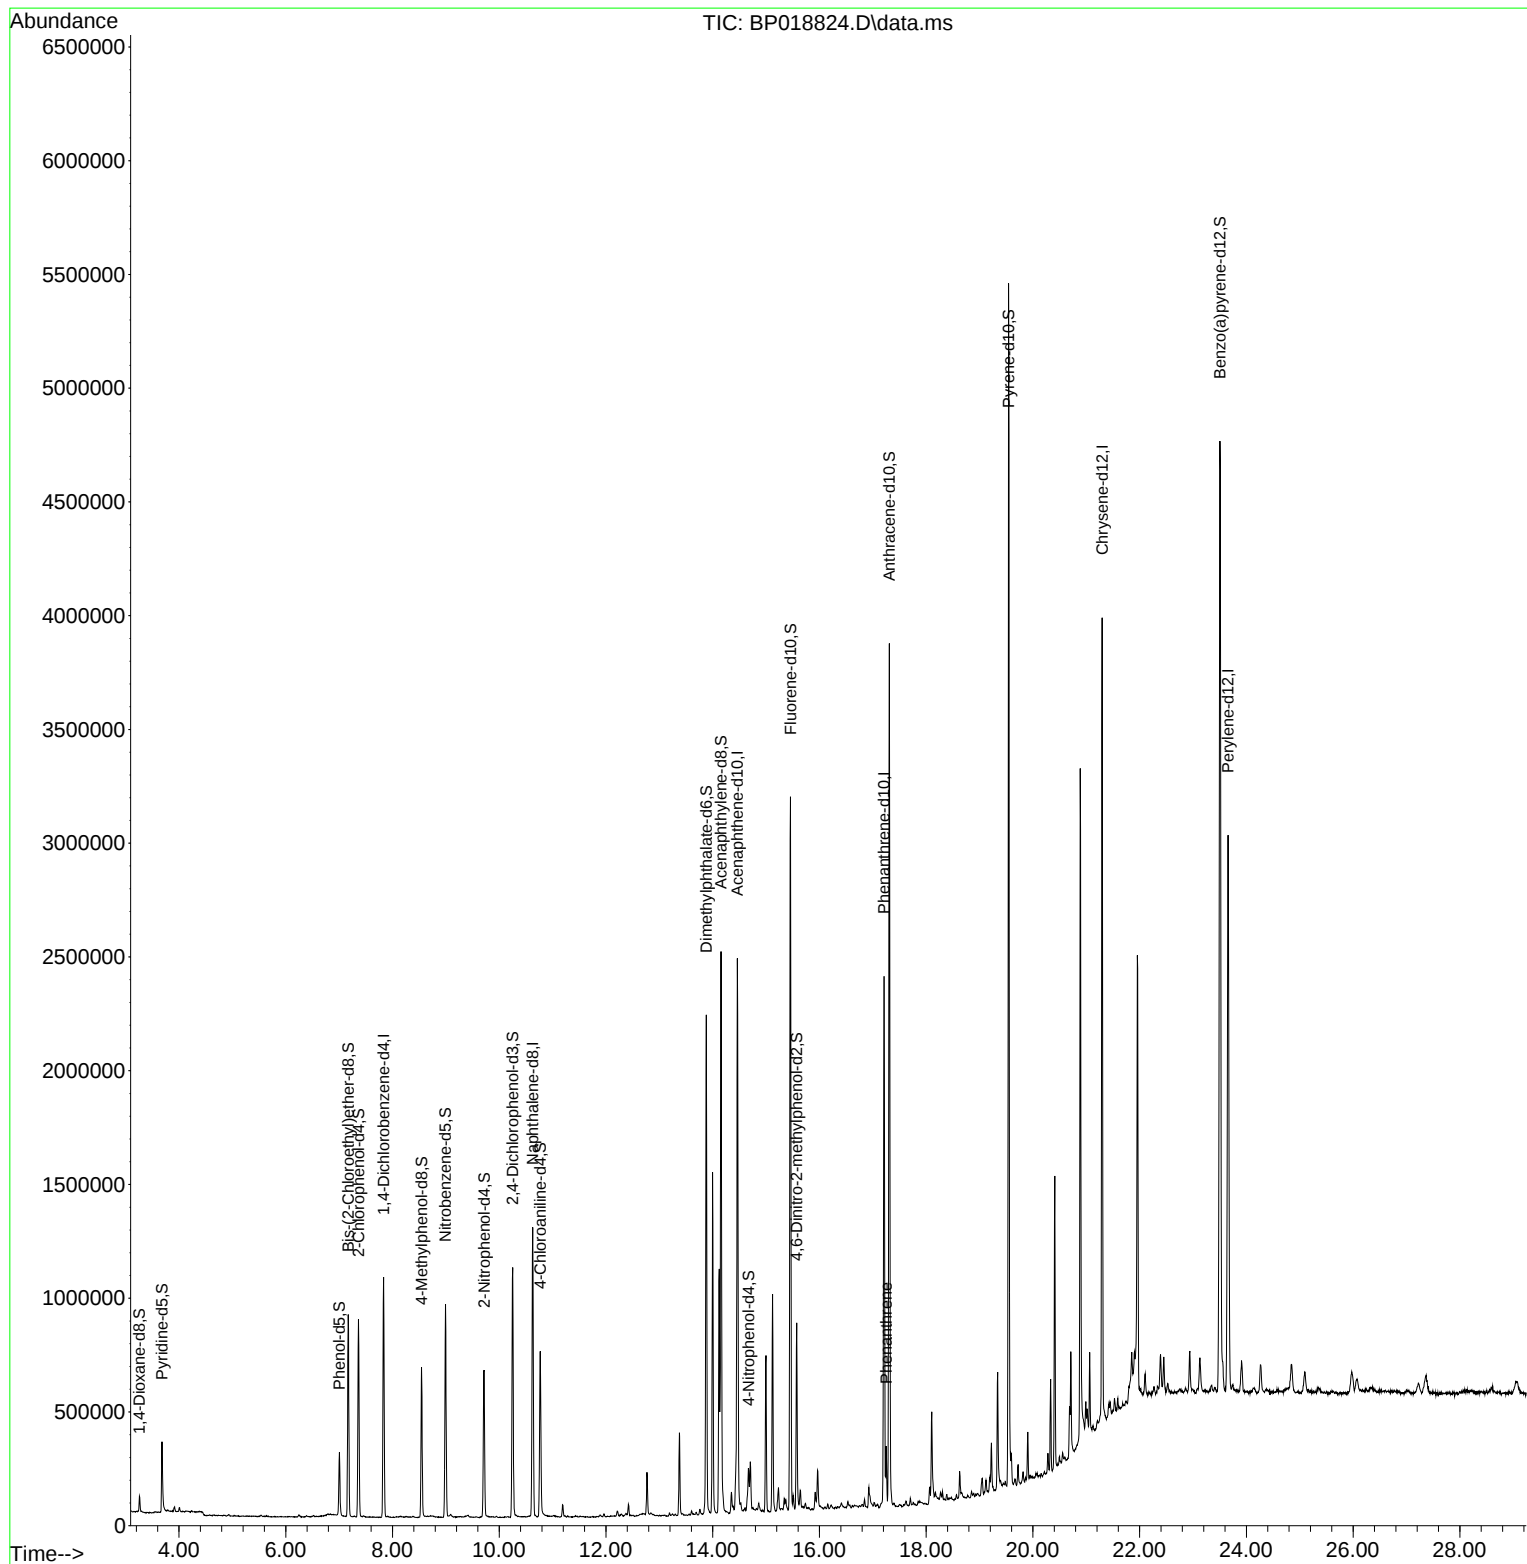

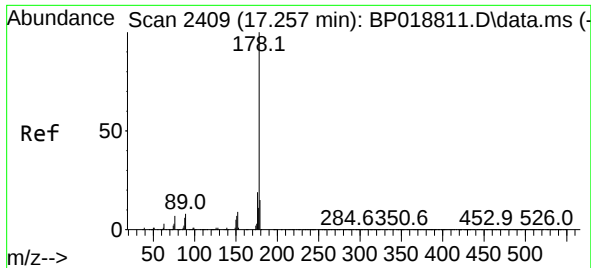

#72
 Phenanthrene
 Concen: 1.779 ng/ul
 RT: 17.251 min Scan# 2408
 Delta R.T. -0.006 min
 Lab File: BP018824.D
 Acq: 14 Dec 2023 02:01

Instrument :
 BNA_P
 ClientSampleId :
 H0AC7

Tgt Ion:	178	Resp:	148572
Ion	Ratio	Lower	Upper
178	100		
179	16.2	12.3	18.5
176	19.1	15.4	23.2

