

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018826.D
 Acq On : 14 Dec 2023 03:08
 Operator : MA/JU
 Sample : 05677-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AD6

Quant Time: Dec 14 03:36:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 13 23:34:47 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.834	152	242253	20.000	ng/u1	0.00
20) Naphthalene-d8	10.628	136	880690	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.463	164	520662	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.210	188	1190320	20.000	ng/u1	0.00
79) Chrysene-d12	21.298	240	1302985	20.000	ng/u1	0.00
88) Perylene-d12	23.657	264	1565487	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	32993	4.641	ng/uL	0.00
4) Pyridine-d5	3.681	84	220109	11.559	ng/u1	0.00
7) Phenol-d5	7.005	99	141213	5.809	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.169	67	379945	26.369	ng/u1	0.00
11) 2-Chlorophenol-d4	7.363	132	400159	21.095	ng/u1	0.00
15) 4-Methylphenol-d8	8.546	113	243941	12.399	ng/u1	0.00
21) Nitrobenzene-d5	8.993	128	231749	29.566	ng/u1	0.00
24) 2-Nitrophenol-d4	9.716	143	230581	28.374	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.251	165	436445	26.265	ng/u1	0.00
31) 4-Chloroaniline-d4	10.769	131	561552	25.858	ng/u1	0.00
46) Dimethylphthalate-d6	13.881	166	1466928	31.568	ng/u1	0.00
49) Acenaphthylene-d8	14.157	160	1595360	31.178	ng/u1	0.00
54) 4-Nitrophenol-d4	14.669	143	41345	5.420	ng/u1	0.00
60) Fluorene-d10	15.457	176	1301624	33.369	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.575	200	177708	24.899	ng/u1	0.00
73) Anthracene-d10	17.310	188	2192496	35.037	ng/u1	0.00
81) Pyrene-d10	19.545	212	2832093	27.923	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.504	264	3225155	35.333	ng/u1	-0.01
Target Compounds						
2) 1,4-Dioxane	3.299	88	11381	1.460	ng/uL	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018826.D
Acq On : 14 Dec 2023 03:08
Operator : MA/JU
Sample : 05677-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AD6

Quant Time: Dec 14 03:36:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 13 23:34:47 2023
Response via : Initial Calibration

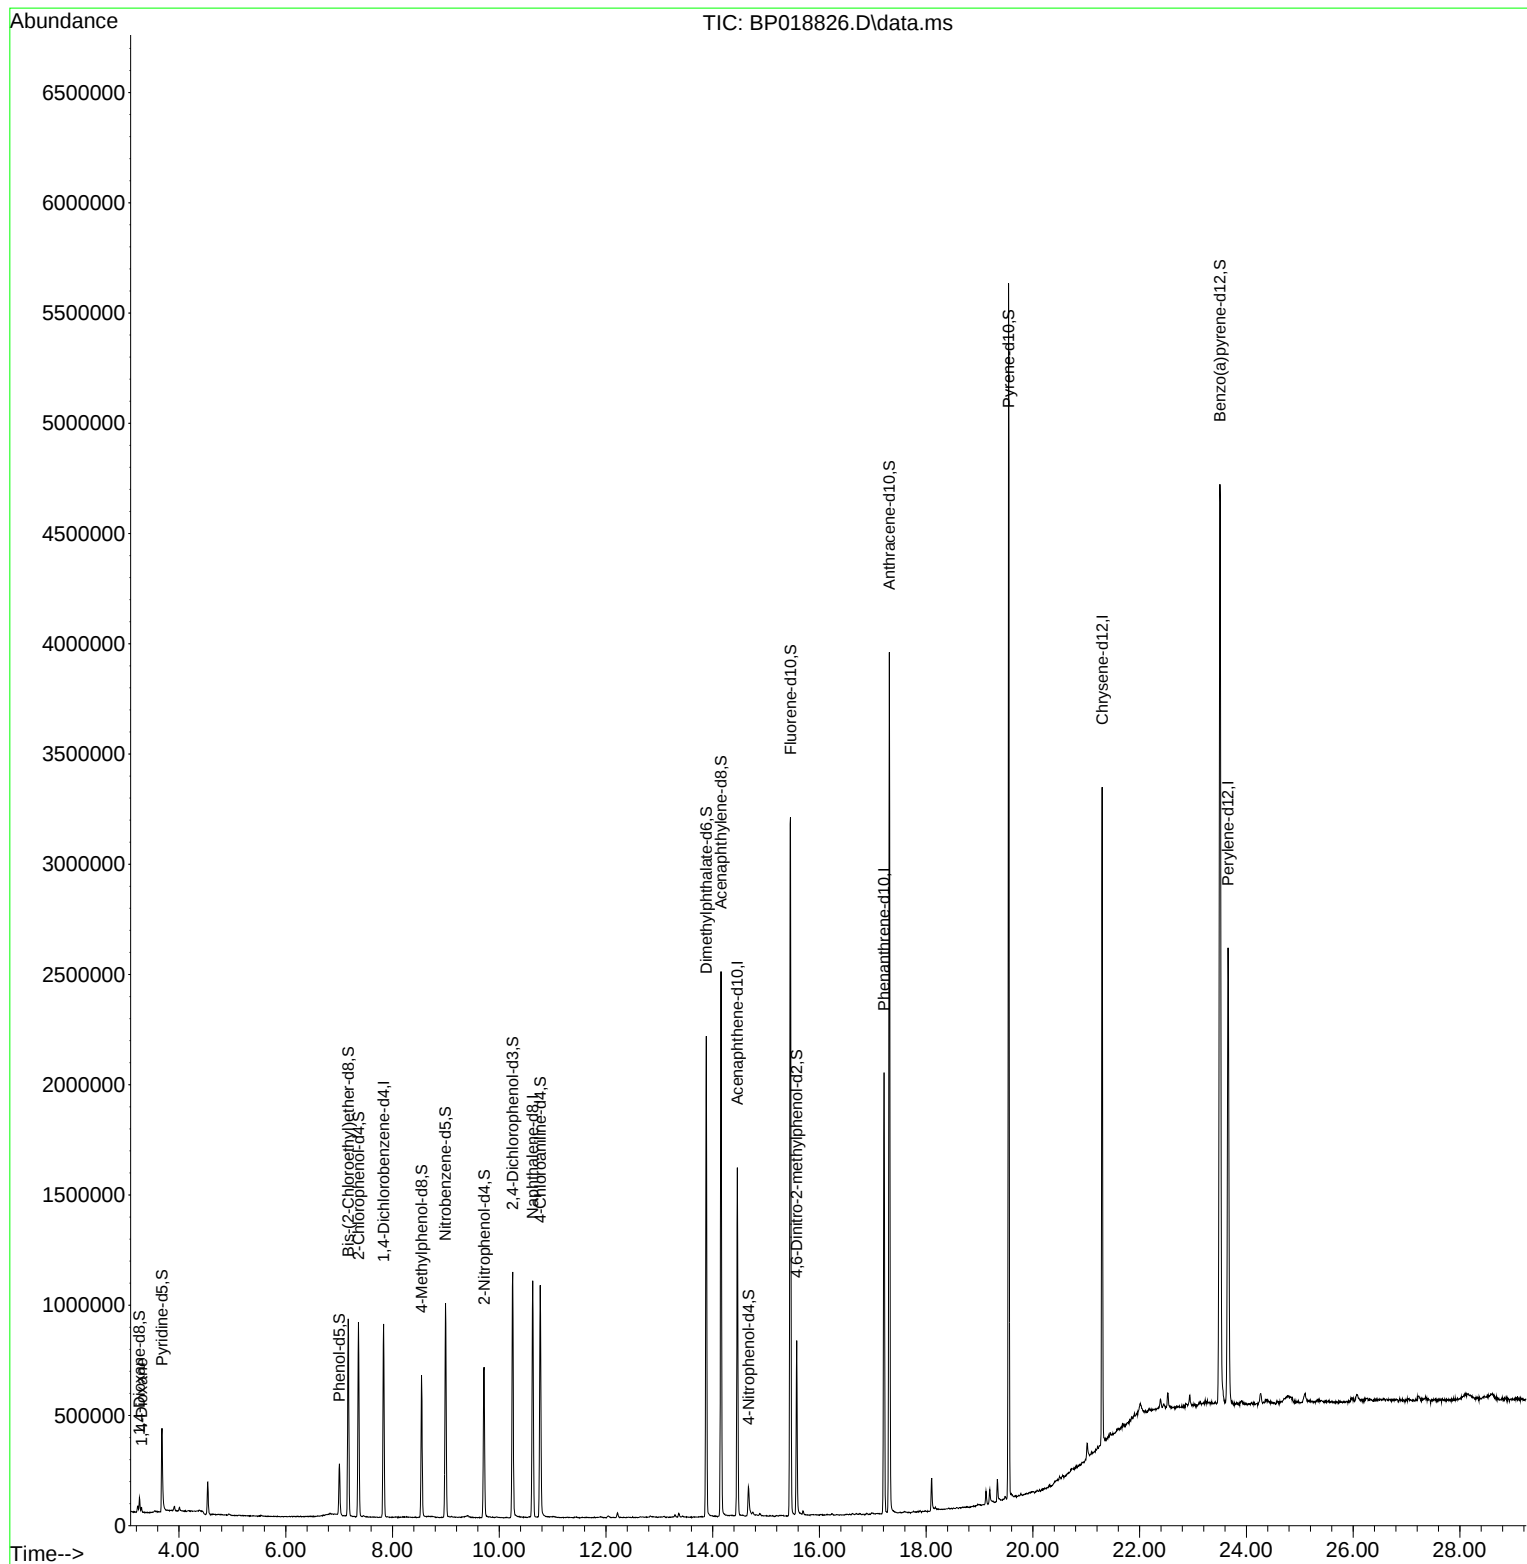

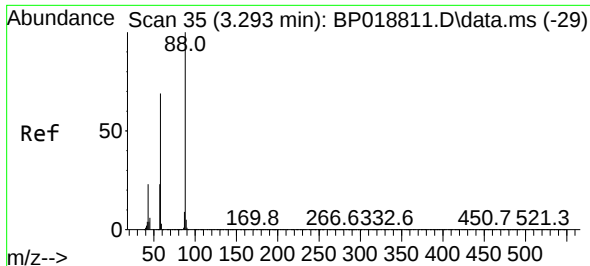

#2
1,4-Dioxane
Concen: 1.460 ng/uL
RT: 3.299 min Scan# 30
Delta R.T. 0.006 min
Lab File: BP018826.D
Acq: 14 Dec 2023 03:08

Instrument :
BNA_P
ClientSampleId :
H0AD6

Tgt Ion: 88 Resp: 11381
Ion Ratio Lower Upper
88 100
43 30.9 21.8 32.6
58 63.0 56.5 84.7

