

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018847.D
 Acq On : 14 Dec 2023 17:35
 Operator : MA/JU
 Sample : 05677-09
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AC9

Quant Time: Dec 14 22:34:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 13 23:34:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.834	152	166986	20.000	ng/u1	0.00
20) Naphthalene-d8	10.628	136	432775	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.463	164	343664	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.210	188	773582	20.000	ng/u1	0.00
79) Chrysene-d12	21.298	240	845688	20.000	ng/u1	0.00
88) Perylene-d12	23.657	264	982186	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	23865	4.870	ng/uL	0.00
4) Pyridine-d5	3.681	84	140056	10.670	ng/u1	0.00
7) Phenol-d5	7.005	99	102748	6.131	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.169	67	300809	30.287	ng/u1	0.00
11) 2-Chlorophenol-d4	7.364	132	305634	23.374	ng/u1	0.00
15) 4-Methylphenol-d8	8.546	113	180837	13.334	ng/u1	0.00
21) Nitrobenzene-d5	8.987	128	148818	38.636	ng/u1	0.00
24) 2-Nitrophenol-d4	9.710	143	127730	31.985	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.246	165	238328	29.186	ng/u1	0.00
31) 4-Chloroaniline-d4	10.769	131	271970	25.485	ng/u1	0.00
46) Dimethylphthalate-d6	13.881	166	1004320	32.744	ng/u1	0.00
49) Acenaphthylene-d8	14.157	160	1124237	33.287	ng/u1	0.00
54) 4-Nitrophenol-d4	14.669	143	24013	4.769	ng/u1	0.00
60) Fluorene-d10	15.451	176	903408	35.089	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.575	200	113705	24.514	ng/u1	0.00
73) Anthracene-d10	17.310	188	1479857	36.388	ng/u1	0.00
81) Pyrene-d10	19.545	212	1930394	29.324	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.504	264	2087534	36.452	ng/u1	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.293	88	9004	1.676	ng/uL	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018847.D
Acq On : 14 Dec 2023 17:35
Operator : MA/JU
Sample : 05677-09
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC9

Quant Time: Dec 14 22:34:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 13 23:34:47 2023
Response via : Initial Calibration

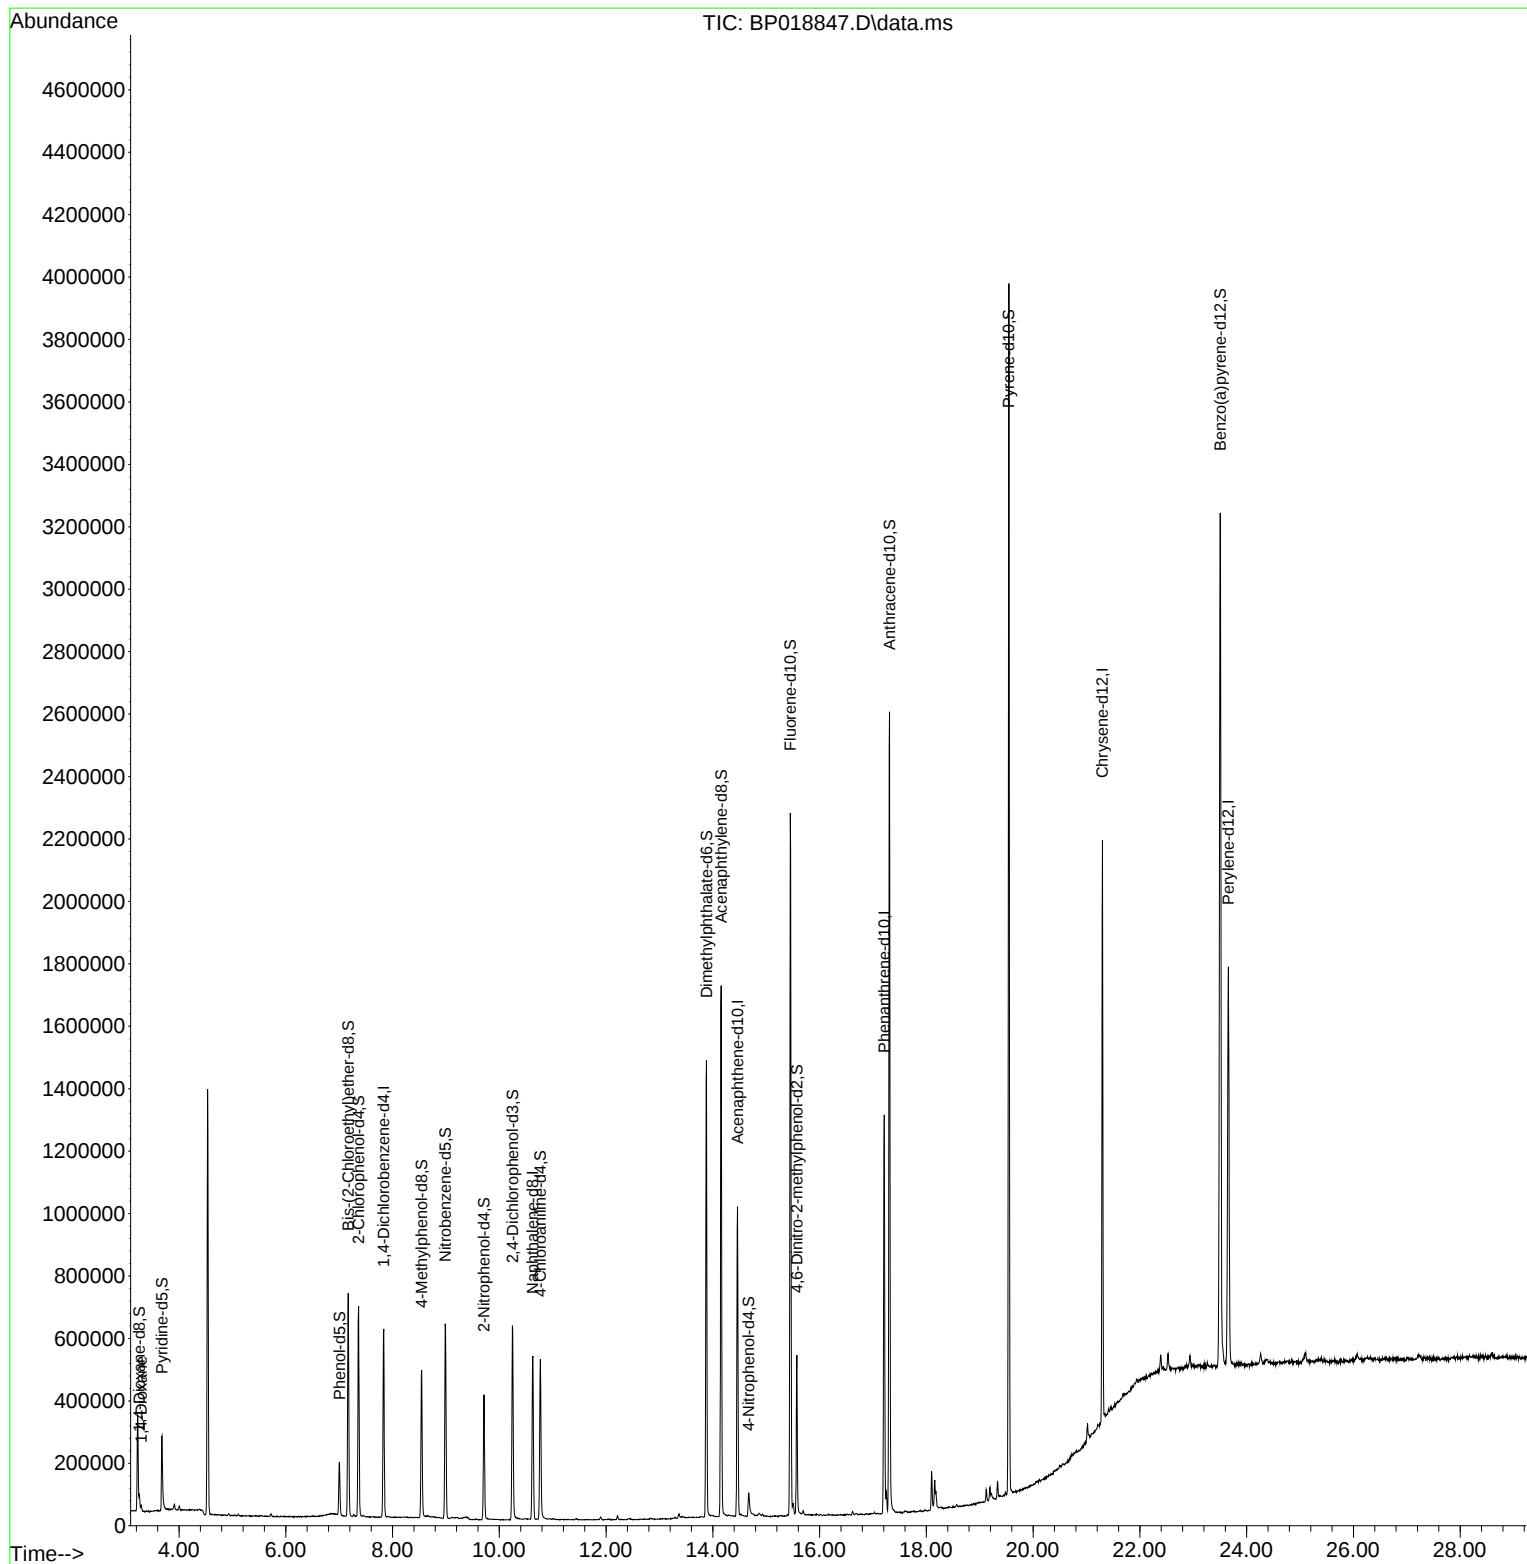

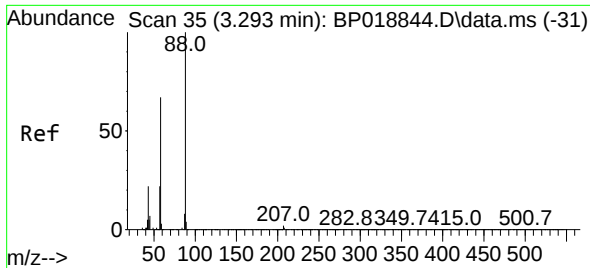

#2
 1,4-Dioxane
 Concen: 1.676 ng/uL
 RT: 3.293 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: BP018847.D
 Acq: 14 Dec 2023 17:35

Instrument :
 BNA_P
 ClientSampleId :
 H0AC9

Tgt Ion:	88	Resp:	9004
Ion	Ratio	Lower	Upper
88	100		
43	25.1	21.8	32.6
58	64.0	56.5	84.7

