

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018855.D
 Acq On : 14 Dec 2023 22:06
 Operator : MA/JU
 Sample : 05627-21DL 5X
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLD3DL

Quant Time: Dec 14 22:47:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 13 23:34:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.828	152	276204	20.000	ng/ul	0.00
20) Naphthalene-d8	10.622	136	988872	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.463	164	533595	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.210	188	1185500	20.000	ng/ul	0.00
79) Chrysene-d12	21.298	240	1373173	20.000	ng/ul	0.00
88) Perylene-d12	23.657	264	1625790	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	8933	1.102	ng/uL	0.00
4) Pyridine-d5	3.687	84	33071	1.523	ng/ul	0.01
7) Phenol-d5	6.999	99	38275	1.381	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.169	67	103378	6.293	ng/ul	0.00
11) 2-Chlorophenol-d4	7.364	132	101627	4.699	ng/ul	0.00
15) 4-Methylphenol-d8	8.546	113	50135	2.235	ng/ul	0.00
21) Nitrobenzene-d5	8.993	128	51812	5.887	ng/ul	0.00
24) 2-Nitrophenol-d4	9.710	143	46504	5.096	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.246	165	96915	5.194	ng/ul	0.00
31) 4-Chloroaniline-d4	10.769	131	125516	5.147	ng/ul	0.00
46) Dimethylphthalate-d6	13.875	166	334366	7.021	ng/ul	0.00
49) Acenaphthylene-d8	14.151	160	343138	6.543	ng/ul	0.00
54) 4-Nitrophenol-d4	14.681	143	7632	0.976	ng/ul	0.01
60) Fluorene-d10	15.451	176	265739	6.648	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.569	200	25784	3.627	ng/ul	-0.01
73) Anthracene-d10	17.304	188	497651	7.985	ng/ul	0.00
81) Pyrene-d10	19.545	212	725476	6.787	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.498	264	784619	8.277	ng/ul	-0.02
Target Compounds						
78) Di-n-butylphthalate	18.175	149	1695074	22.256	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018855.D
Acq On : 14 Dec 2023 22:06
Operator : MA/JU
Sample : 05627-21DL 5X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLD3DL

Quant Time: Dec 14 22:47:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 13 23:34:47 2023
Response via : Initial Calibration

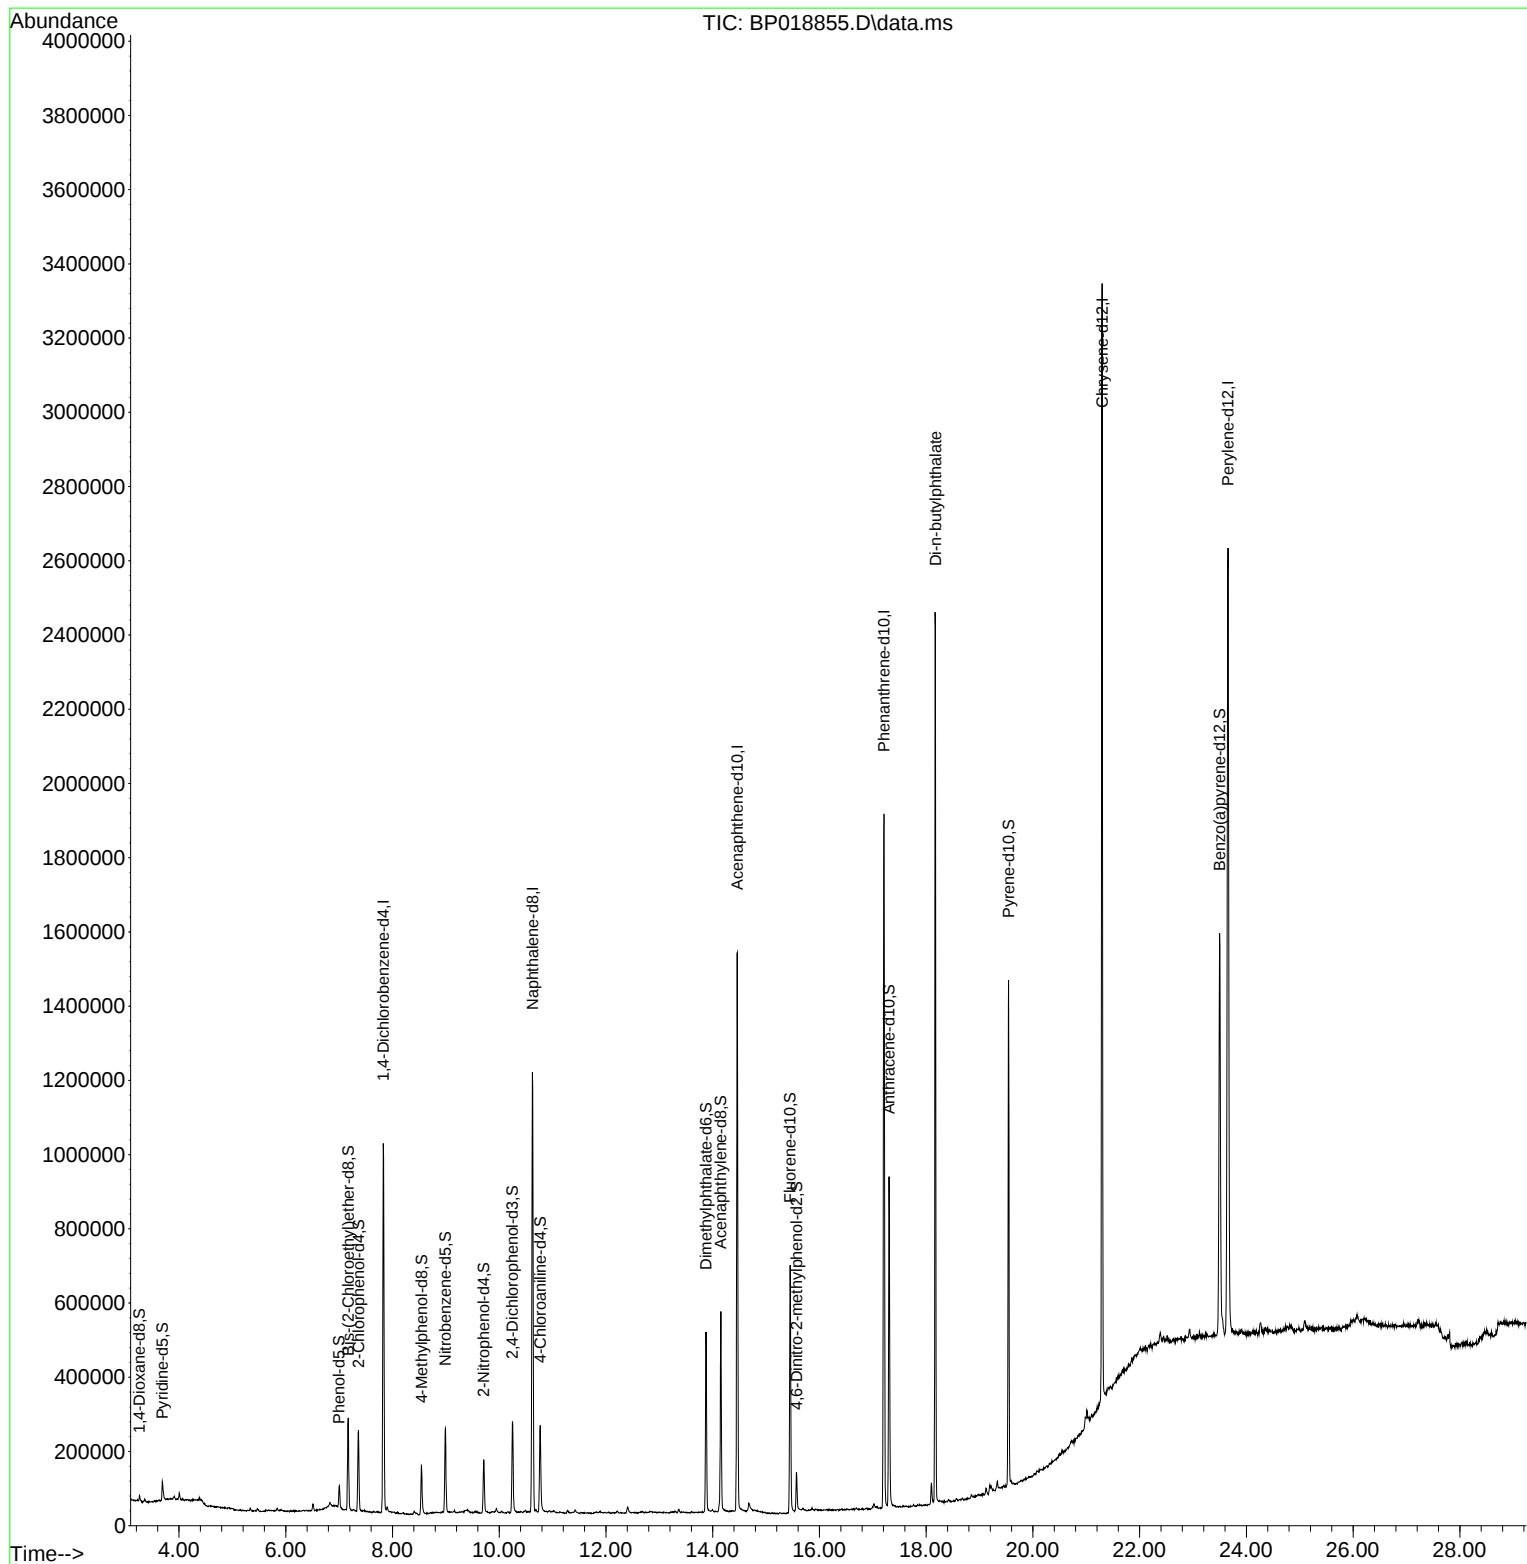

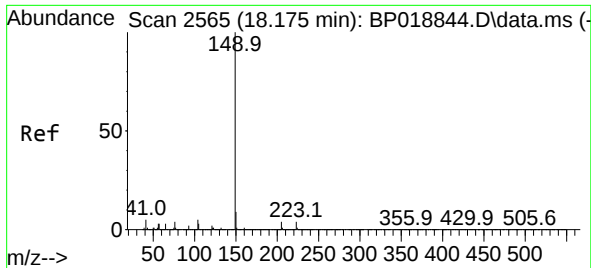

#78
 Di-n-butylphthalate
 Concen: 22.256 ng/ul
 RT: 18.175 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP018855.D
 Acq: 14 Dec 2023 22:06

Instrument :
 BNA_P
 ClientSampleId :
 DCLD3DL

Tgt Ion:149 Resp: 1695074

Ion	Ratio	Lower	Upper
149	100		
150	9.0	7.4	11.2
104	4.9	3.9	5.9

